

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022624\
 Data File : VD078546.D
 Acq On : 26 Feb 2024 10:38
 Operator : RP/MD
 Sample : VD0226SBL01
 Misc : 5.00G/5ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0226SBL01

Quant Time: Feb 27 03:23:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021324S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 14 01:16:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	149468	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	277741	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	327127	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	165133	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	52735	32.631	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	65.260%
35) Dibromofluoromethane	7.810	113	79380	44.993	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	89.980%
50) Toluene-d8	10.269	98	347037	49.173	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	98.340%
62) 4-Bromofluorobenzene	12.575	95	132462	64.497	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	129.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022624\
Data File : VD078546.D
Acq On : 26 Feb 2024 10:38
Operator : RP/MD
Sample : VD0226SBL01
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0226SBL01

Quant Time: Feb 27 03:23:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021324S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 14 01:16:20 2024
Response via : Initial Calibration




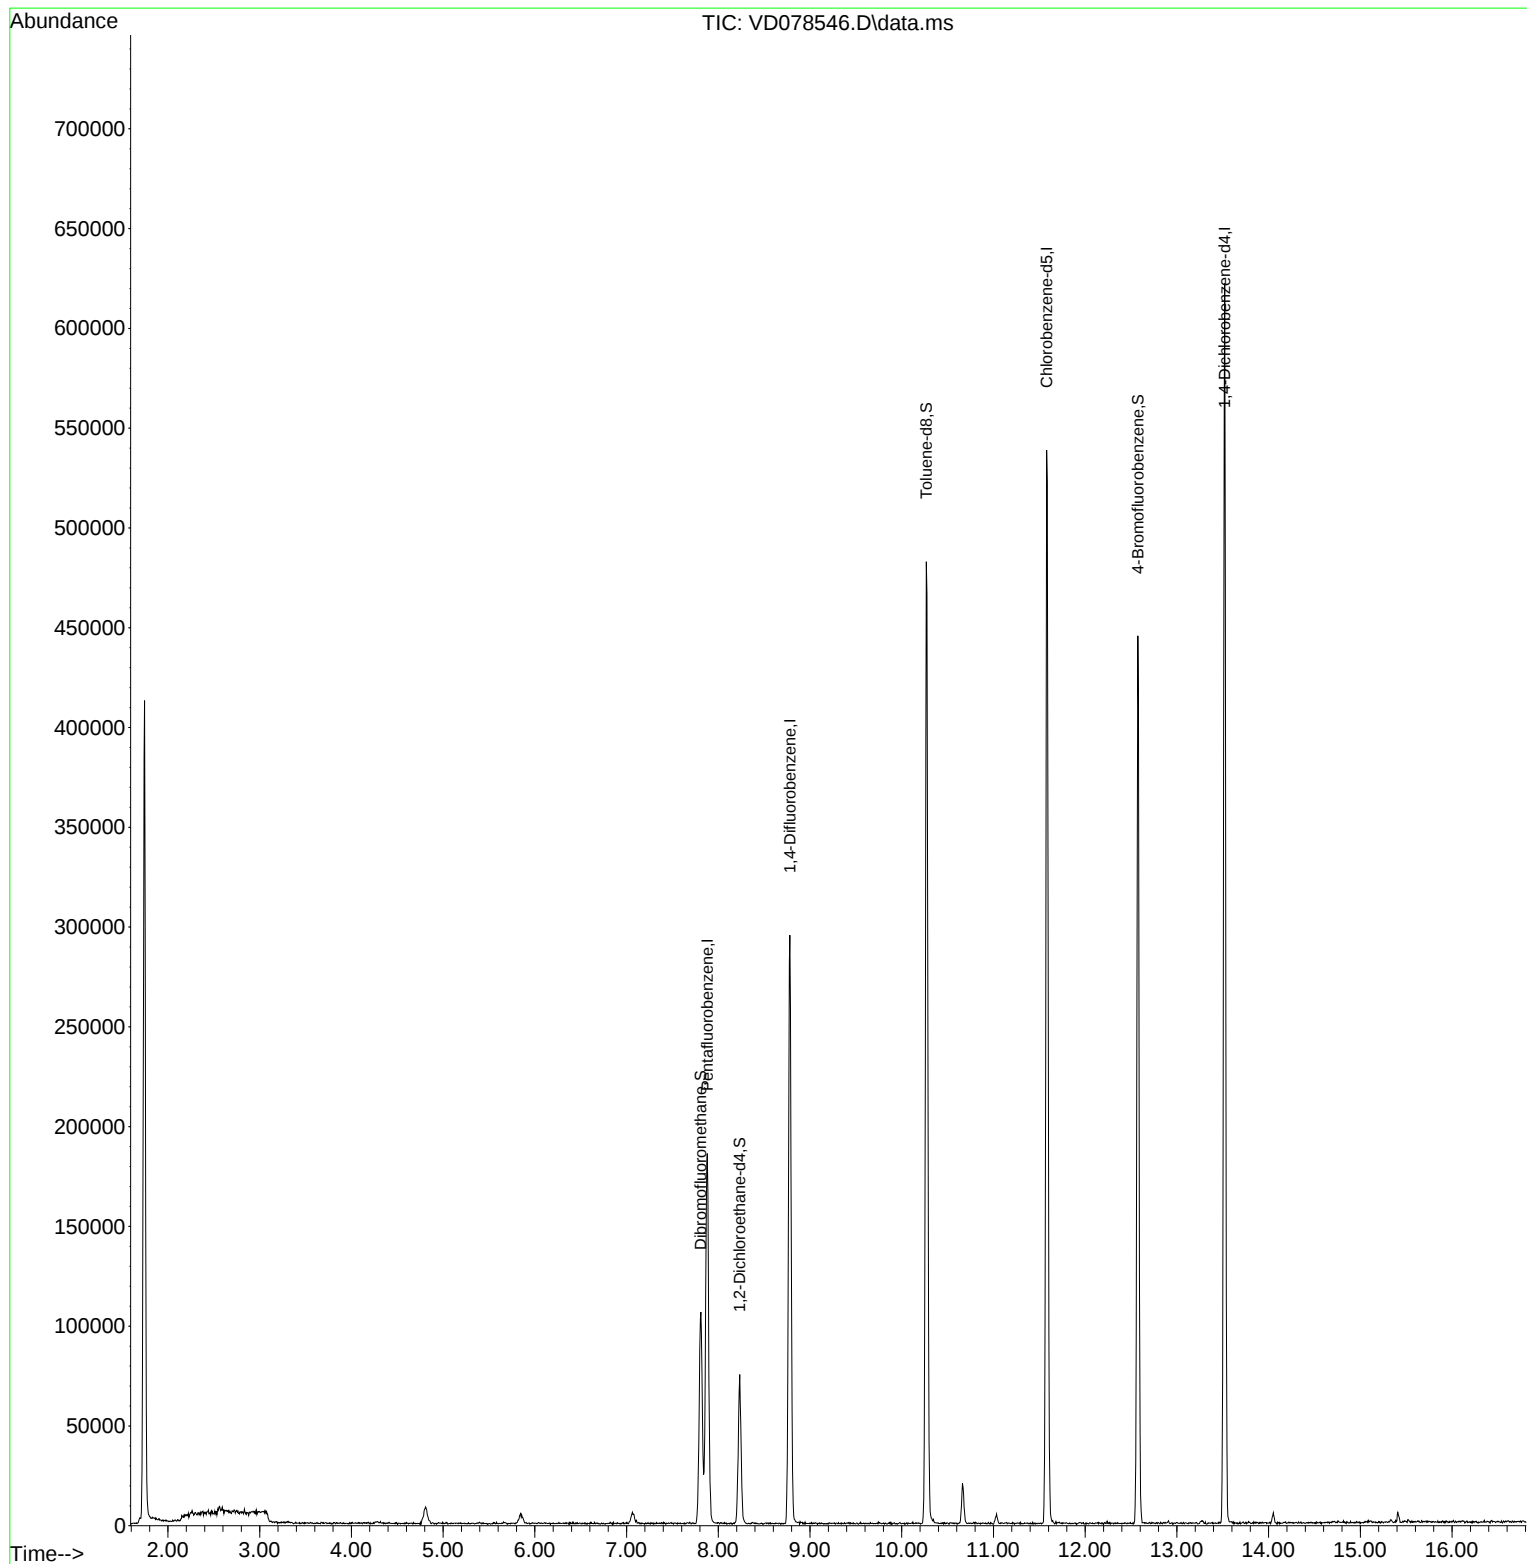


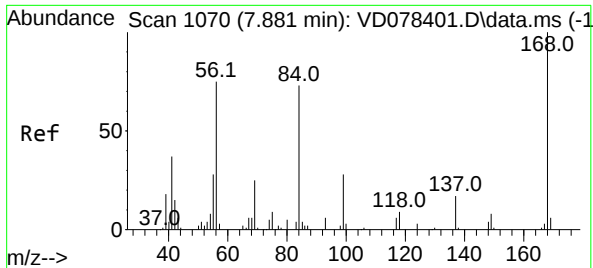

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1070
Delta R.T. -0.000 min
Lab File: VD078546.D
Acq: 26 Feb 2024 10:38




Instrument :
MSVOA_D
ClientSampleId :
VD0226SBL01


Tgt Ion:168 Resp: 149468
Ion Ratio Lower Upper
168 100
99 50.4 36.7 55.1

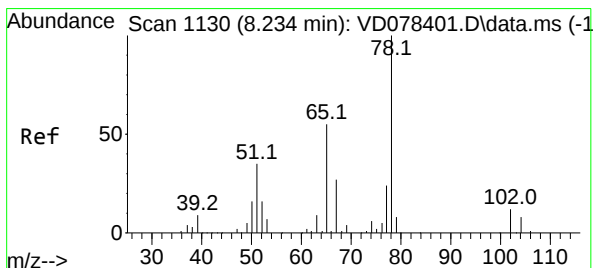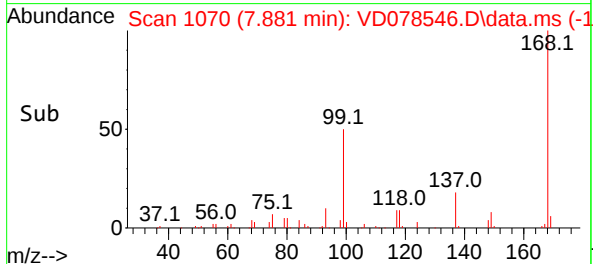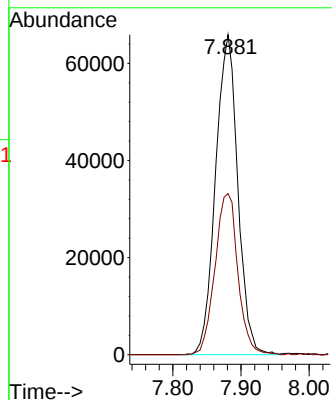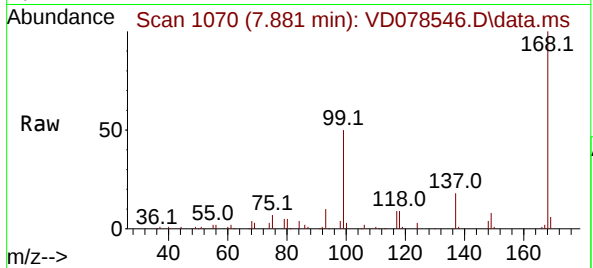

#33
1,2-Dichloroethane-d4
Concen: 32.631 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VD078546.D
Acq: 26 Feb 2024 10:38

Tgt Ion: 65 Resp: 52735
Ion Ratio Lower Upper
65 100
67 57.0 0.0 115.0

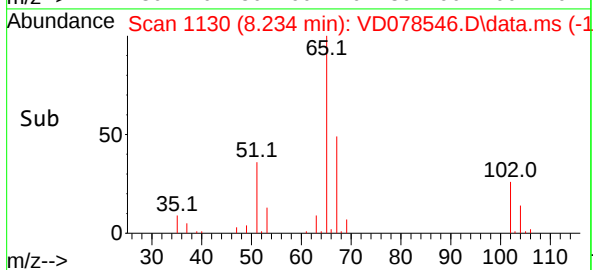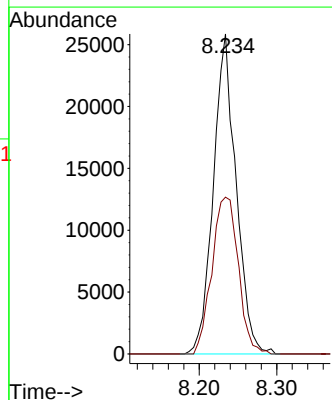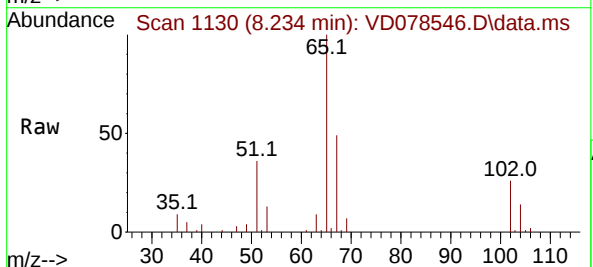

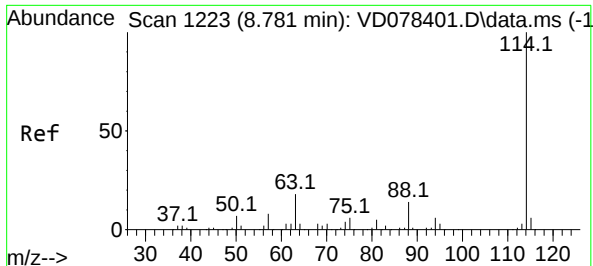

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. -0.000 min

Lab File: VD078546.D

Acq: 26 Feb 2024 10:38

Instrument :

MSVOA_D

ClientSampleId :

VD0226SBL01





Tgt Ion:114 Resp: 277741

Ion Ratio Lower Upper

114 100

63 16.9 0.0 33.4

88 13.5 0.0 26.2

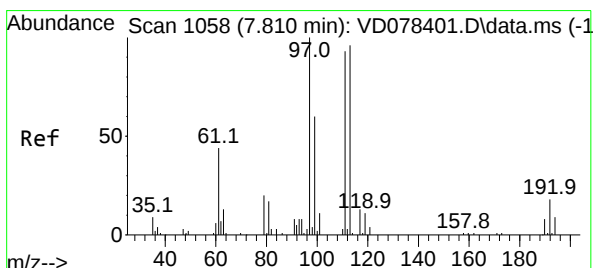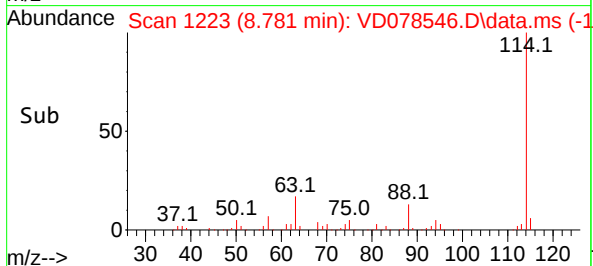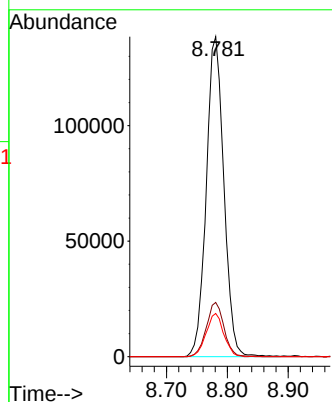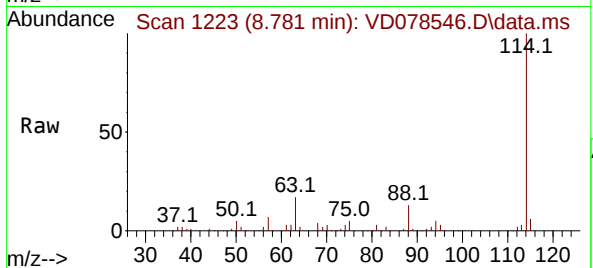

#35

Dibromofluoromethane

Concen: 44.993 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. -0.000 min

Lab File: VD078546.D

Acq: 26 Feb 2024 10:38




Tgt Ion:113 Resp: 79380


Ion Ratio Lower Upper

113 100

111 101.3 84.7 127.1

192 19.0 16.8 25.2


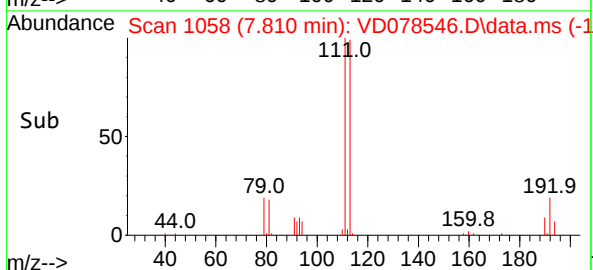
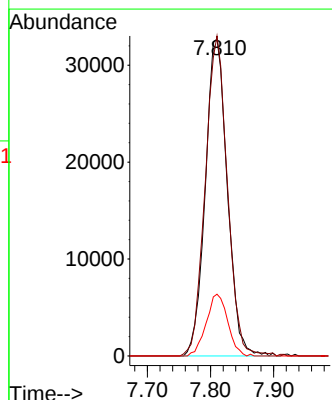
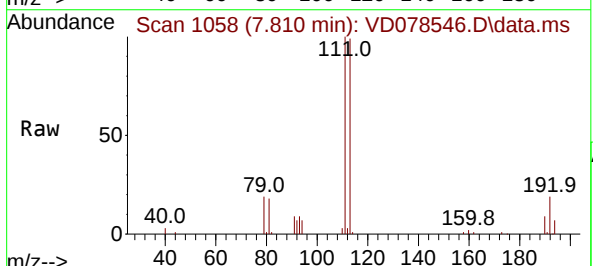


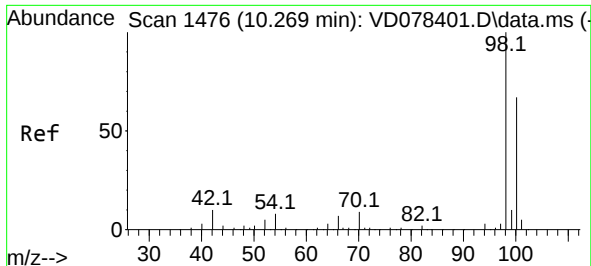

#50
Toluene-d8
Concen: 49.173 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD078546.D
Acq: 26 Feb 2024 10:38




Instrument :
MSVOA_D
ClientSampleId :
VD0226SBL01


Tgt Ion: 98 Resp: 347037
Ion Ratio Lower Upper
98 100
100 64.8 50.3 75.5

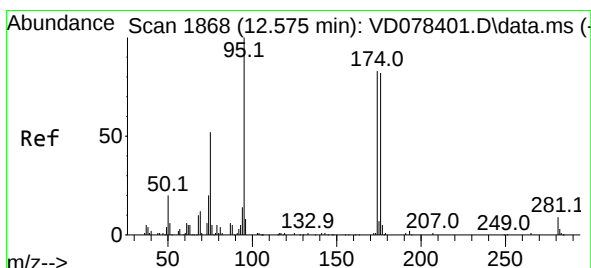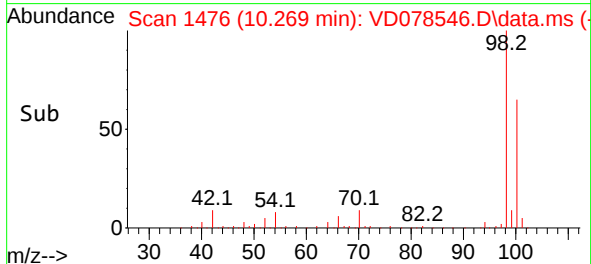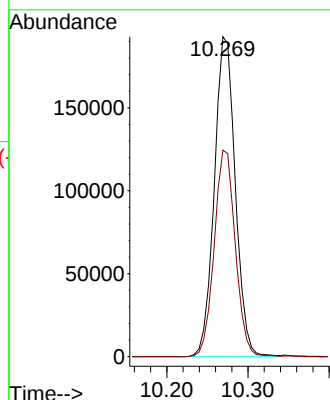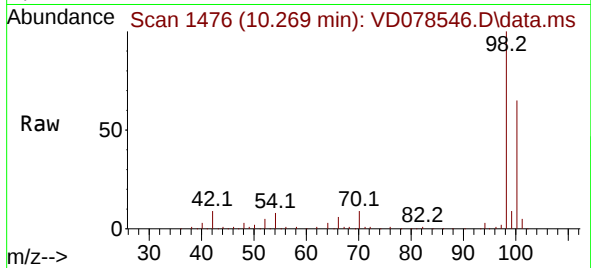

#62
4-Bromofluorobenzene
Concen: 64.497 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD078546.D
Acq: 26 Feb 2024 10:38

Tgt Ion: 95 Resp: 132462
Ion Ratio Lower Upper
95 100
174 93.8 0.0 201.8
176 90.1 0.0 191.8


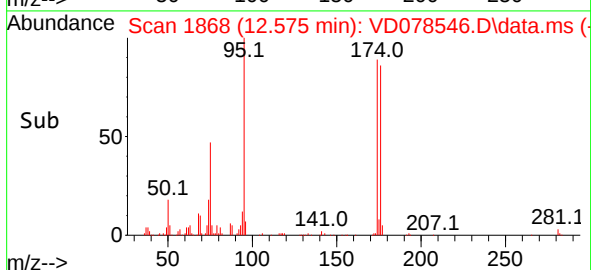
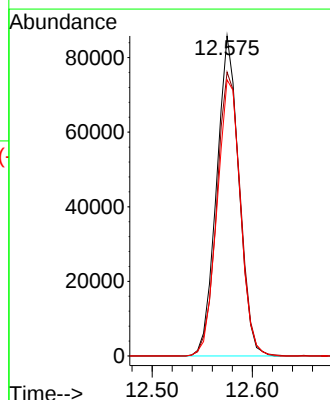
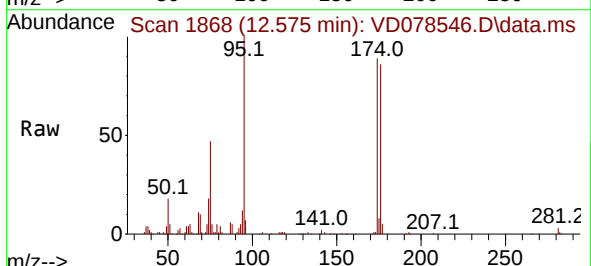


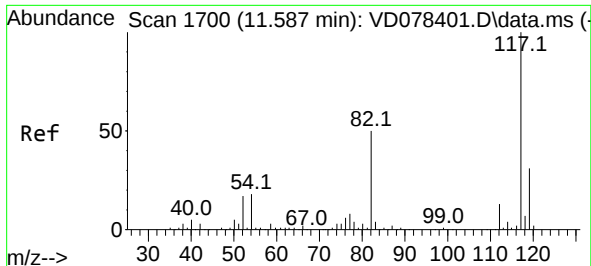

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1
Delta R.T. -0.006 min
Lab File: VD078546.D
Acq: 26 Feb 2024 10:38

Instrument :
MSVOA_D
ClientSampleId :
VD0226SBL01

Tgt Ion:117 Resp: 327127
Ion Ratio Lower Upper
117 100
82 50.0 38.3 57.5
119 32.8 25.0 37.4

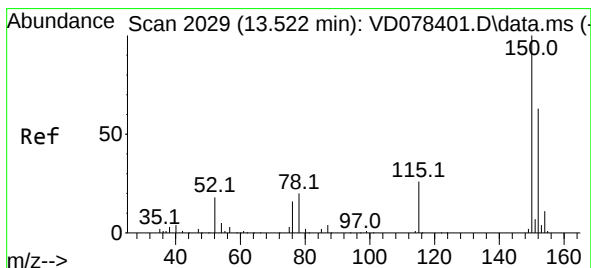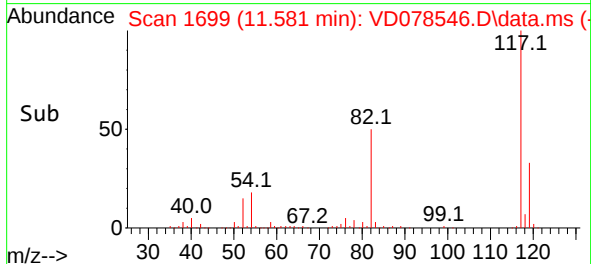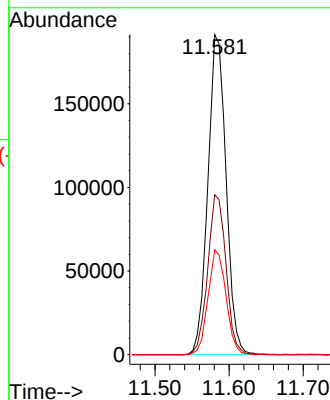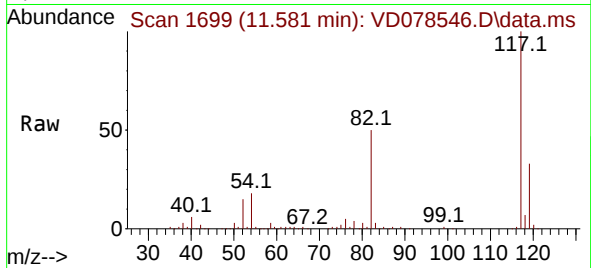

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. -0.000 min
Lab File: VD078546.D
Acq: 26 Feb 2024 10:38

Tgt Ion:152 Resp: 165133
Ion Ratio Lower Upper
152 100
115 57.2 27.1 81.3
150 158.9 0.0 353.6

