


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD022720\
Data File : VD065337.D
Acq On : 27 Feb 2020 09:34
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D021820S.M
Title : SW846 8260
Last Update : Wed Feb 19 03:26:54 2020

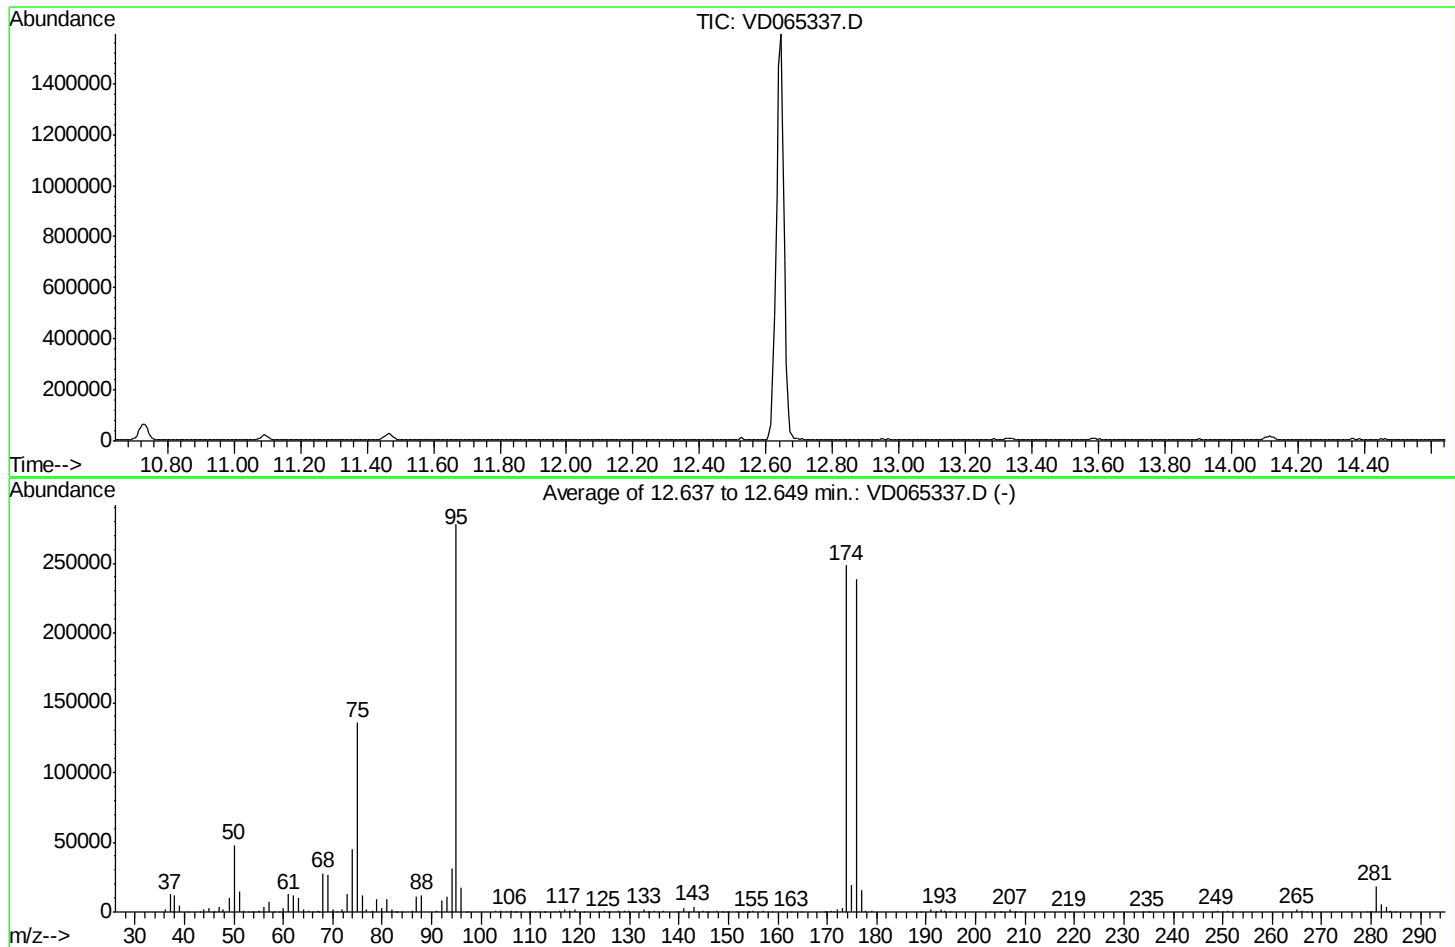

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	47901	PASS
75	95	30	60	48.8	135658	PASS
95	95	100	100	100.0	277866	PASS
96	95	5	9	6.3	17412	PASS
173	174	0.00	2	1.3	3141	PASS
174	95	50	100	89.4	248426	PASS
175	174	5	9	7.6	18909	PASS
176	174	95	101	96.2	238954	PASS
177	176	5	9	6.6	15792	PASS