


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD022820\  
Data File : VD065350.D  
Acq On : 28 Feb 2020 09:21  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D021820S.M  
Title : SW846 8260  
Last Update : Wed Feb 19 03:26:54 2020

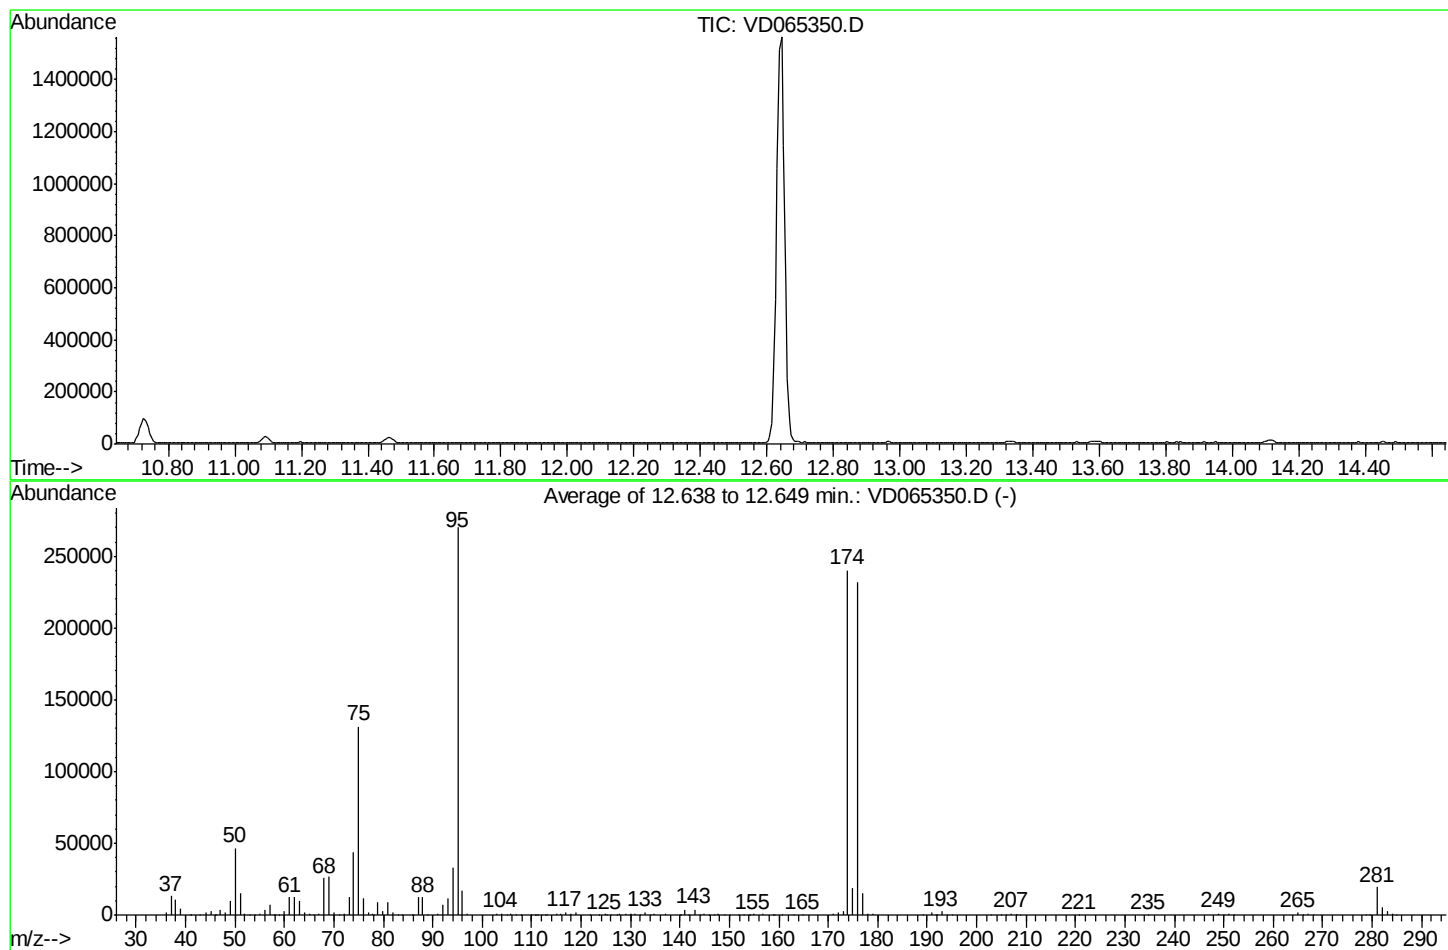

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1813

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.3      | 46720   | PASS             |
| 75          | 95           | 30           | 60           | 48.6      | 131421  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 270229  | PASS             |
| 96          | 95           | 5            | 9            | 6.3       | 17040   | PASS             |
| 173         | 174          | 0.00         | 2            | 1.3       | 3078    | PASS             |
| 174         | 95           | 50           | 100          | 89.0      | 240448  | PASS             |
| 175         | 174          | 5            | 9            | 7.6       | 18338   | PASS             |
| 176         | 174          | 95           | 101          | 96.4      | 231808  | PASS             |
| 177         | 176          | 5            | 9            | 6.7       | 15625   | PASS             |