

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022822\
 Data File : VD072120.D
 Acq On : 28 Feb 2022 14:03
 Operator : VA/SY
 Sample : N1655-07RE
 Misc : 6.89G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 REMOTE-1RE

Quant Time: Mar 01 08:12:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021822S.M
 Quant Title : SW846 8260
 QLast Update : Sat Feb 19 04:05:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	45651	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	74463	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	78875	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	38059	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	34414	72.675	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	145.340%
35) Dibromofluoromethane	7.914	113	28695	63.604	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	127.200%
50) Toluene-d8	10.332	98	88821	53.089	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	106.180%
62) 4-Bromofluorobenzene	12.626	95	34851	56.709	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	113.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022822\
Data File : VD072120.D
Acq On : 28 Feb 2022 14:03
Operator : VA/SY
Sample : N1655-07RE
Misc : 6.89G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
REMOTE-1RE

Quant Time: Mar 01 08:12:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021822S.M
Quant Title : SW846 8260
QLast Update : Sat Feb 19 04:05:38 2022
Response via : Initial Calibration

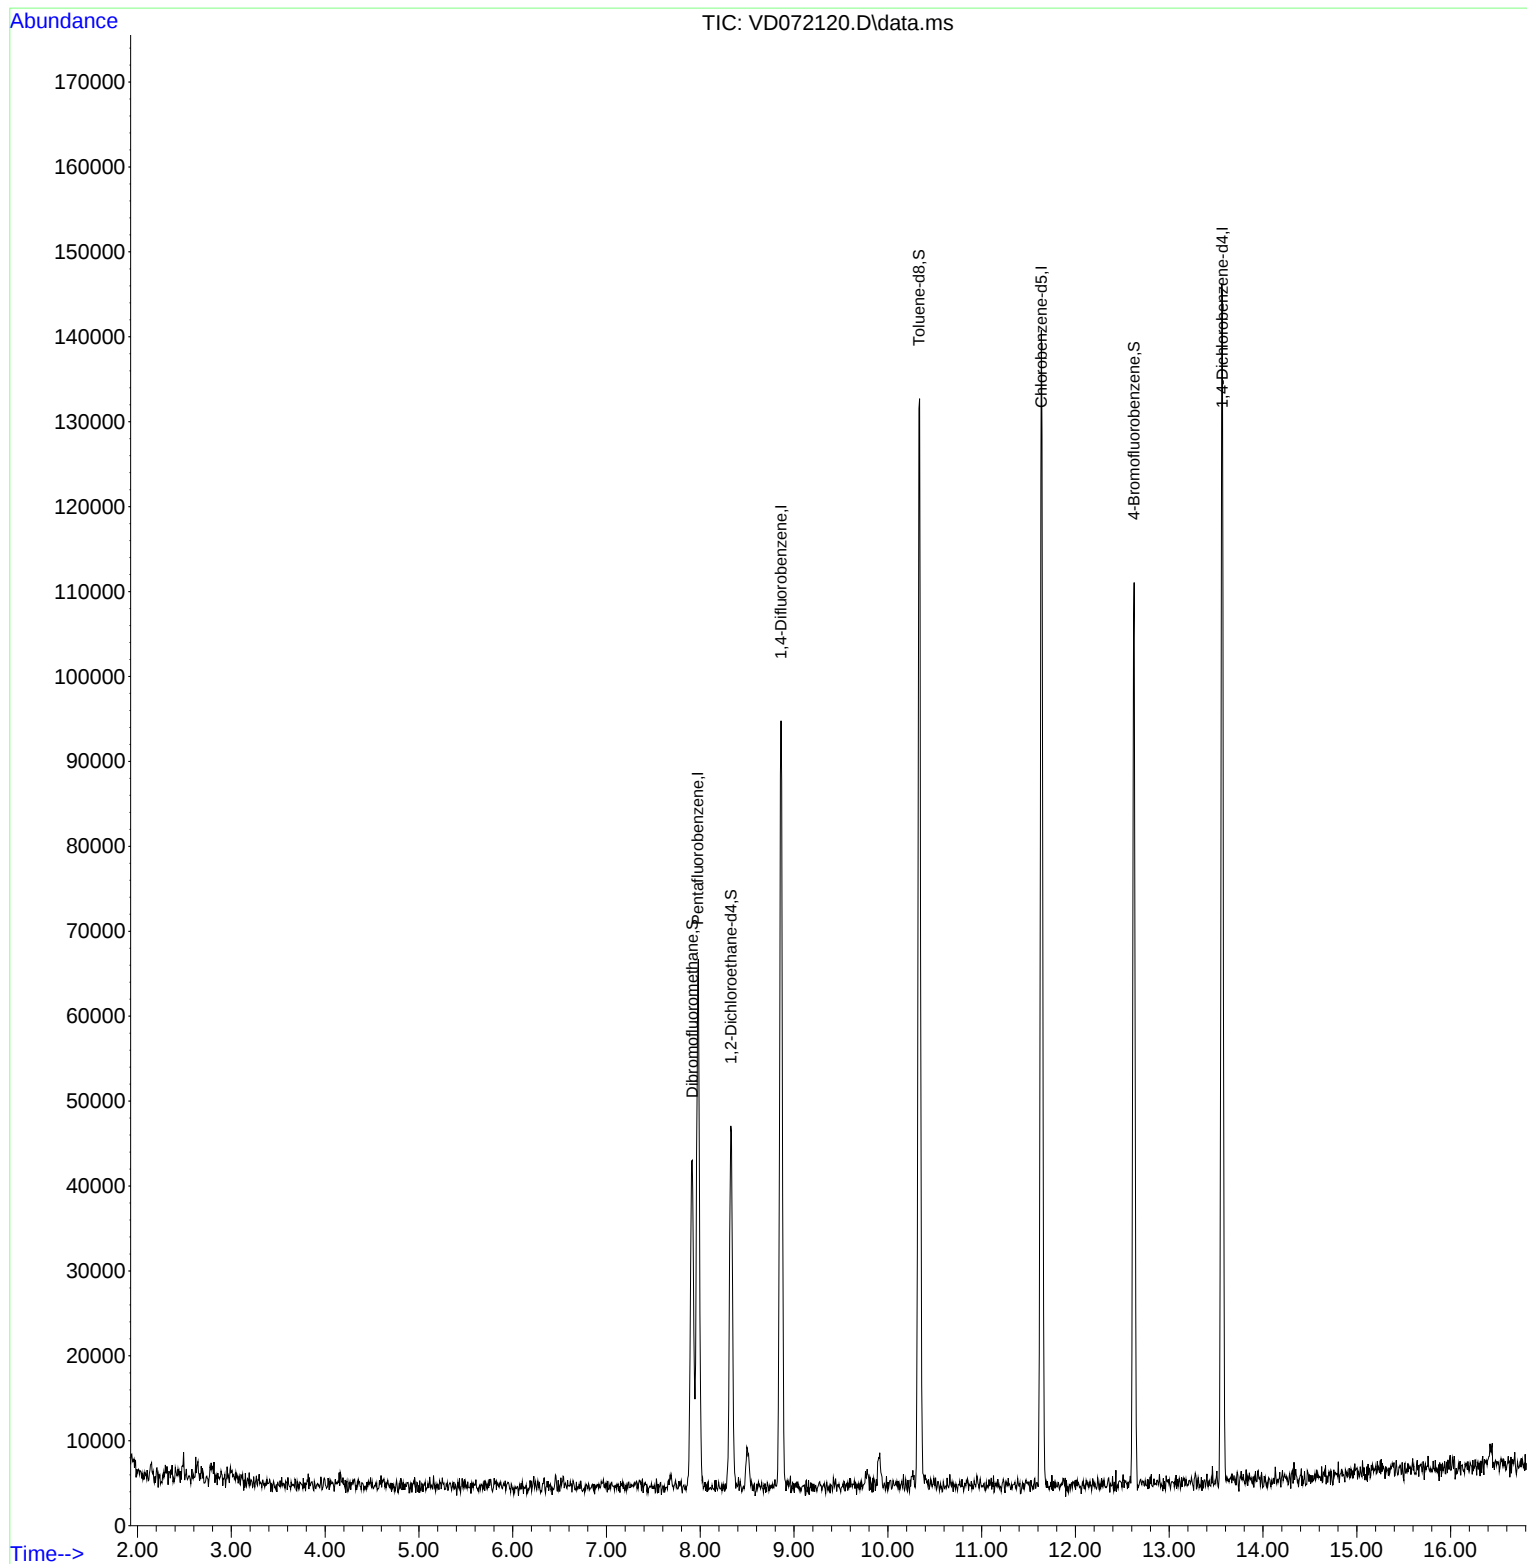

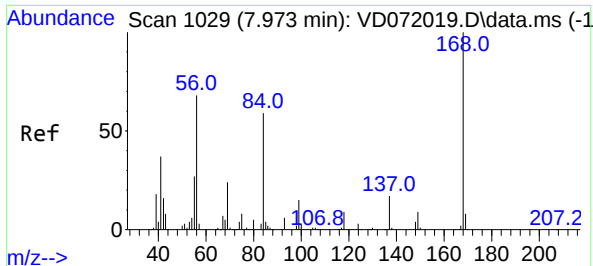

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.973 min Scan# 1029

Delta R.T. 0.000 min

Lab File: VD072120.D

Acq: 28 Feb 2022 14:03

Instrument :

MSVOA_D

ClientSampleId :





REMOTE-1RE

Tgt Ion:168 Resp: 45651

Ion Ratio Lower Upper

168 100

99 60.5 47.1 70.7

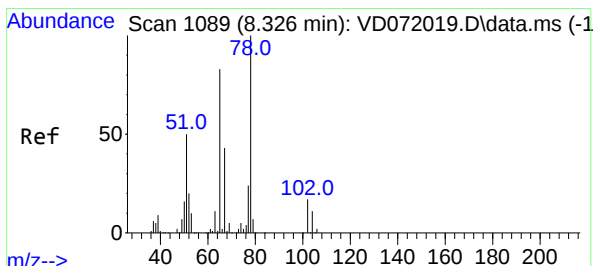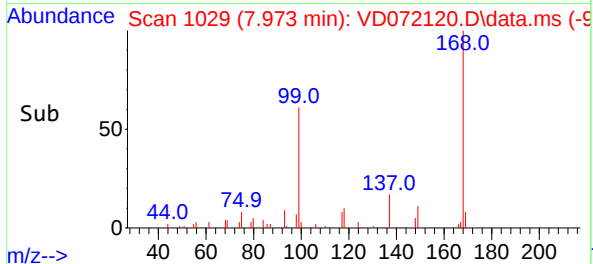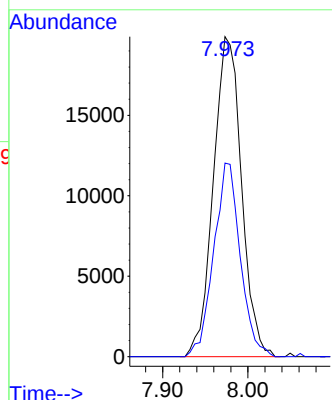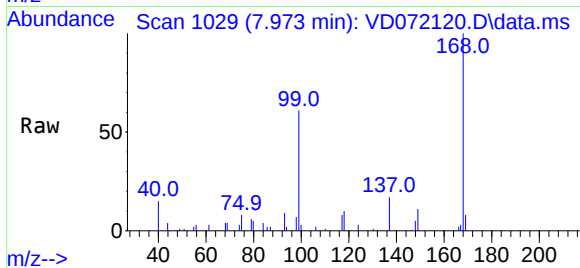

1,2-Dichloroethane-d4

Concen: 72.675 ug/l

RT: 8.326 min Scan# 1089

Delta R.T. 0.000 min

Lab File: VD072120.D




Acq: 28 Feb 2022 14:03


Tgt Ion: 65 Resp: 34414

Ion Ratio Lower Upper

65 100

67 53.9 0.0 105.6

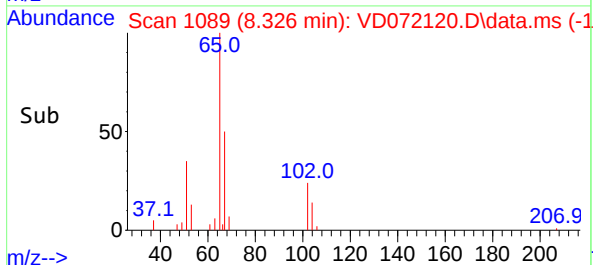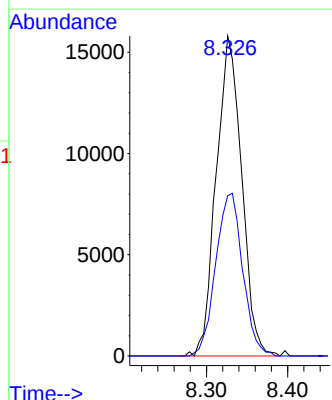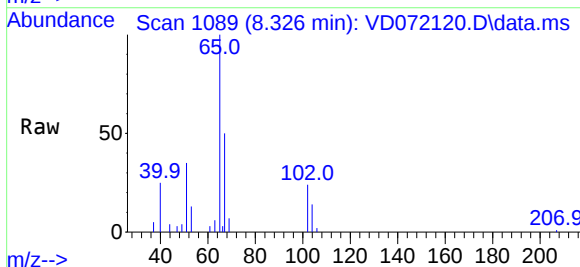




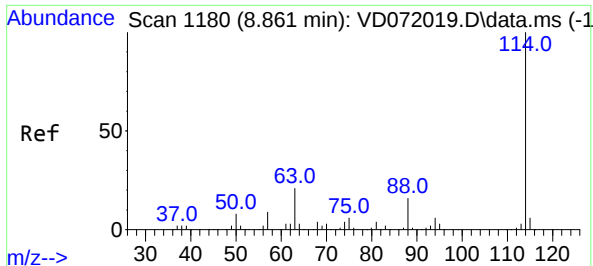


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD072120.D
Acq: 28 Feb 2022 14:03

Instrument :
MSVOA_D
ClientSampleId :
REMOTE-1RE

Tgt Ion:114 Resp: 74463




Ion	Ratio	Lower	Upper
114	100		
63	20.6	0.0	42.2
88	19.2	0.0	31.2

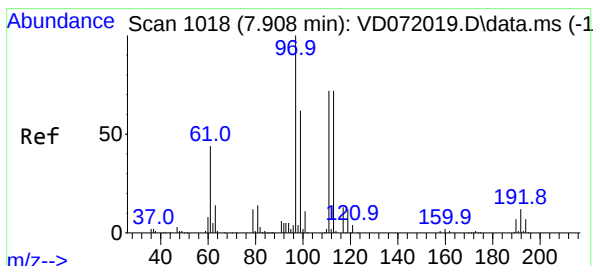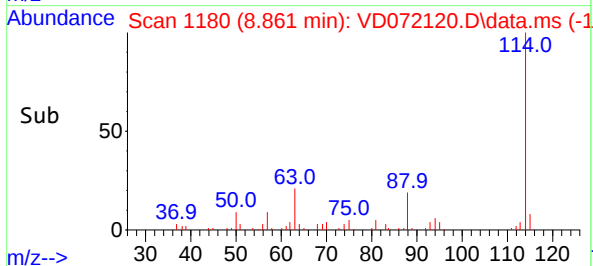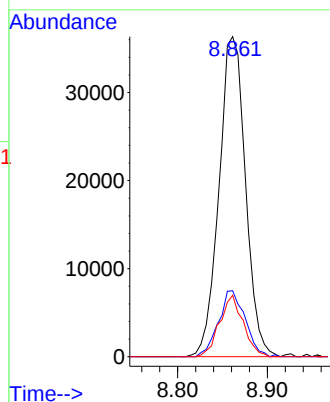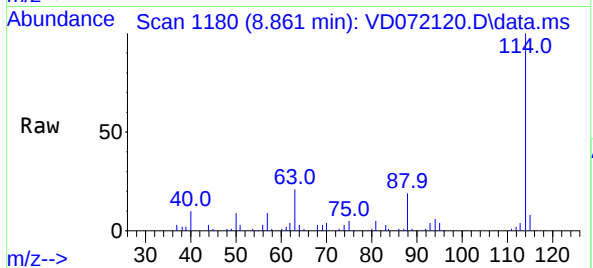


#35
Dibromofluoromethane
Concen: 63.604 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. 0.006 min
Lab File: VD072120.D
Acq: 28 Feb 2022 14:03

Tgt Ion:113 Resp: 28695

Ion	Ratio	Lower	Upper
113	100		
111	103.0	83.0	124.4
192	21.8	15.3	22.9


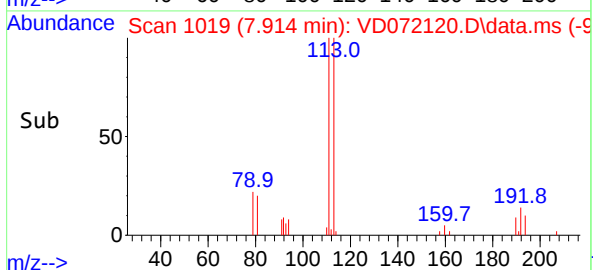
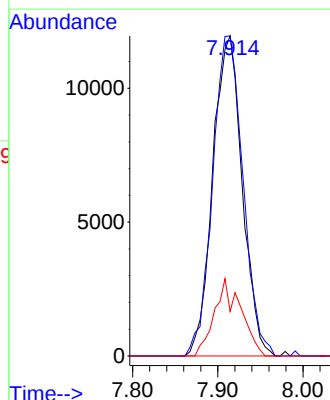
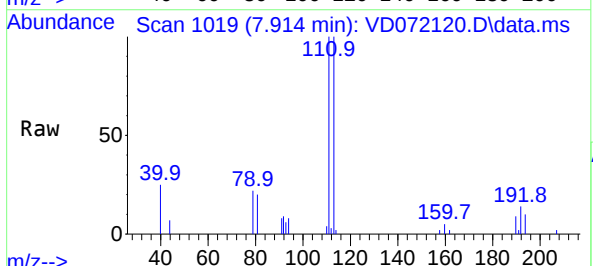


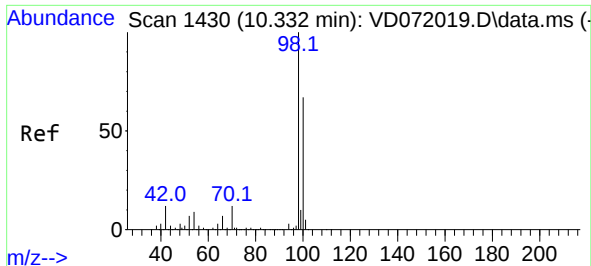

#50
Toluene-d8
Concen: 53.089 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. 0.000 min
Lab File: VD072120.D
Acq: 28 Feb 2022 14:03




Instrument :
MSVOA_D
ClientSampleId :
REMOTE-1RE


Tgt Ion: 98 Resp: 88821
Ion Ratio Lower Upper
98 100
100 66.0 53.8 80.6

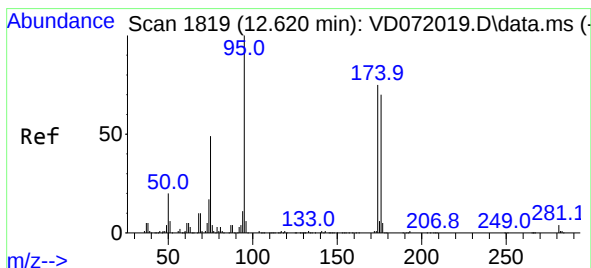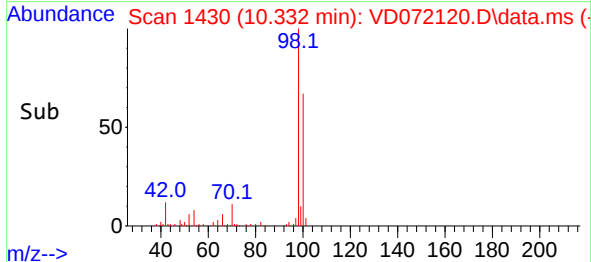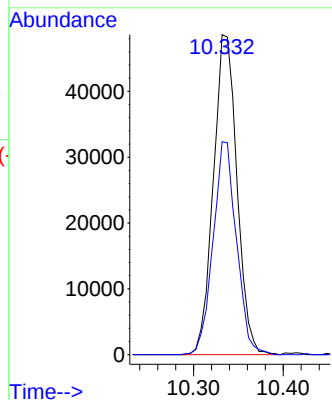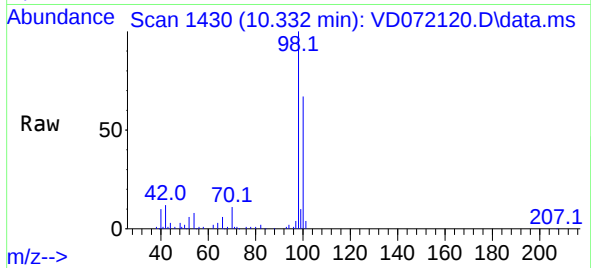

#62
4-Bromofluorobenzene
Concen: 56.709 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. 0.006 min
Lab File: VD072120.D
Acq: 28 Feb 2022 14:03

Tgt Ion: 95 Resp: 34851
Ion Ratio Lower Upper
95 100
174 82.1 0.0 155.0
176 76.4 0.0 148.8


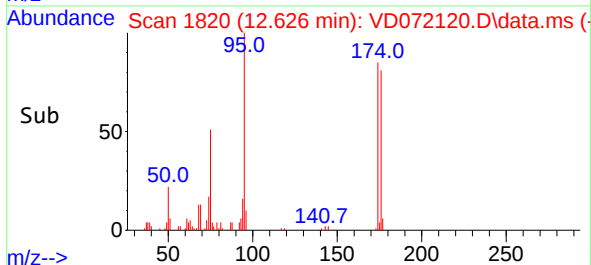
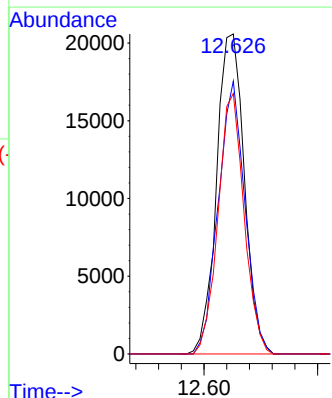
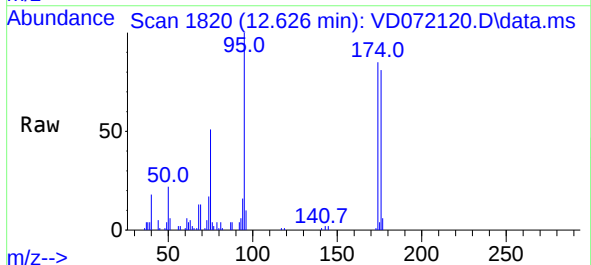


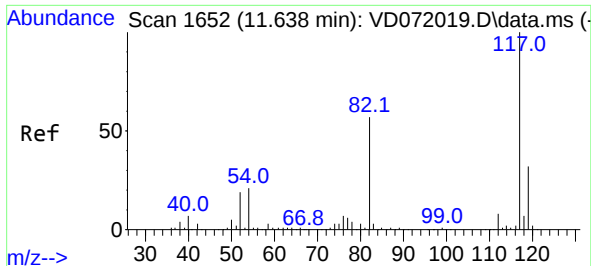

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 117
Delta R.T. 0.000 min
Lab File: VD072120.D
Acq: 28 Feb 2022 14:03

Instrument :
MSVOA_D
ClientSampleId :
REMOTE-1RE

Tgt Ion:117 Resp: 78875
Ion Ratio Lower Upper
117 100
82 57.4 45.4 68.0
119 33.3 25.4 38.2

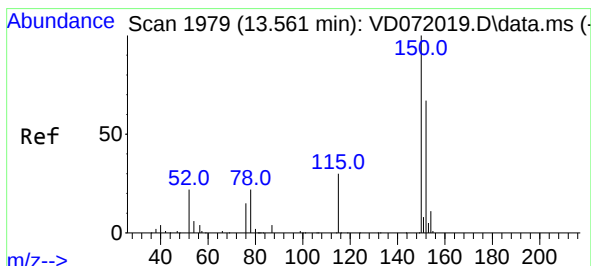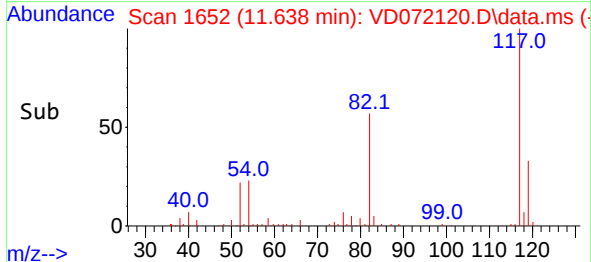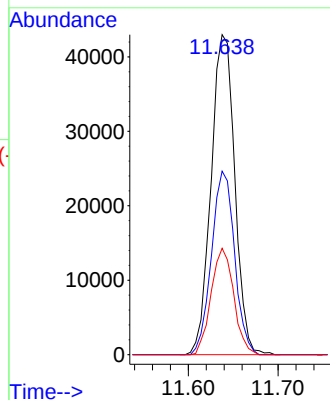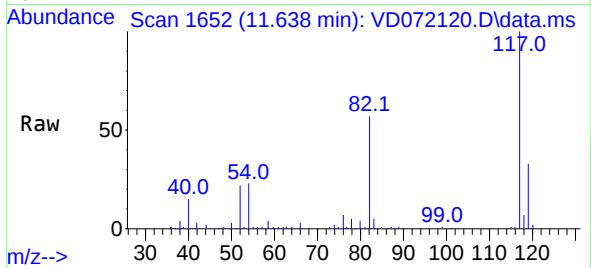

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. 0.006 min
Lab File: VD072120.D
Acq: 28 Feb 2022 14:03

Tgt Ion:152 Resp: 38059
Ion Ratio Lower Upper
152 100
115 61.4 29.9 89.7
150 160.1 0.0 347.6

