
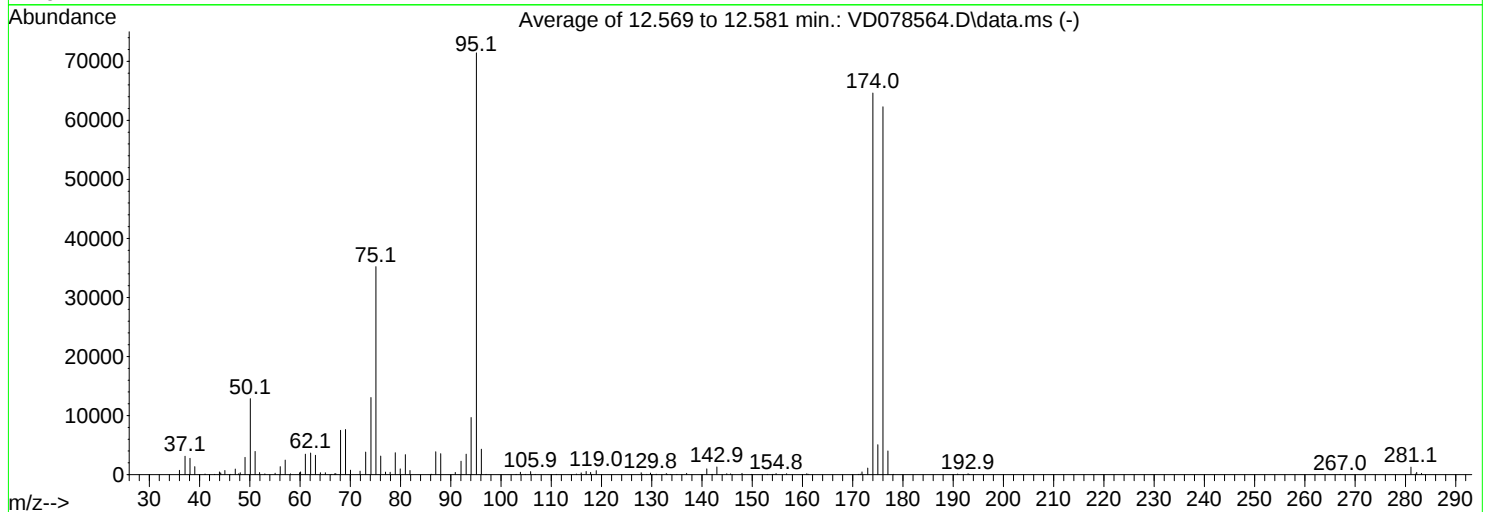


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022824\
Data File : VD078564.D
Acq On : 28 Feb 2024 08:57
Operator : RP/MD
Sample : BFB204
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB204

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM022724SMA.M
Title : SFAM01.0
Last Update : Wed Feb 28 23:05:03 2024

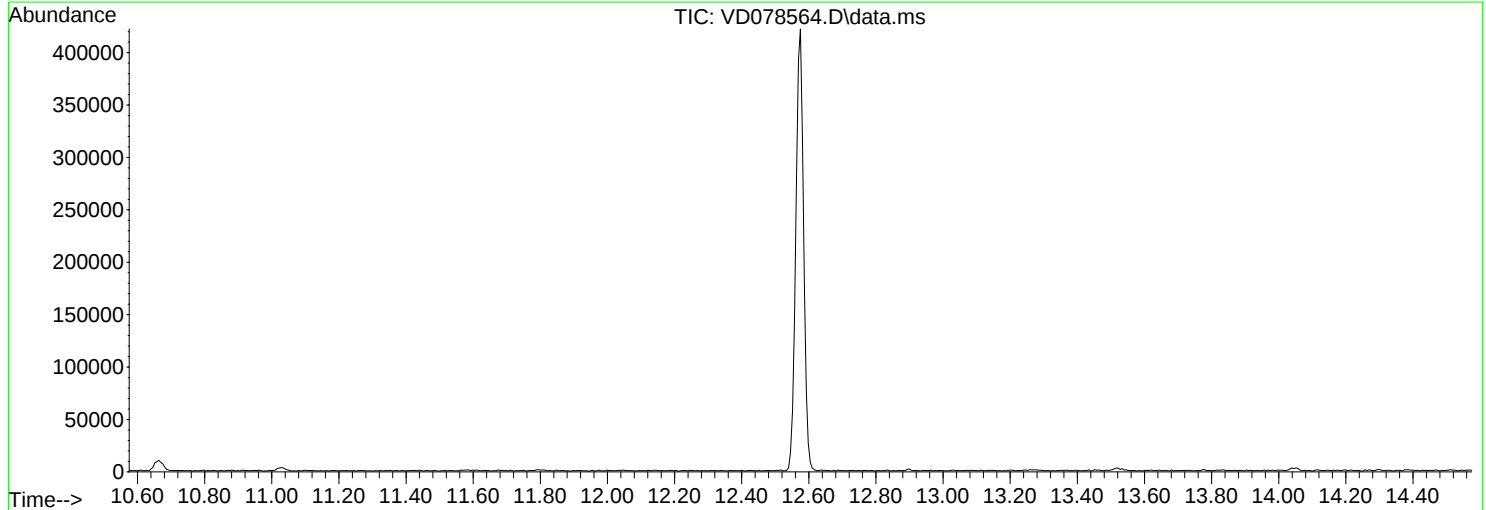

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	12861	PASS
75	95	30	80	49.3	35221	PASS
95	95	100	100	100.0	71435	PASS
96	95	5	9	6.0	4315	PASS
173	174	0.00	2	1.7	1107	PASS
174	95	50	120	90.5	64637	PASS
175	174	5	9	7.8	5063	PASS
176	174	95	105	96.4	62296	PASS
177	176	5	10	6.4	4002	PASS

Scan 1860 (12.528 min): VD078564.D\data.ms
BFB204

m/z	Abundance
40.00	788.0
43.90	196.0

Instrument :
MSVOA_D
ClientSampleId :
BFB204

m/z	Abundance
36.00	769.0
37.10	3554.0
38.10	2888.0
39.00	1655.0
40.00	659.0
44.00	957.0
45.10	825.0
47.10	925.0
48.10	395.0
49.00	3036.0
50.10	13922.0
51.00	4151.0
52.00	511.0
53.10	195.0
55.10	192.0
56.10	1514.0
57.20	2538.0
58.10	216.0
59.90	979.0
61.10	3429.0
62.10	3941.0
63.00	3341.0
64.10	274.0
65.10	321.0
66.90	410.0
68.10	7849.0
69.00	7349.0
70.10	976.0
72.00	881.0
73.00	4190.0
74.10	13316.0
75.10	37248.0
76.10	3218.0
77.10	413.0
78.00	372.0
79.00	4185.0
80.00	852.0
81.00	3657.0
81.90	661.0
86.10	277.0
87.00	4174.0
88.00	4177.0
90.90	345.0
92.00	2680.0
93.00	3685.0
94.10	10557.0
95.10	75048.0
96.10	4863.0
97.00	206.0
103.90	329.0
105.80	460.0
106.80	198.0
111.00	156.0
115.00	159.0
115.90	346.0
116.90	578.0
117.90	279.0
118.90	735.0
128.00	581.0
129.80	340.0
132.90	213.0
135.00	203.0
136.90	209.0
141.00	861.0
142.00	159.0
143.00	1269.0
145.00	241.0
147.90	242.0
154.10	158.0
154.70	161.0
160.80	289.0
171.50	260.0
173.00	1040.0
174.00	66848.0
175.00	5037.0
176.00	63200.0
177.00	3875.0
178.10	155.0
190.90	170.0
193.00	228.0
281.10	864.0
282.00	345.0
283.20	190.0

Instrument :
MSVOA_D
ClientSampleId :
BFB204

m/z	Abundance
36.00	741.0
37.10	3365.0
38.10	3428.0
39.10	1444.0
40.10	879.0
43.00	170.0
44.20	905.0
45.00	730.0
46.10	163.0
47.10	1061.0
47.80	474.0
49.10	3608.0
50.10	14953.0
51.10	4260.0
51.90	235.0
55.00	356.0
56.10	1435.0
57.00	2490.0
58.10	173.0
60.10	799.0
61.10	3915.0
62.10	4477.0
63.10	3698.0
64.10	327.0
65.00	390.0
66.20	174.0
67.10	341.0
68.00	8539.0
69.10	9180.0
70.00	728.0
71.90	471.0
73.10	4081.0
74.10	15049.0
75.10	39896.0
76.00	3491.0
76.90	450.0
77.90	518.0
78.90	4380.0
79.90	1067.0
80.90	3651.0
81.90	966.0
87.00	3951.0
88.00	3317.0
90.90	499.0
92.00	2295.0
93.00	3919.0
94.10	10575.0
95.10	79184.0
96.10	4829.0
103.00	200.0
103.90	417.0
104.80	155.0
105.90	770.0
115.00	189.0
116.00	356.0
117.00	623.0
117.90	523.0
119.00	652.0
127.80	247.0
128.20	179.0
129.00	166.0
129.70	318.0
132.90	384.0
133.70	163.0
136.90	211.0
140.90	1284.0
142.90	1430.0
144.90	236.0
145.70	216.0
148.00	257.0
149.80	207.0
153.00	163.0
154.80	211.0
156.80	375.0
160.90	175.0
171.10	181.0
171.90	834.0
173.00	1514.0
174.00	71328.0
175.00	5685.0
176.00	69752.0
177.00	4577.0
190.90	176.0
192.90	251.0
267.00	160.0
281.10	1127.0
282.30	419.0
283.20	435.0

Instrument :
MSVOA_D
ClientSampleId :
BFB204

m/z	Abundance
36.00	671.0
37.10	2429.0
38.10	1992.0
39.10	1010.0
40.00	903.0
41.10	302.0
44.00	985.0
45.00	557.0
47.10	824.0
48.10	556.0
49.10	2113.0
50.10	9707.0
51.10	3363.0
52.00	303.0
52.90	222.0
55.00	179.0
56.00	1084.0
57.00	2349.0
60.10	554.0
61.00	3061.0
62.10	2526.0
63.10	2799.0
64.00	369.0
65.00	239.0
67.10	277.0
68.10	6138.0
69.10	6419.0
70.10	574.0
71.90	469.0
73.00	3230.0
74.10	10845.0
75.10	28520.0
76.10	2766.0
77.00	424.0
77.90	304.0
78.90	2537.0
80.00	1036.0
80.90	2874.0
81.80	491.0
87.00	3515.0
88.00	3192.0
90.80	268.0
92.10	1885.0
93.10	2789.0
94.00	7872.0
95.10	60072.0
96.10	3252.0
103.80	459.0
106.00	332.0
116.00	244.0
116.90	434.0
117.80	336.0
118.90	671.0
127.80	172.0
129.70	195.0
130.90	230.0
133.10	150.0
137.00	229.0
141.00	790.0
142.90	1190.0
145.70	233.0
147.90	189.0
154.70	194.0
156.90	159.0
161.10	219.0
171.80	519.0
172.90	766.0
174.00	55736.0
175.00	4466.0
176.00	53936.0
177.00	3555.0
193.20	174.0
281.10	1865.0
282.20	720.0

Instrument :
MSVOA_D
ClientSampleId :
BFB204