

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030121\
 Data File : VD068472.D
 Acq On : 01 Mar 2021 10:58
 Operator : VA/SY
 Sample : VD0301SBL01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0301SBL01

Quant Time: Mar 01 20:44:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 26 14:04:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	439502	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	770917	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	729690	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	331474	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	216259	49.25	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	98.50%
35) Dibromofluoromethane	7.920	113	231792	49.91	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.82%
50) Toluene-d8	10.338	98	969560	52.42	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.84%
62) 4-Bromofluorobenzene	12.632	95	311473	52.25	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	104.50%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030121\
Data File : VD068472.D
Acq On : 01 Mar 2021 10:58
Operator : VA/SY
Sample : VD0301SBL01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0301SBL01

Quant Time: Mar 01 20:44:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
Quant Title : SW846 8260
QLast Update : Fri Feb 26 14:04:14 2021
Response via : Initial Calibration




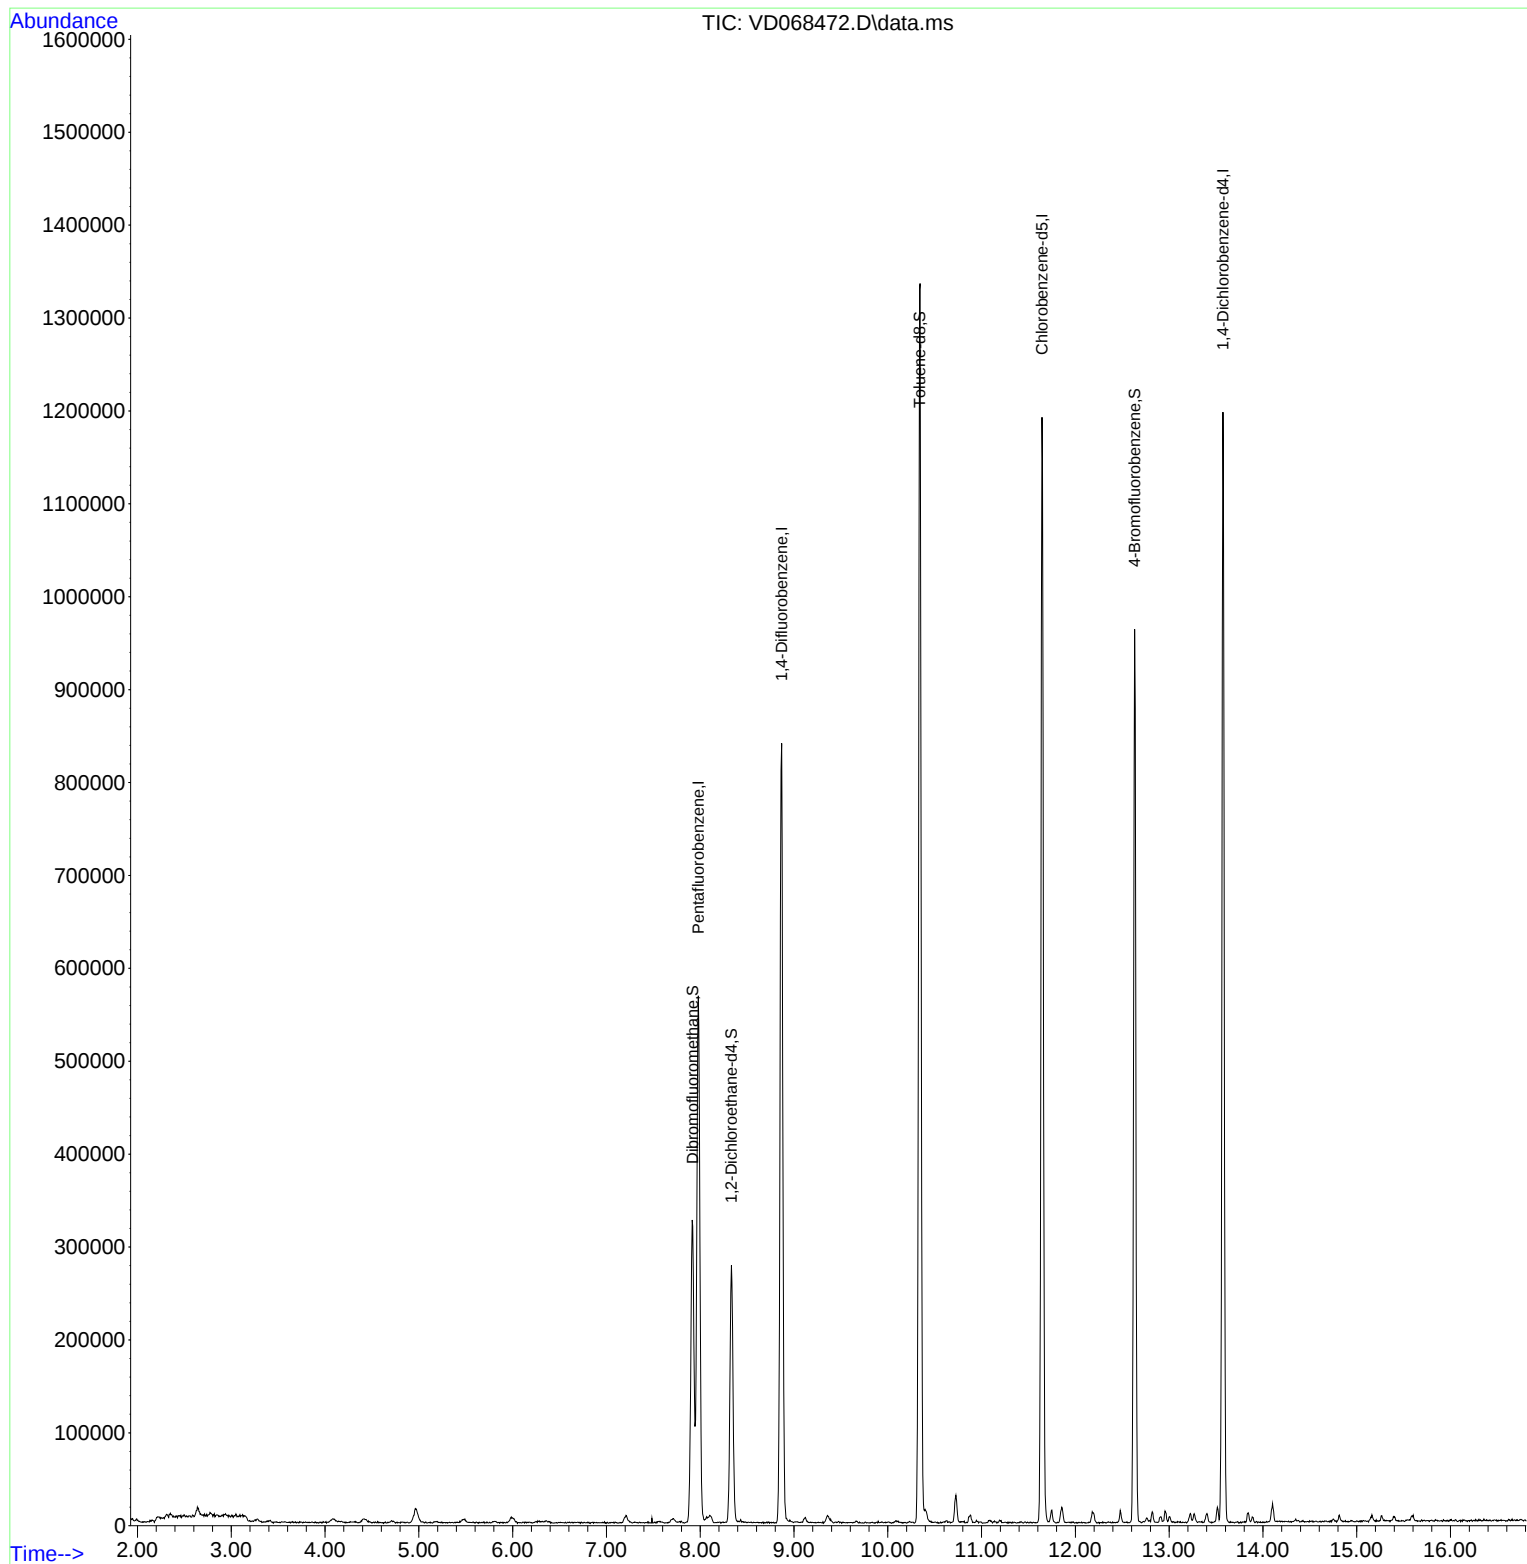


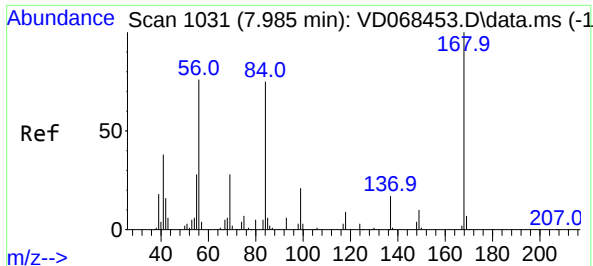

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD068472.D
Acq: 01 Mar 2021 10:58




Instrument :
MSVOA_D
ClientSampleId :
VD0301SBL01


Tgt Ion:168 Resp: 439502
Ion Ratio Lower Upper
168 100
99 55.6 43.5 65.3

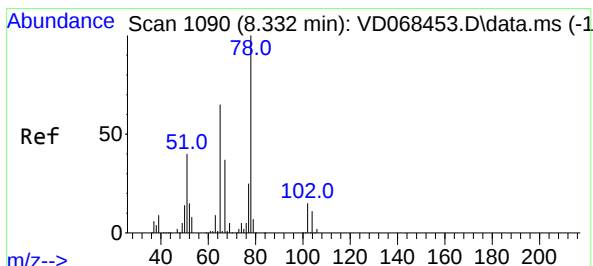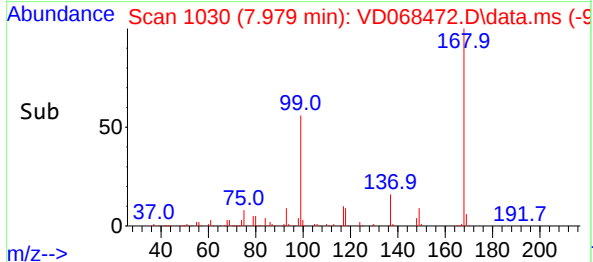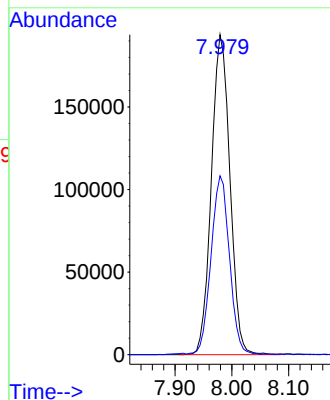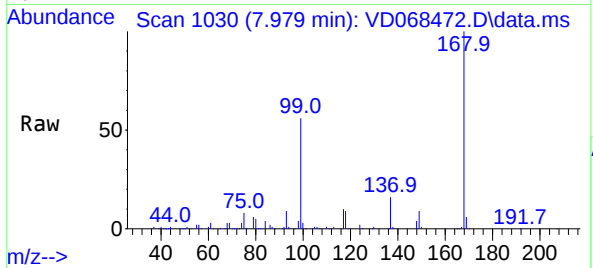

#33
1,2-Dichloroethane-d4
Concen: 49.25 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. 0.001 min
Lab File: VD068472.D
Acq: 01 Mar 2021 10:58

Tgt Ion: 65 Resp: 216259
Ion Ratio Lower Upper
65 100
67 54.1 0.0 105.0

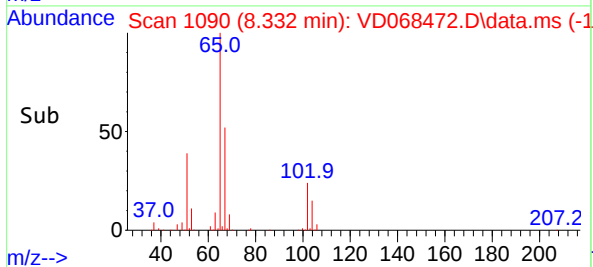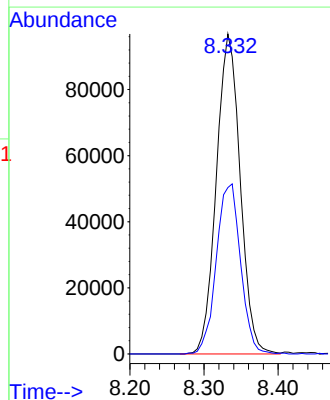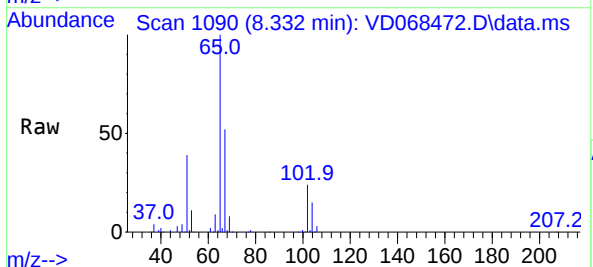




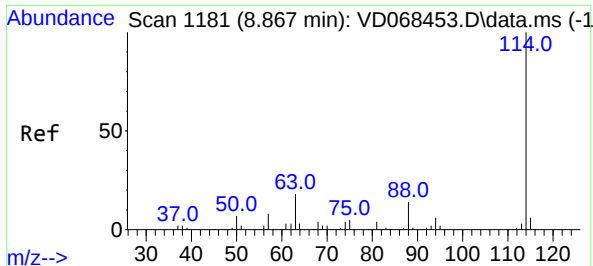


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.001 min
Lab File: VD068472.D
Acq: 01 Mar 2021 10:58

Instrument :
MSVOA_D
ClientSampleId :
VD0301SBL01




Tgt Ion:114 Resp: 770917
Ion Ratio Lower Upper
114 100
63 18.0 0.0 34.8
88 14.6 0.0 31.6

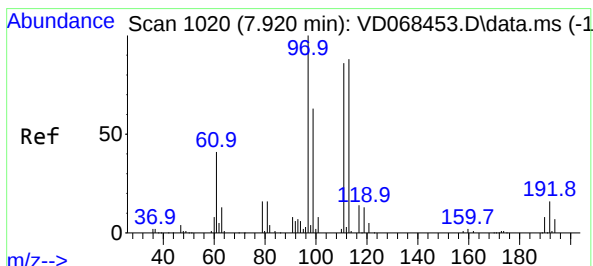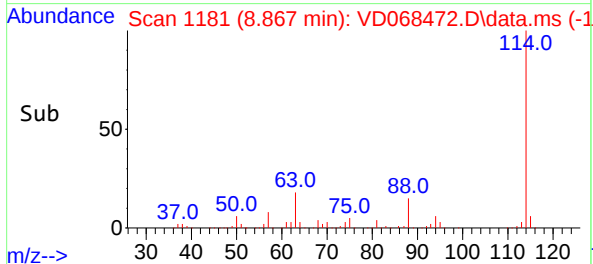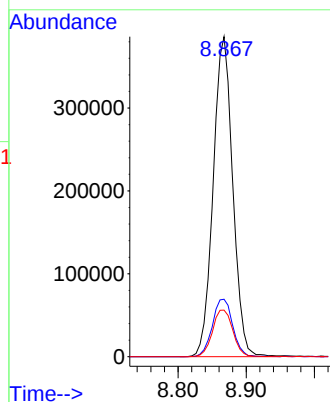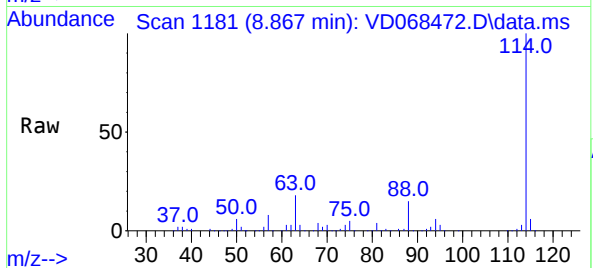


#35

Dibromofluoromethane
Concen: 49.91 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. 0.000 min
Lab File: VD068472.D
Acq: 01 Mar 2021 10:58

Tgt Ion:113 Resp: 231792
Ion Ratio Lower Upper
113 100
111 105.1 81.4 122.0
192 19.8 16.1 24.1


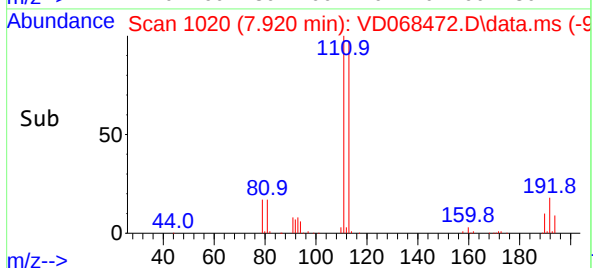
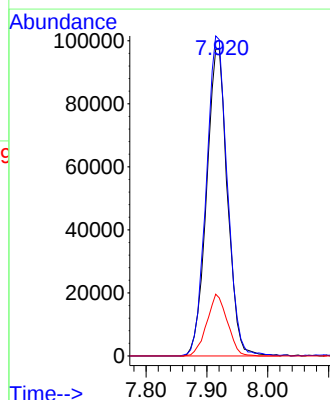
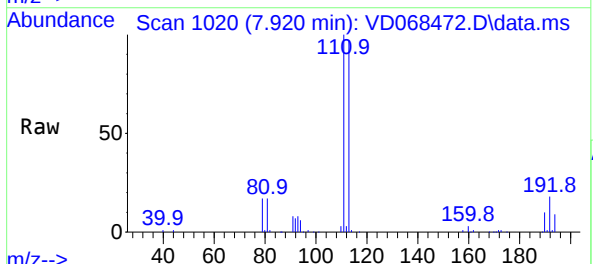


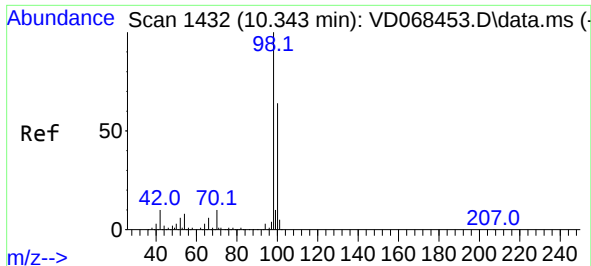

#50
Toluene-d8
Concen: 52.42 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.005 min
Lab File: VD068472.D
Acq: 01 Mar 2021 10:58




Instrument :
MSVOA_D
ClientSampleId :
VD0301SBL01


Tgt Ion: 98 Resp: 969560
Ion Ratio Lower Upper
98 100
100 63.8 53.0 79.4

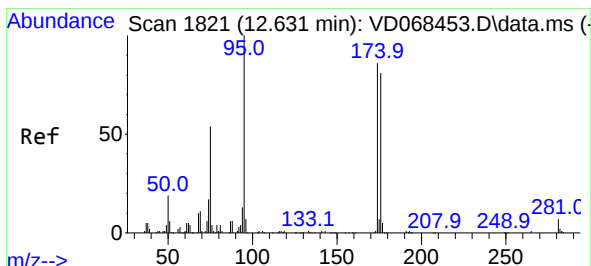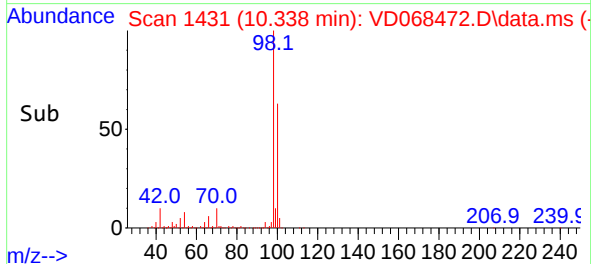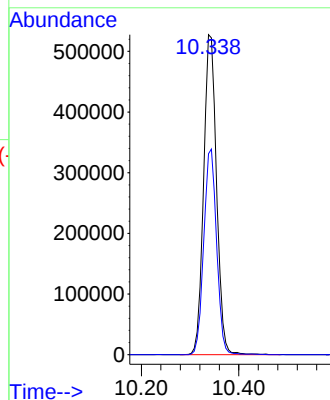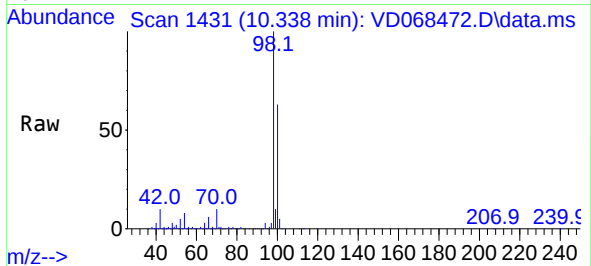

#62
4-Bromofluorobenzene
Concen: 52.25 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.001 min
Lab File: VD068472.D
Acq: 01 Mar 2021 10:58

Tgt Ion: 95 Resp: 311473
Ion Ratio Lower Upper
95 100
174 84.3 0.0 172.4
176 80.0 0.0 168.4


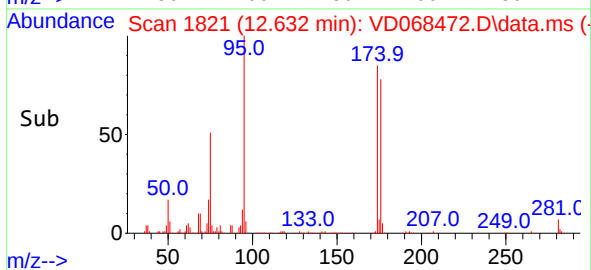
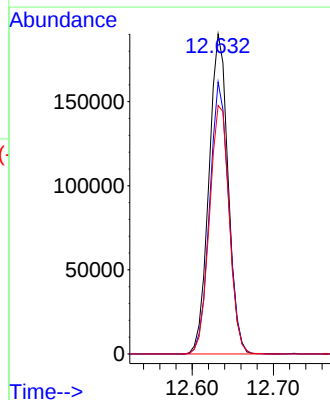
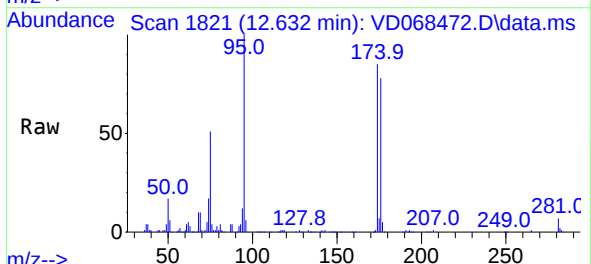


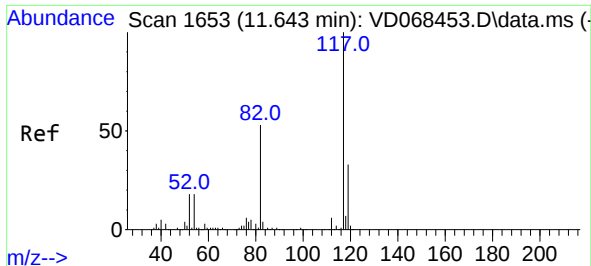

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. 0.001 min
Lab File: VD068472.D
Acq: 01 Mar 2021 10:58

Instrument :
MSVOA_D
ClientSampleId :
VD0301SBL01

Tgt Ion:	117	Resp:	729690
Ion	Ratio	Lower	Upper
117	100		
82	52.4	41.4	62.0
119	33.1	26.1	39.1

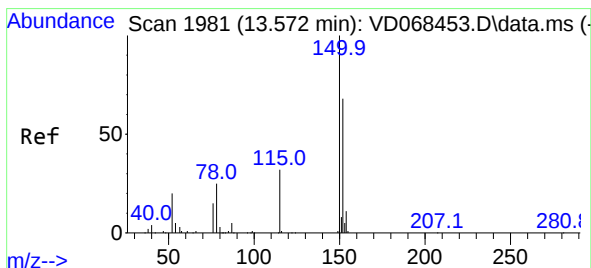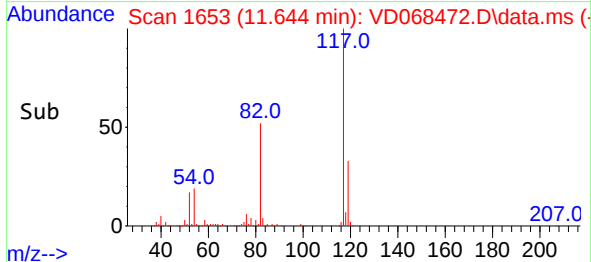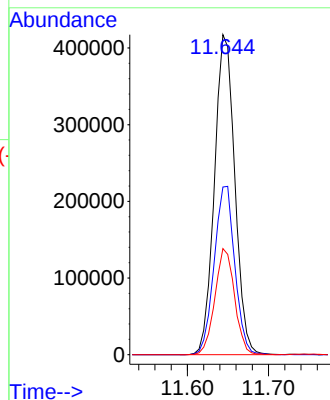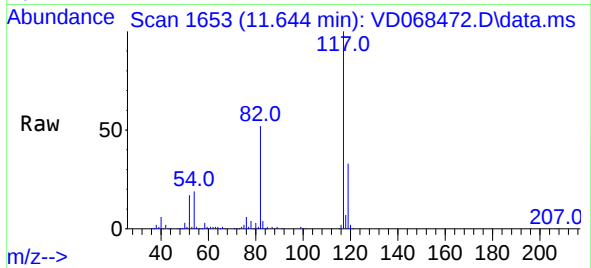

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. 0.001 min
Lab File: VD068472.D
Acq: 01 Mar 2021 10:58

Tgt Ion:	152	Resp:	331474
Ion	Ratio	Lower	Upper
152	100		
115	57.8	28.9	86.8
150	156.4	0.0	344.4

