
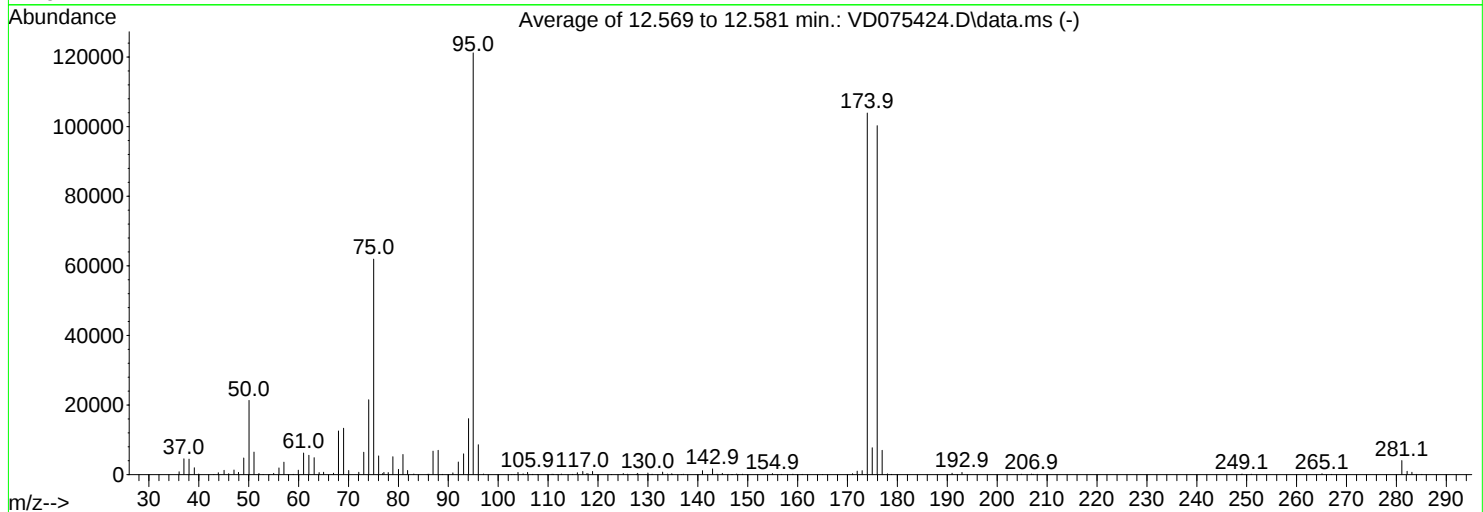


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030123\
Data File : VD075424.D
Acq On : 01 Mar 2023 12:50
Operator : KP/SY
Sample : BFB102
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB102

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Title : SFAM01.0
Last Update : Fri Mar 03 04:38:18 2023

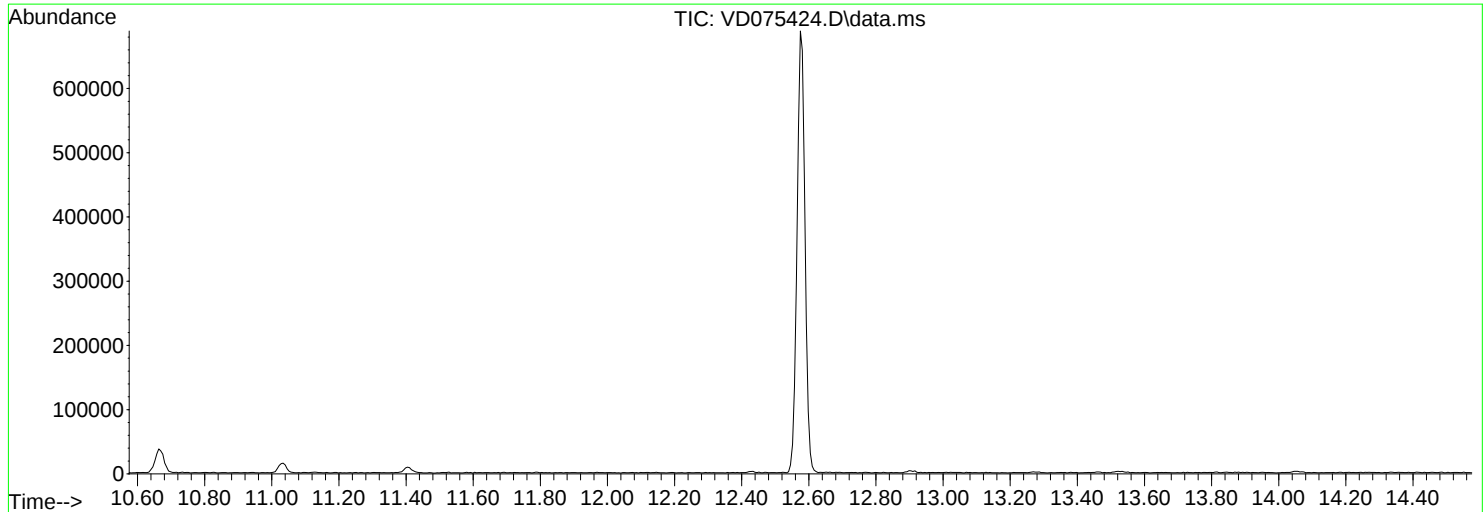

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	21328	PASS
75	95	30	80	51.1	61933	PASS
95	95	100	100	100.0	121216	PASS
96	95	5	9	7.1	8612	PASS
173	174	0.00	2	1.1	1138	PASS
174	95	50	120	85.7	103904	PASS
175	174	5	9	7.5	7744	PASS
176	174	95	105	96.5	100299	PASS
177	176	5	10	7.0	6988	PASS

m/z	Abundance
40.00	1177.0
41.00	233.0
43.90	789.0

Instrument :
MSVOA_D
ClientSampleId :
BFB102

m/z	Abundance
36.10	593.0
37.00	3934.0
38.10	4124.0
39.10	1723.0
40.00	1211.0
43.90	1538.0
45.00	1101.0
46.10	210.0
47.00	1037.0
48.00	515.0
49.00	4151.0
50.00	18088.0
51.00	6035.0
52.00	336.0
52.90	154.0
55.10	412.0
56.00	1574.0
57.00	3551.0
57.90	197.0
59.90	764.0
61.00	5622.0
62.00	4985.0
63.10	4393.0
64.20	660.0
65.00	692.0
67.00	334.0
68.00	11180.0
69.00	11538.0
70.00	1135.0
72.10	582.0
73.00	5561.0
74.10	18920.0
75.00	53616.0
76.00	4906.0
76.80	808.0
77.90	339.0
78.90	4268.0
80.10	1150.0
80.90	5108.0
81.90	908.0
83.10	299.0
86.90	6103.0
87.90	6346.0
90.90	407.0
92.00	3771.0
93.10	4981.0
94.00	13578.0
95.00	105504.0
96.00	7698.0
97.10	427.0
103.20	180.0
104.00	521.0
104.90	236.0
106.00	656.0
111.10	324.0
112.60	187.0
115.80	493.0
117.00	1036.0
117.90	556.0
118.90	774.0
124.90	160.0
127.80	395.0
130.00	522.0
130.80	171.0
133.00	810.0
134.70	334.0
140.90	1134.0
142.90	1301.0
143.90	239.0
144.90	408.0
146.80	189.0
147.80	205.0
148.90	184.0
154.90	220.0
159.00	226.0
171.00	266.0
171.90	1091.0
172.90	1097.0
173.90	86872.0
174.90	6235.0
175.90	83224.0
177.00	5480.0
178.10	164.0
191.00	297.0
193.00	379.0
194.10	178.0
206.90	180.0
248.90	189.0
281.10	2320.0
282.10	544.0
283.10	500.0

Instrument :
MSVOA_D
ClientSampleId :
BFB102

m/z	Abundance
36.10	1128.0
37.00	4907.0
38.10	5203.0
39.10	2223.0
40.00	1218.0
43.00	188.0
43.90	1195.0
45.00	1306.0
45.90	292.0
47.10	1917.0
48.00	930.0
49.00	4736.0
50.10	24144.0
51.00	7409.0
52.10	478.0
54.20	201.0
54.90	449.0
56.10	2474.0
57.00	3919.0
58.90	273.0
60.00	1729.0
61.00	6344.0
62.10	5996.0
63.10	4795.0
64.00	630.0
65.00	626.0
66.90	389.0
67.10	390.0
68.00	12708.0
69.00	14476.0
70.10	1203.0
72.00	866.0
73.00	6908.0
74.00	23384.0
75.00	68056.0
76.10	5374.0
77.10	1129.0
77.90	490.0
78.90	6116.0
80.00	1535.0
80.90	6323.0
81.90	1496.0
83.10	225.0
85.80	292.0
87.00	7945.0
87.90	7291.0
90.90	682.0
92.00	3912.0
93.00	6528.0
94.00	18416.0
95.00	133056.0
96.00	9560.0
102.70	208.0
103.90	896.0
105.00	322.0
105.80	698.0
106.90	244.0
107.90	183.0
111.80	152.0
112.70	350.0
115.90	564.0
116.90	907.0
117.70	422.0
118.90	1112.0
125.00	295.0
125.90	160.0
128.00	558.0
130.00	435.0
133.00	597.0
134.10	167.0
134.90	414.0
136.70	207.0
141.00	970.0
141.90	151.0
142.90	1993.0
143.80	212.0
144.90	397.0
146.00	153.0
147.80	294.0
149.00	190.0
155.00	318.0
156.80	299.0
159.10	163.0
165.00	158.0
171.10	289.0
171.90	824.0
173.00	1271.0
173.90	112984.0
175.00	9343.0
176.00	110392.0
177.00	7818.0
178.00	281.0

Instrument :
MSVOA_D
ClientSampleId :
BFB102

190.90	377.0
192.00	153.0
193.00	709.0
204.90	235.0
207.20	353.0
249.10	285.0
251.00	197.0
265.10	304.0
281.10	3998.0
282.20	1374.0
283.10	585.0

Instrument :
MSVOA_D
ClientSampleId :
BFB102

m/z	Abundance
36.00	746.0
37.00	4897.0
38.00	4004.0
39.10	1935.0
40.00	1688.0
44.00	1330.0
45.10	1273.0
46.00	280.0
47.00	1077.0
47.80	513.0
49.00	5410.0
50.00	21752.0
51.10	5997.0
52.00	199.0
55.10	234.0
56.10	1775.0
57.10	3303.0
59.90	1351.0
61.00	6629.0
62.00	5661.0
63.10	5420.0
64.10	549.0
65.00	766.0
66.90	159.0
68.00	13775.0
69.00	14051.0
70.00	1263.0
72.00	662.0
73.10	6868.0
74.00	22304.0
75.10	64128.0
76.00	5812.0
77.10	844.0
78.00	929.0
78.90	5133.0
79.90	1894.0
80.90	5948.0
81.80	1129.0
86.10	404.0
87.00	6179.0
88.00	7345.0
88.80	345.0
90.90	477.0
92.00	3259.0
93.00	6452.0
94.10	16307.0
95.00	125088.0
96.00	8578.0
97.00	153.0
103.90	555.0
105.10	186.0
105.90	643.0
109.80	189.0
110.80	468.0
114.90	345.0
115.90	600.0
116.90	809.0
118.00	734.0
118.90	843.0
122.70	176.0
125.10	483.0
125.90	210.0
127.90	523.0
130.00	378.0
130.90	191.0
132.90	858.0
133.90	331.0
134.70	310.0
137.10	456.0
140.90	1287.0
143.00	1727.0
144.90	332.0
146.10	175.0
147.00	171.0
148.20	187.0
154.90	376.0
160.90	249.0
170.90	256.0
172.00	1085.0
173.00	1045.0
174.00	111856.0
175.00	7653.0
176.00	107280.0
176.90	7666.0
177.90	230.0
178.80	278.0
190.90	528.0
192.90	868.0
204.80	192.0
206.90	313.0
208.10	233.0
249.00	228.0

Instrument :
MSVOA_D
ClientSampleId :
BFB102

250.80	181.0
265.10	478.0
267.00	258.0
281.10	5783.0
282.10	1049.0
283.10	980.0
284.00	239.0
285.10	242.0

Instrument :
MSVOA_D
ClientSampleId :
BFB102