
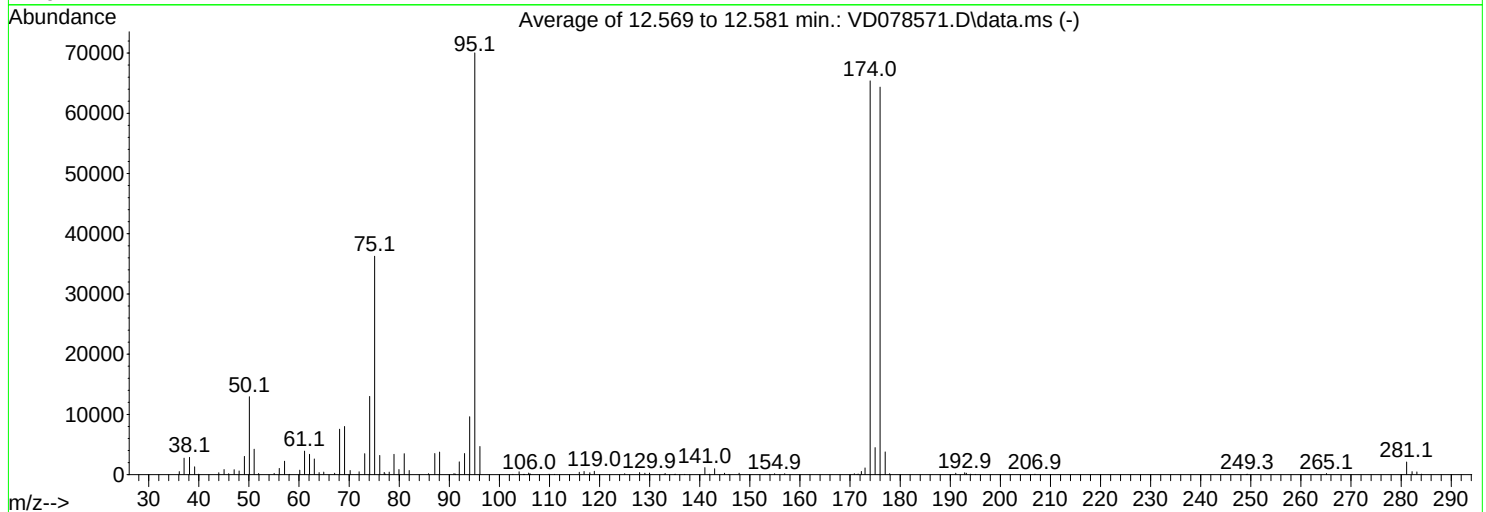


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030124\
Data File : VD078571.D
Acq On : 01 Mar 2024 08:36
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D030124S.M
Title : SW846 8260
Last Update : Sat Mar 02 03:50:17 2024

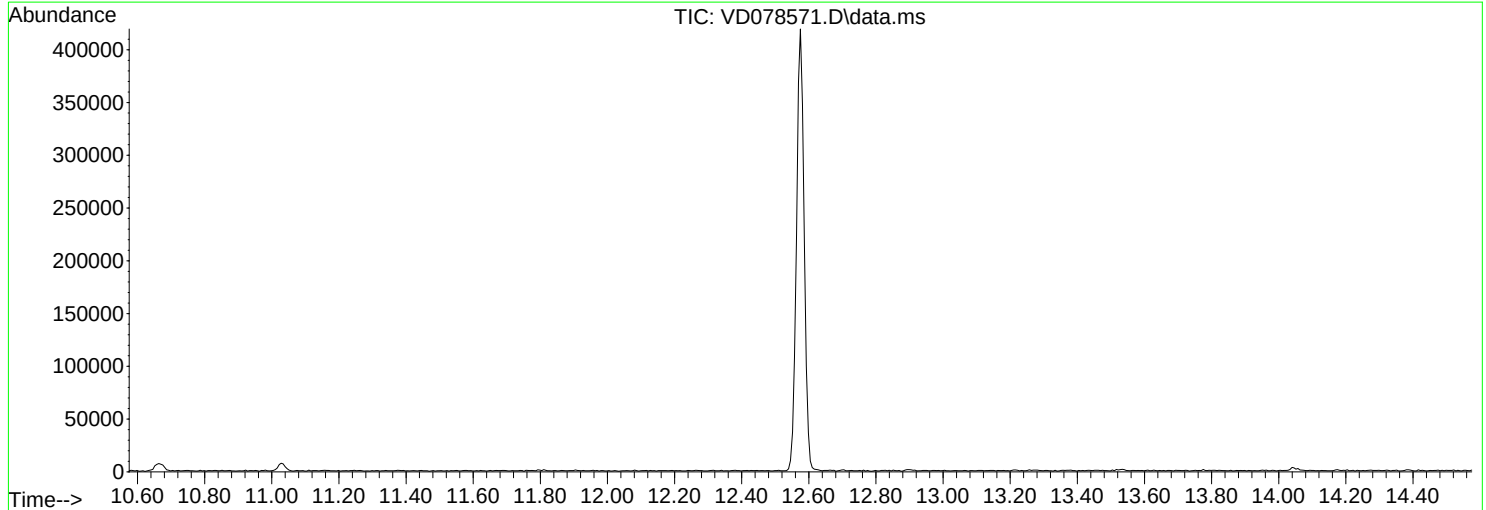

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	12940	PASS
75	95	30	60	51.8	36264	PASS
95	95	100	100	100.0	70035	PASS
96	95	5	9	6.7	4680	PASS
173	174	0.00	2	1.7	1116	PASS
174	95	50	100	93.4	65384	PASS
175	174	5	9	6.9	4494	PASS
176	174	95	101	98.4	64352	PASS
177	176	5	9	5.8	3764	PASS