

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD030220\
 Data File : VD065375.D
 Acq On : 02 Mar 2020 13:13
 Operator : VA/SY
 Sample : L1745-01
 Misc : 9.46G/5.00ml/MSVOA D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 MP-2-COMP

Quant Time: Mar 02 13:35:08 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D021820S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 19 03:26:54 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	547017	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	912641	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	832182	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	386575	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.34	65	285130	57.94	ug/l	0.00
Spiked Amount	50.000		Recovery	=	115.88%	
35) Dibromofluoromethane	7.92	113	294546	52.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.86%	
50) Toluene-d8	10.34	98	1086379	51.07	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.14%	
62) 4-Bromofluorobenzene	12.64	95	341171	50.62	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.24%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD030220\
Data File : VD065375.D
Acq On : 02 Mar 2020 13:13
Operator : VA/SY
Sample : L1745-01
Misc : 9.46G/5.00ml/MSVOA D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
MP-2-COMP

Quant Time: Mar 02 13:35:08 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D021820S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 19 03:26:54 2020
Response via : Initial Calibration

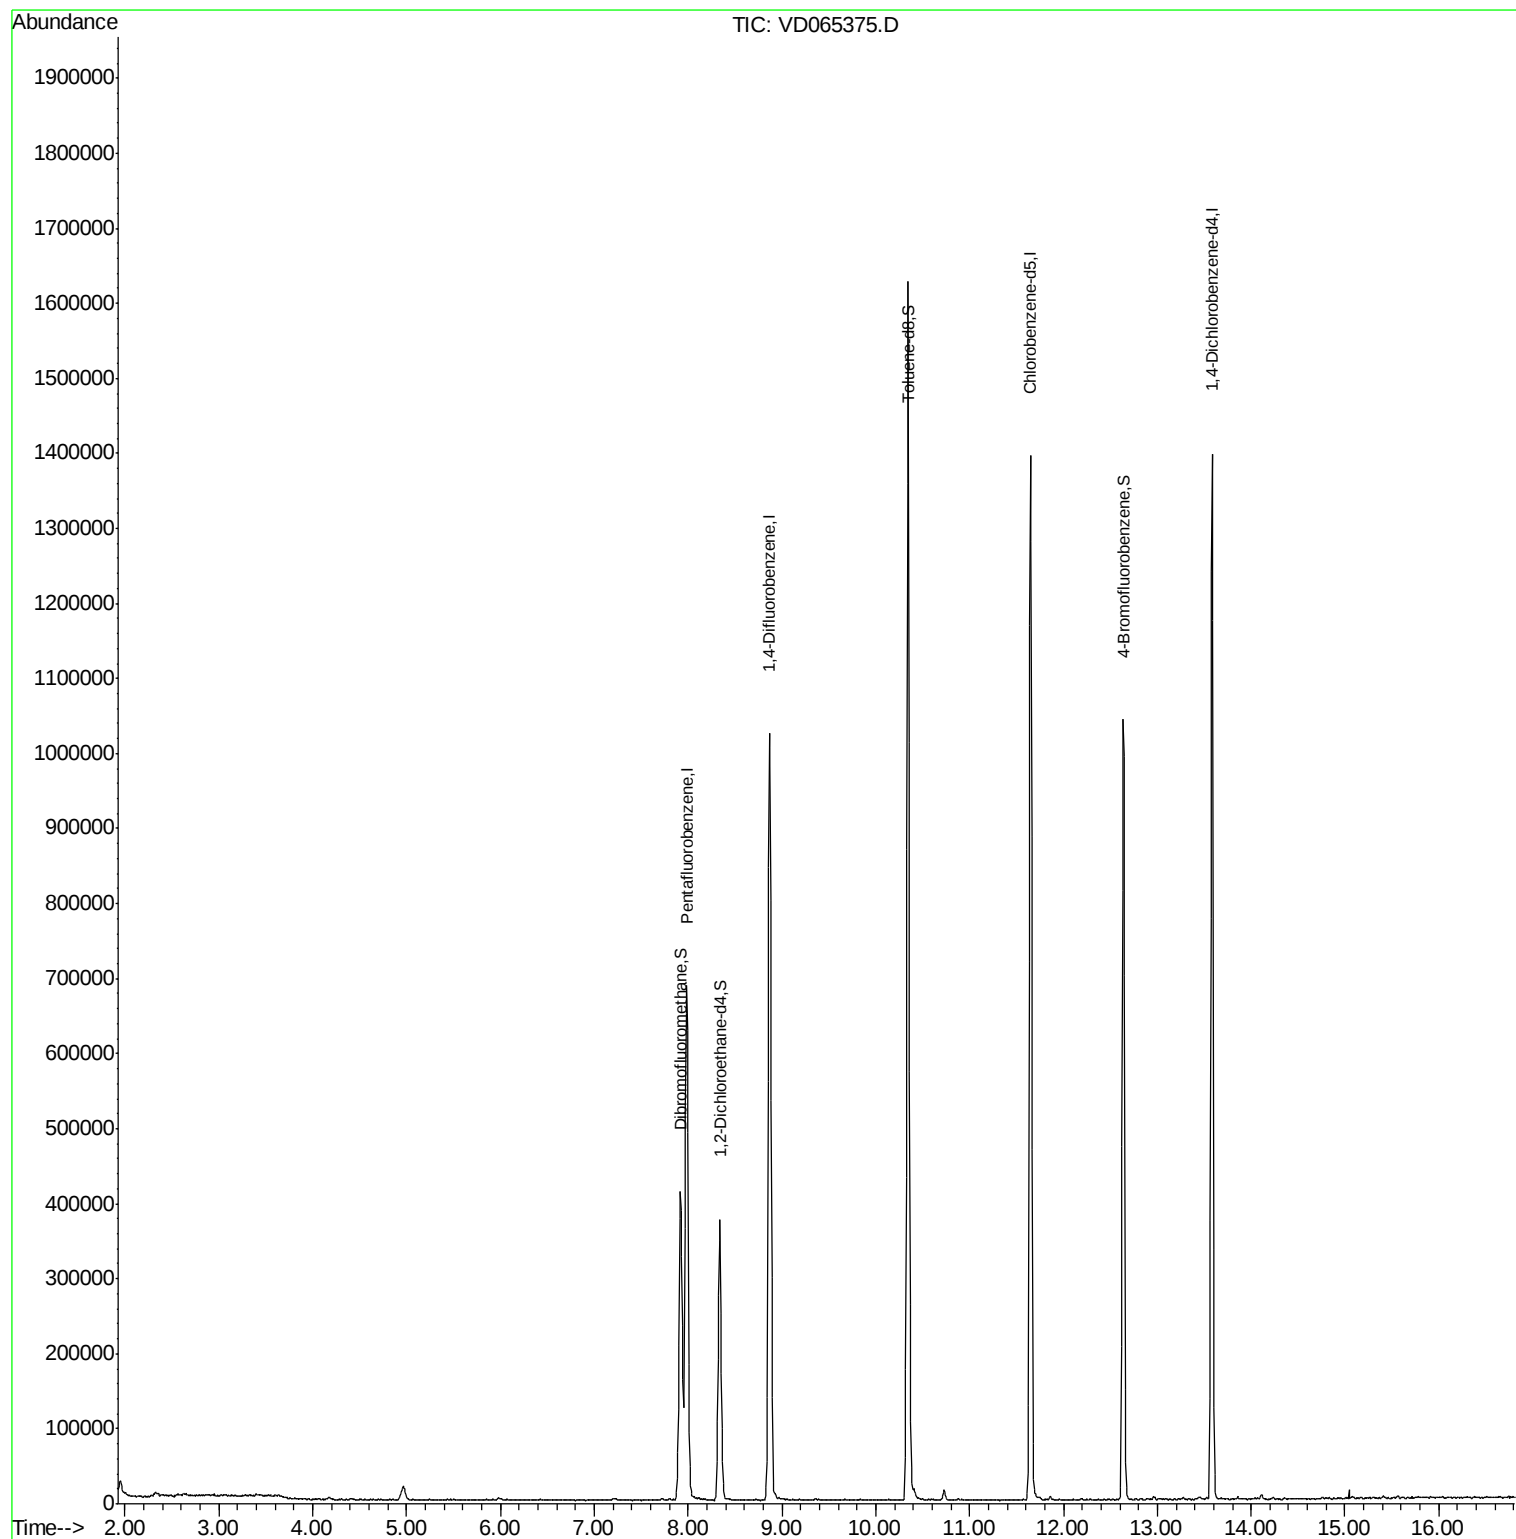

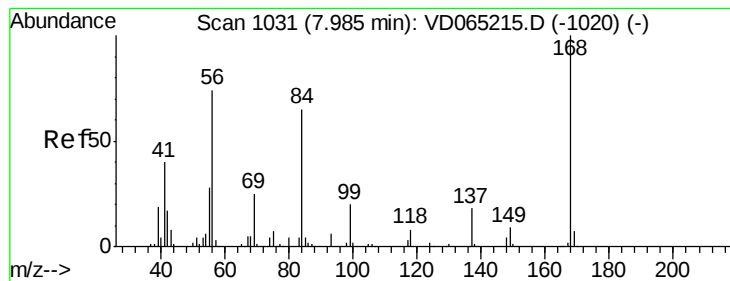

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VD065375.D

Acq: 02 Mar 2020 13:13

Instrument :

MSVOA_D

ClientSampleId :


MP-2-COMP

Tot Ion:168 Resp: 547017

Ion Ratio Lower Upper




168 100

99 51.7 41.4 62.2

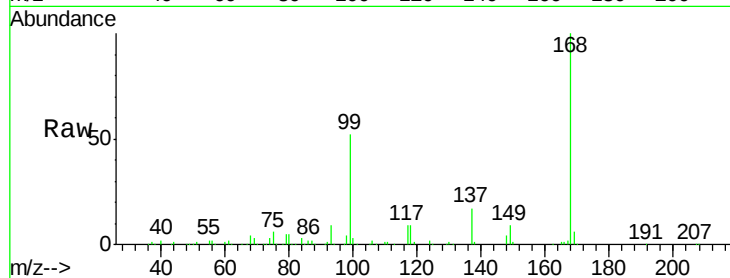

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

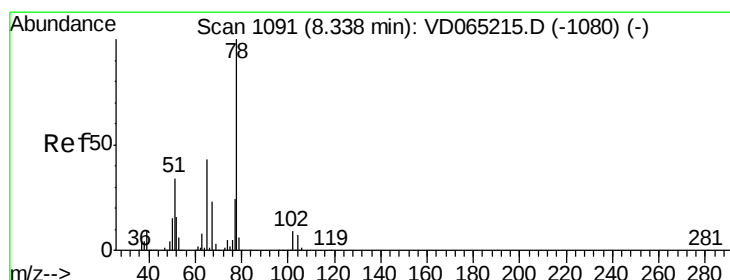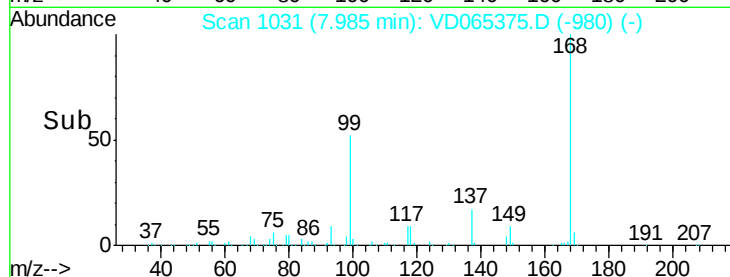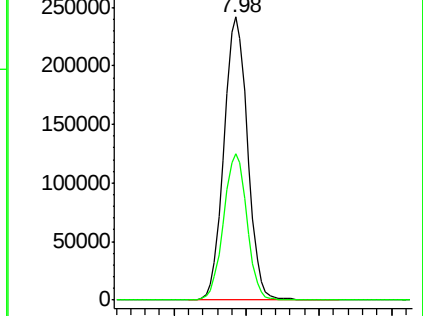

#33

1,2-Dichloroethane-d4

Concen: 57.941 ug/l

RT: 8.34 min Scan# 1091

Delta R.T. 0.00 min

Lab File: VD065375.D


Acq: 02 Mar 2020 13:13

Tgt Ion: 65 Resp: 285130

Ion Ratio Lower Upper



65 100


67 53.2 0.0 106.8

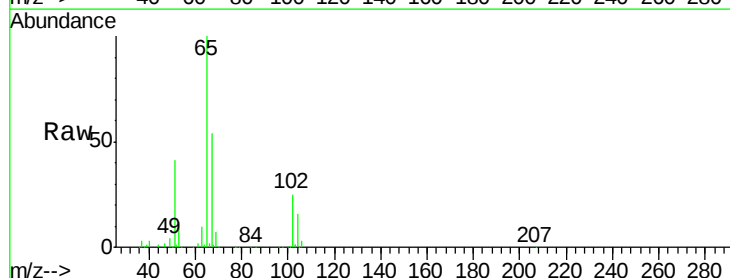

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

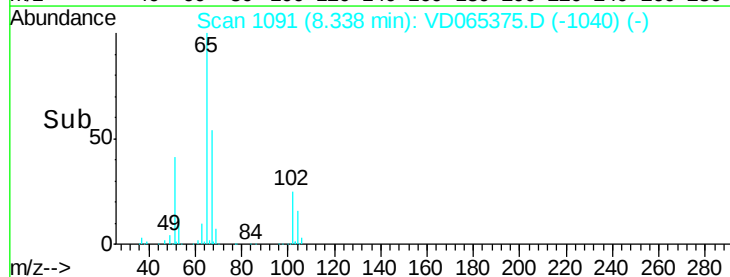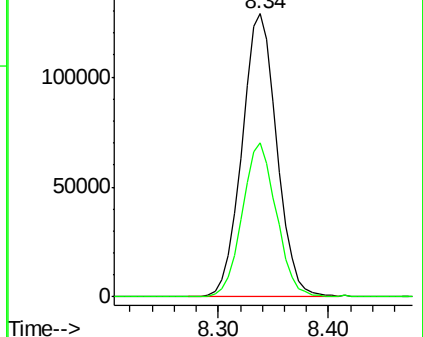


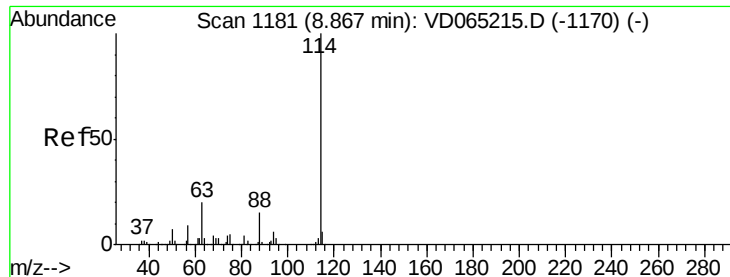




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. 0.00 min
 Lab File: VD065375.D
 Acq: 02 Mar 2020 13:13

Instrument :
 MSVOA_D
 ClientSampleId :
 MP-2-COMP

Tot Ion:114 Resp: 912641
 Ion Ratio Lower Upper
 114 100
 63 19.5 0.0 39.4
 88 14.3 0.0 30.4

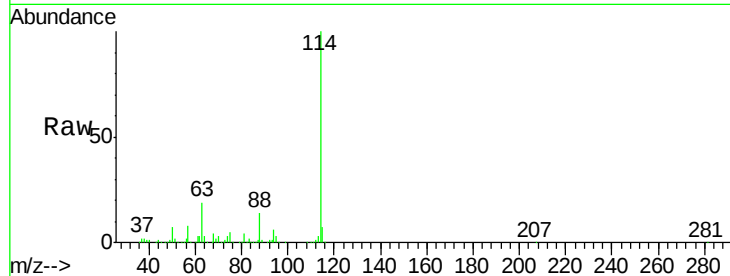


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): V
 Ion 87.90 (87.60 to 88.60): V

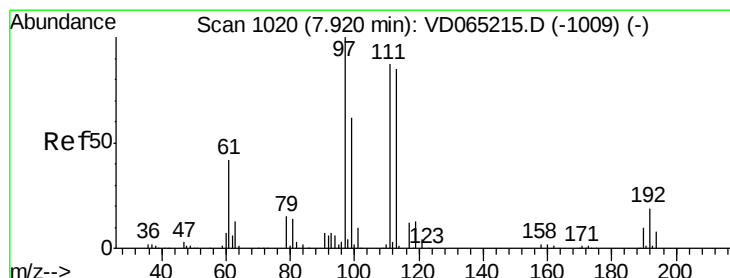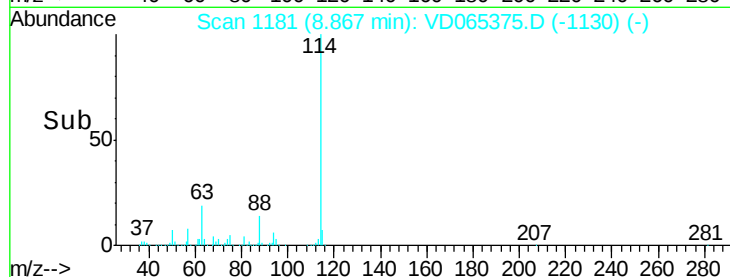
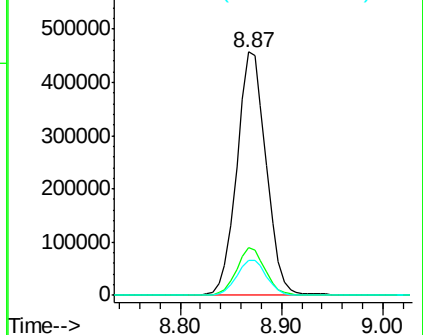


#35
 Dibromofluoromethane
 Concen: 52.931 ug/l
 RT: 7.92 min Scan# 1020
 Delta R.T. 0.00 min
 Lab File: VD065375.D
 Acq: 02 Mar 2020 13:13

Tgt Ion:113 Resp: 294546
 Ion Ratio Lower Upper
 113 100
 111 103.0 82.9 124.3
 192 22.0 17.3 25.9

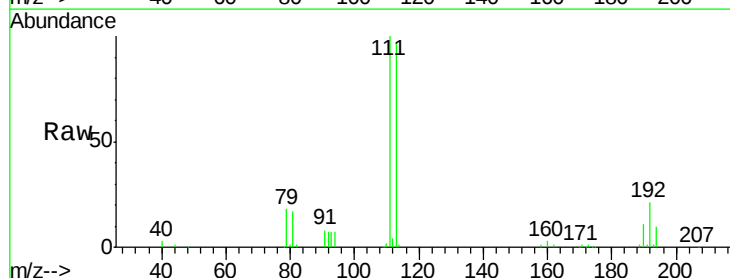

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



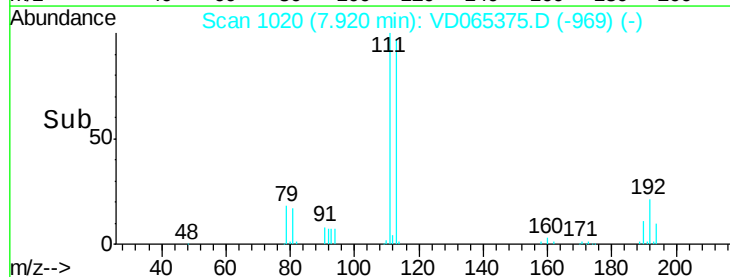
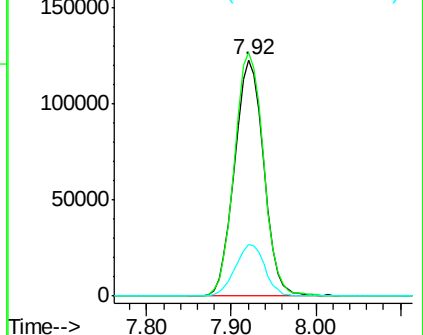




#50
Toluene-d8
Concen: 51.067 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. 0.00 min
Lab File: VD065375.D
Acq: 02 Mar 2020 13:13




Instrument :
MSVOA_D
ClientSampleId :
MP-2-COMP


Tot Ion: 98 Resp: 1086379
Ion Ratio Lower Upper
98 100
100 66.0 52.0 78.0

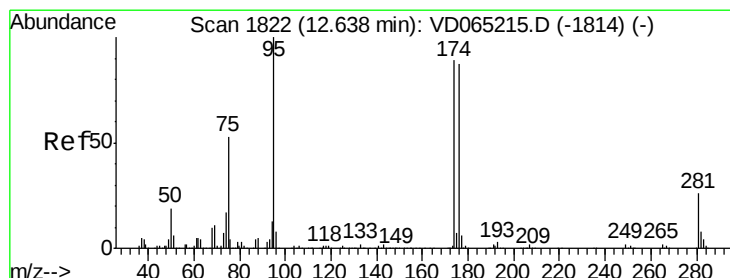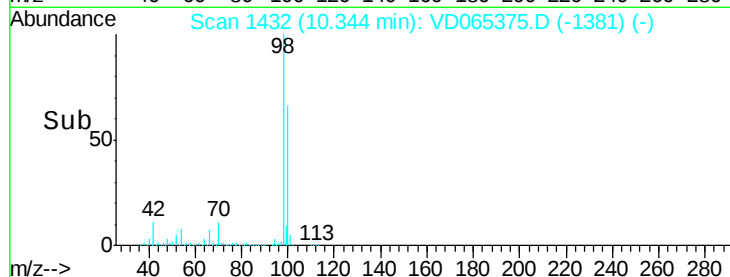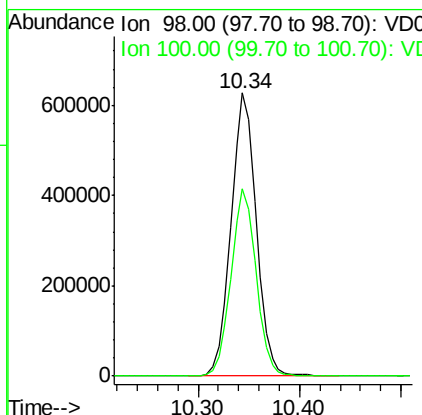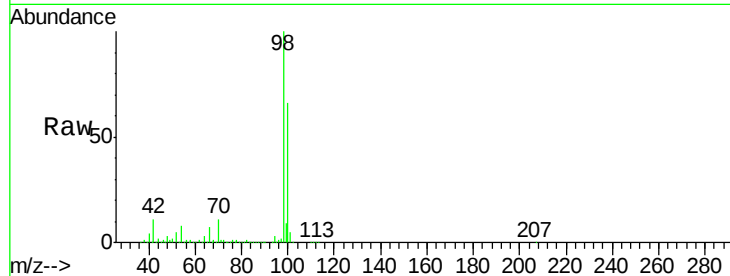

#62
4-Bromofluorobenzene
Concen: 50.624 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. 0.00 min
Lab File: VD065375.D
Acq: 02 Mar 2020 13:13

Tgt Ion: 95 Resp: 341171
Ion Ratio Lower Upper
95 100
174 89.4 0.0 178.0
176 87.0 0.0 174.4


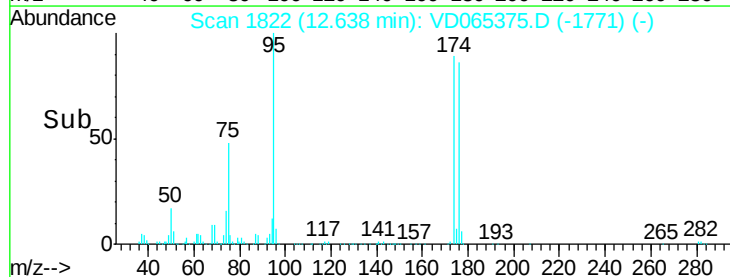
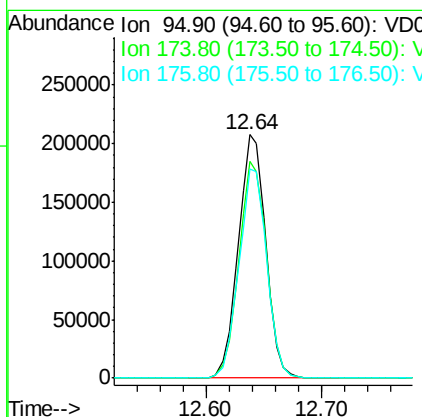
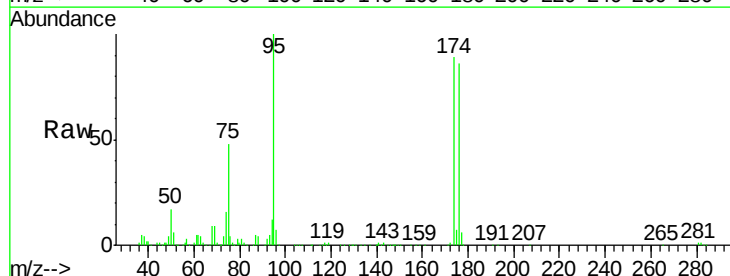


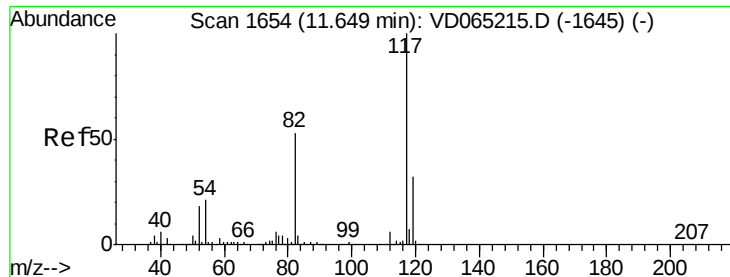

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD065375.D
Acq: 02 Mar 2020 13:13

Instrument :
MSVOA_D
ClientSampleId :
MP-2-COMP

Tot Ion:117 Resp: 832182
Ion Ratio Lower Upper
117 100
82 51.8 42.7 64.1
119 31.5 25.5 38.3

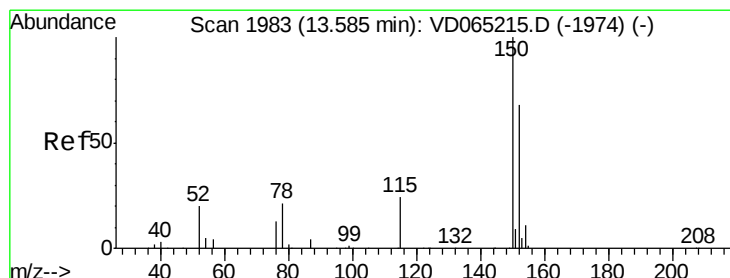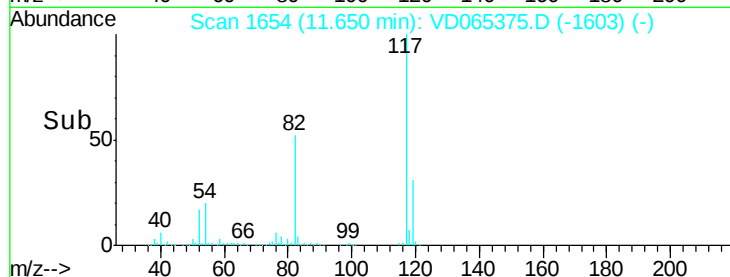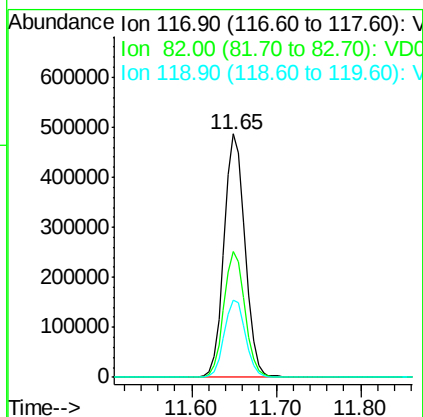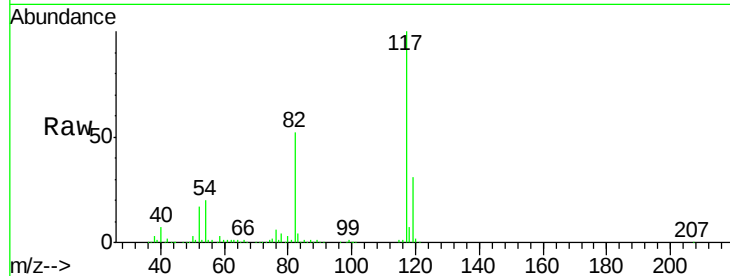

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1983
Delta R.T. 0.00 min
Lab File: VD065375.D
Acq: 02 Mar 2020 13:13

Tgt Ion:152 Resp: 386575
Ion Ratio Lower Upper
152 100
115 55.3 27.6 82.8
150 157.4 0.0 347.4

