

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030221\
 Data File : VD068500.D
 Acq On : 02 Mar 2021 17:06
 Operator : VA/SY
 Sample : M1540-01
 Misc : 6.60G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 PR-01-030221

Quant Time: Mar 02 23:59:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 26 14:04:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	47521	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	87333	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	90796	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.579	152	51981	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	37750	79.51	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	159.02%
35) Dibromofluoromethane	7.914	113	30277	57.55	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	115.10%
50) Toluene-d8	10.344	98	105297	50.25	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	100.50%
62) 4-Bromofluorobenzene	12.632	95	45206	66.94	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	133.88%


Target Compounds						Qvalue
10) Methyl Iodide	4.309	142	64	2.72	ug/l #	38
16) Acetone	4.162	43	904	11.99	ug/l #	44
20) Methylene Chloride	4.973	84	165	Below Cal	#	14
25) 2-Butanone	7.220	43	118	1.09	ug/l #	43
31) Cyclohexane	7.973	56	936	1.08	ug/l #	83
36) 1,1-Dichloropropene	7.979	75	3553	4.28	ug/l #	43
38) Carbon Tetrachloride	7.979	117	4752	6.09	ug/l #	12
55) 1,1,2-Trichloroethane	10.767	97	1179	2.75	ug/l #	18
59) 2-Hexanone	10.949	43	1423	8.06	ug/l #	19
67) Ethyl Benzene	11.749	91	14413	4.37	ug/l	92
68) m/p-Xylenes	11.849	106	27887	22.25	ug/l	94
69) o-Xylene	12.179	106	26339	22.81	ug/l	96
71) Bromoform	12.632	173	485	1.49	ug/l #	28
73) Isopropylbenzene	12.479	105	18948	4.91	ug/l	100
74) N-amyl acetate	12.267	43	15276	23.26	ug/l #	58
75) 1,1,2,2-Tetrachloroethane	12.667	83	3941	5.94	ug/l #	26
76) 1,2,3-Trichloropropane	12.885	75	1813	3.93	ug/l #	100
78) n-propylbenzene	12.820	91	83784	18.19	ug/l	100
79) 2-Chlorotoluene	12.885	91	29499	11.54	ug/l #	39
80) 1,3,5-Trimethylbenzene	12.961	105	203248	64.32	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.632	75	21682	109.65	ug/l #	14
82) 4-Chlorotoluene	12.955	91	20960	7.79	ug/l #	42
83) tert-Butylbenzene	13.267	119	87464	32.51	ug/l #	70
84) 1,2,4-Trimethylbenzene	13.267	105	683184	215.89	ug/l	97
85) sec-Butylbenzene	13.396	105	79017	20.79	ug/l	84
86) p-Isopropyltoluene	13.514	119	73122	21.20	ug/l	98
89) n-Butylbenzene	13.838	91	135088	40.60	ug/l #	76
90) Hexachloroethane	14.114	117	48463	70.68	ug/l #	10
92) 1,2-Dibromo-3-Chloropr...	14.520	75	2145	18.35	ug/l #	25
93) 1,2,4-Trichlorobenzene	15.149	180	1933	1.72	ug/l #	1
95) Naphthalene	15.396	128	171279	84.03	ug/l #	93
96) 1,2,3-Trichlorobenzene	15.614	180	3863	3.96	ug/l #	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030221\
Data File : VD068500.D
Acq On : 02 Mar 2021 17:06
Operator : VA/SY
Sample : M1540-01
Misc : 6.60G/5.00ml/MSVOA_D/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221


Quant Time: Mar 02 23:59:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
Quant Title : SW846 8260
QLast Update : Fri Feb 26 14:04:14 2021
Response via : Initial Calibration

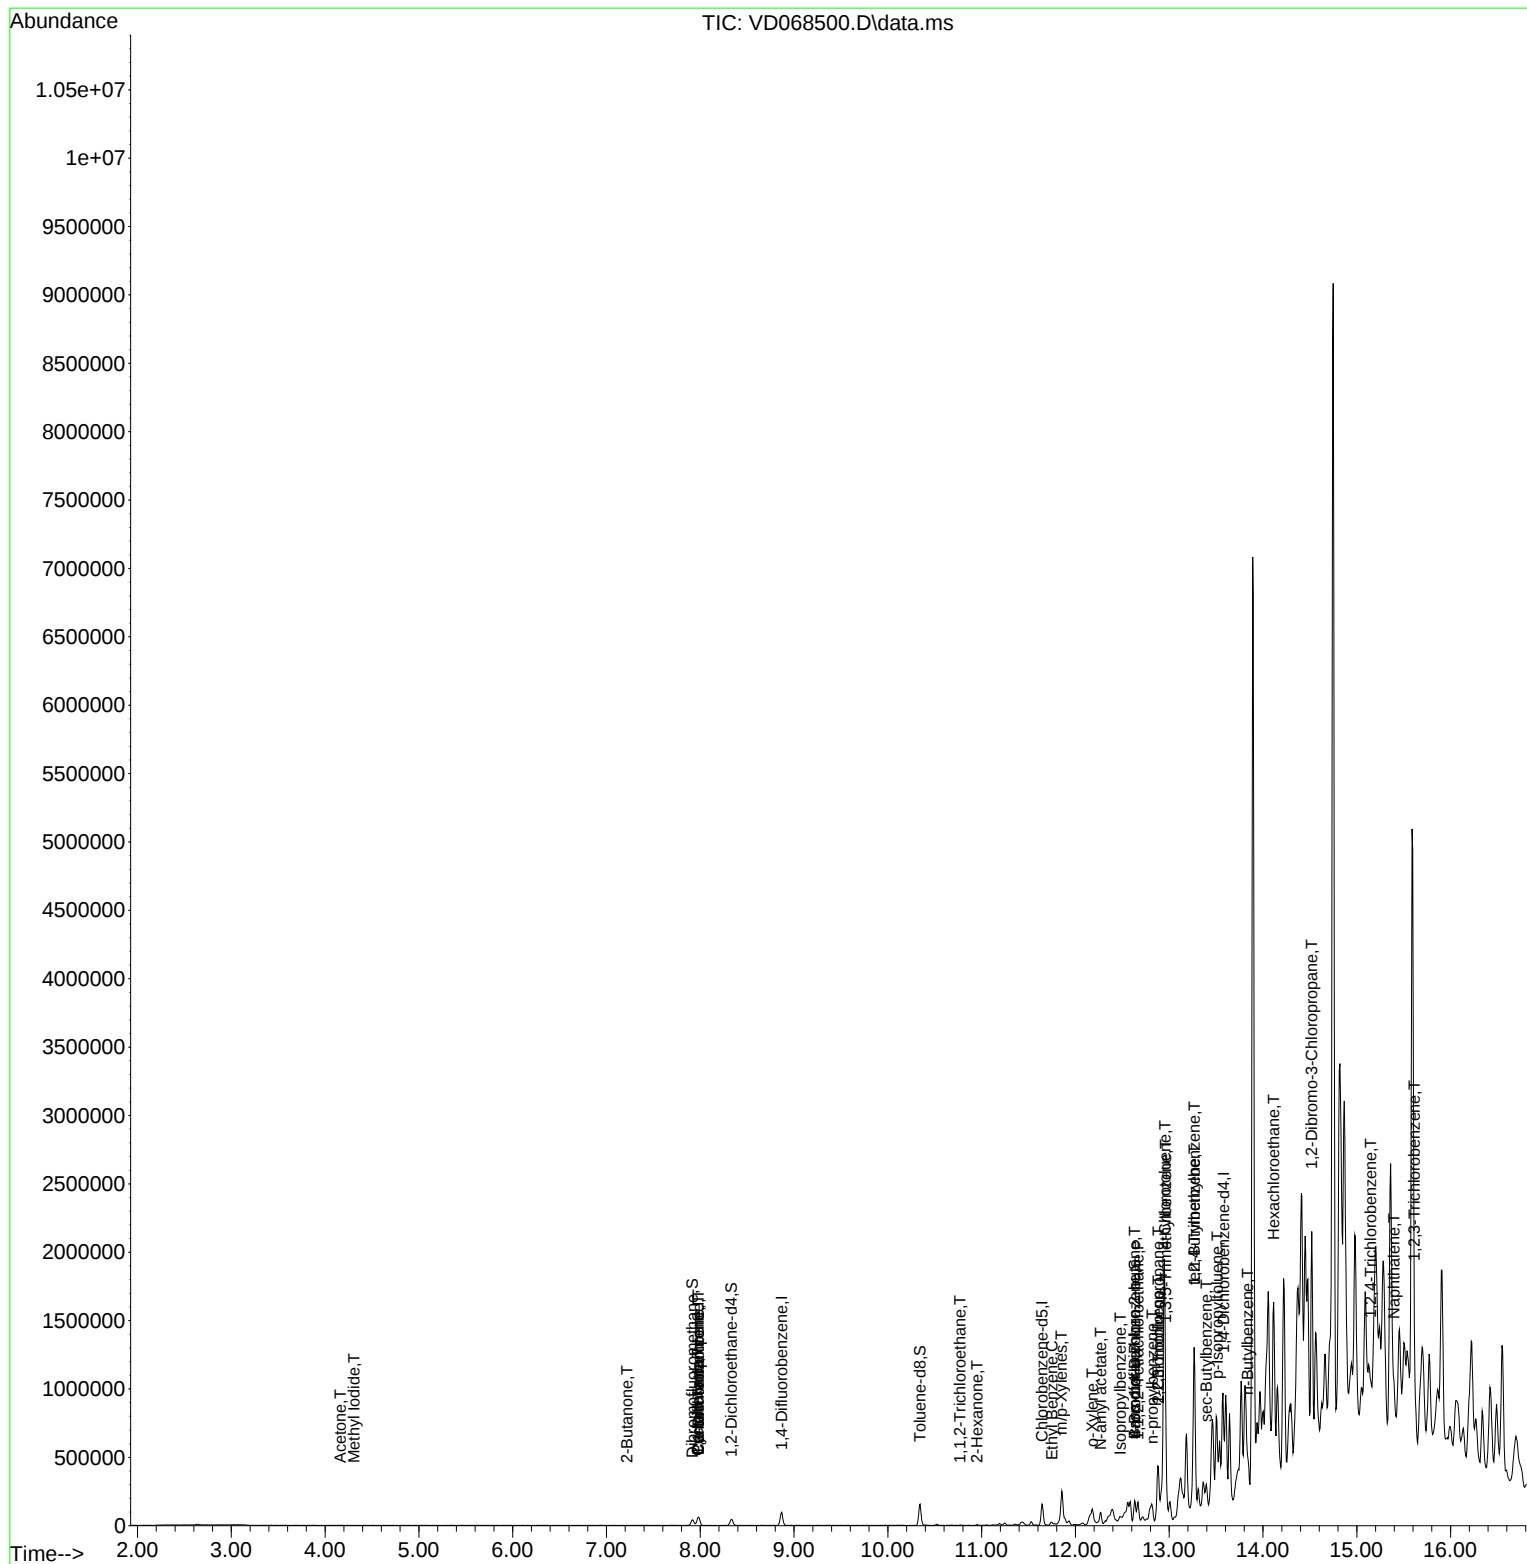



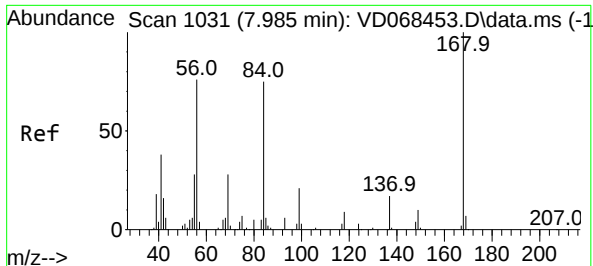


#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221



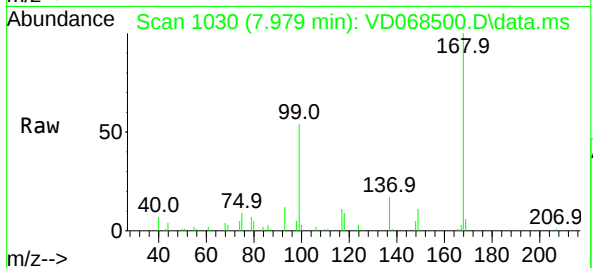



Tgt Ion:168 Resp: 47521
Ion Ratio Lower Upper
168 100
99 54.1 43.5 65.3

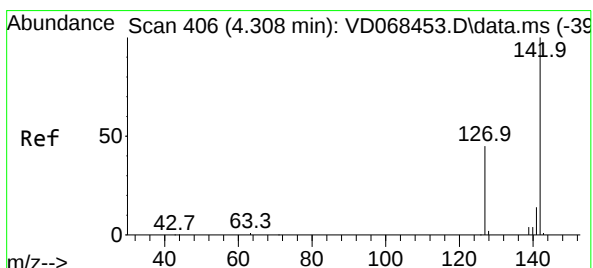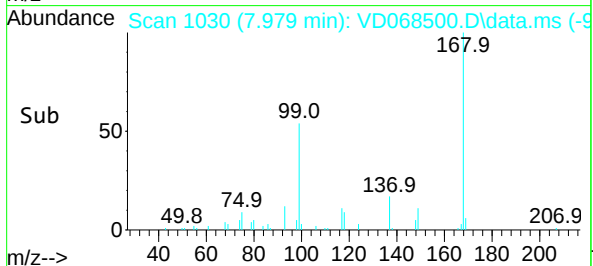

#10
Methyl Iodide
Concen: 2.72 ug/l
RT: 4.309 min Scan# 406
Delta R.T. 0.001 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion:142 Resp: 64
Ion Ratio Lower Upper
142 100
127 0.0 37.9 56.9#
141 0.0 11.5 17.3#


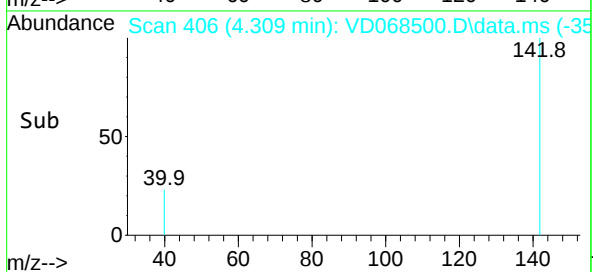

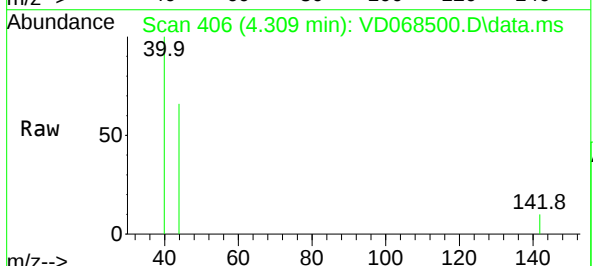




#16
Acetone
Concen: 11.99 ug/l
RT: 4.162 min Scan# 381
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06




Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221


Tgt Ion: 43 Resp: 904
Ion Ratio Lower Upper
43 100
58 0.0 24.2 36.4#

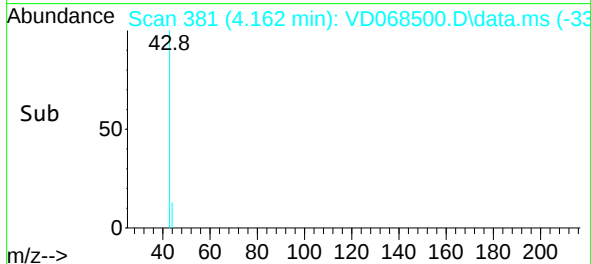

#20
Methylene Chloride
Concen: Below Cal
RT: 4.973 min Scan# 519
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06


Tgt Ion: 84 Resp: 165
Ion Ratio Lower Upper
84 100
49 0.0 77.4 116.2#
51 0.0 26.1 39.1#
86 0.0 51.8 77.8#

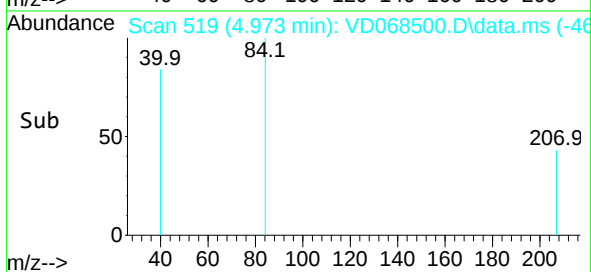






#25
2-Butanone
Concen: 1.09 ug/l
RT: 7.220 min Scan# 901
Delta R.T. 0.006 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Instrument :
MSVOA_D
ClientSampled :
PR-01-030221







Tgt Ion: 43 Resp: 118
Ion Ratio Lower Upper
43 100
72 0.0 25.1 37.7#

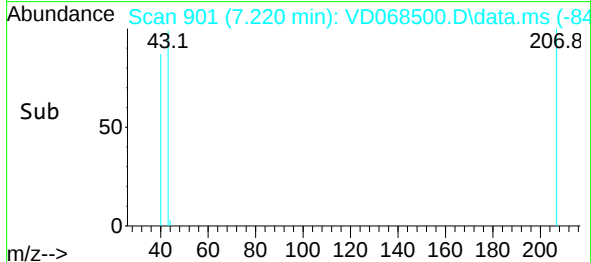

#31
Cyclohexane
Concen: 1.08 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. -0.017 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion: 56 Resp: 936
Ion Ratio Lower Upper
56 100
69 68.2 30.1 45.1#
84 98.7 82.1 123.1


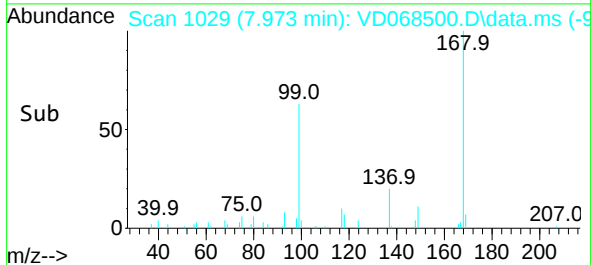

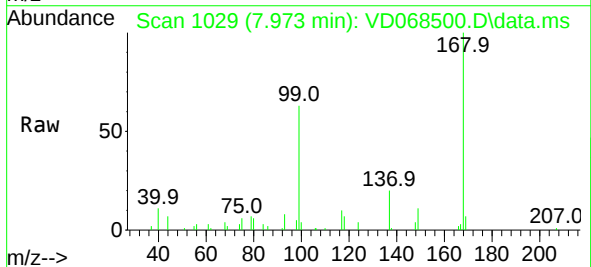


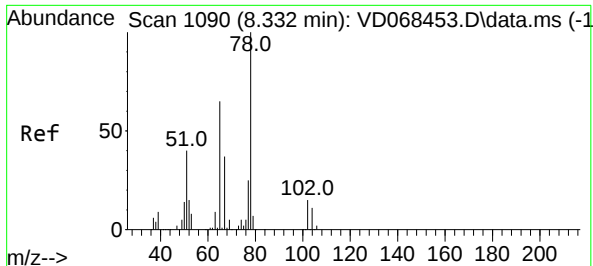

#33
1,2-Dichloroethane-d4
Concen: 79.51 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06




Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221


Tgt Ion: 65 Resp: 37750
Ion Ratio Lower Upper
65 100
67 49.0 0.0 105.0

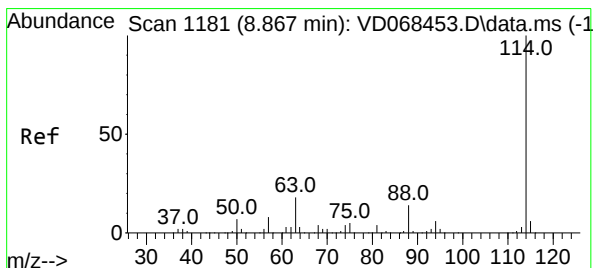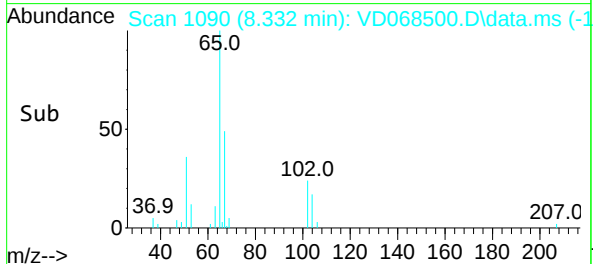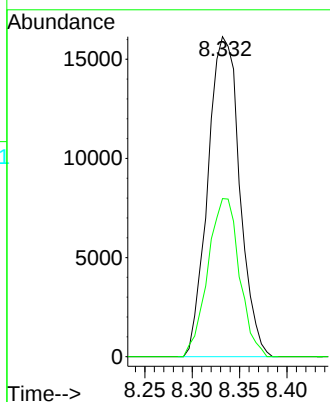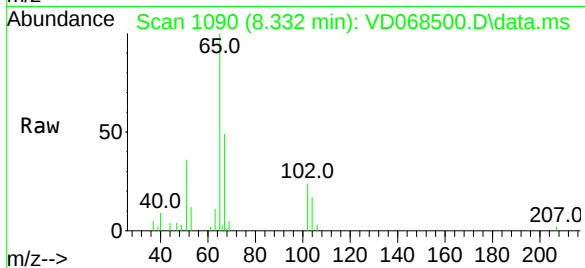

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion: 114 Resp: 87333
Ion Ratio Lower Upper
114 100
63 20.0 0.0 34.8
88 12.7 0.0 31.6

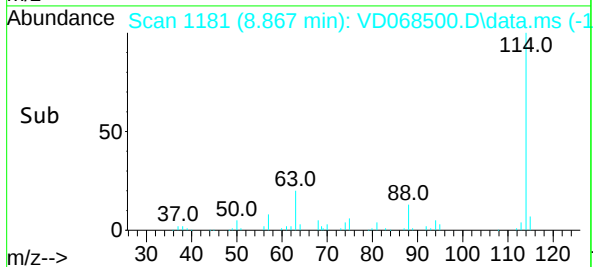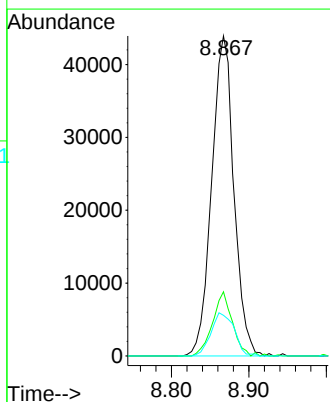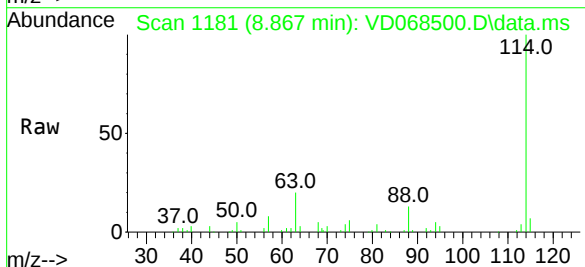

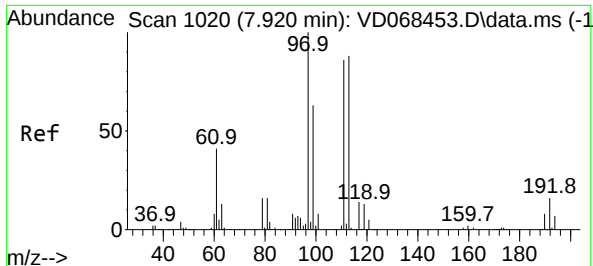

#35

Dibromofluoromethane

Concen: 57.55 ug/l

RT: 7.914 min Scan# 1019

Delta R.T. -0.006 min

Lab File: VD068500.D

Acq: 02 Mar 2021 17:06





Tgt Ion:113 Resp: 30277

Ion Ratio Lower Upper

113 100

111 95.6 81.4 122.0

192 19.7 16.1 24.1

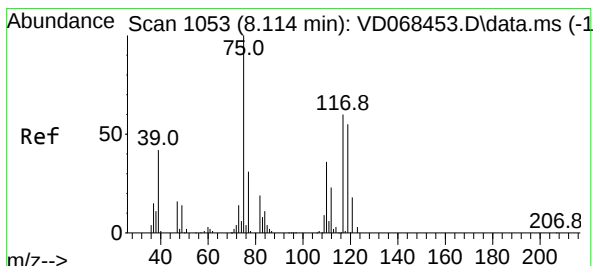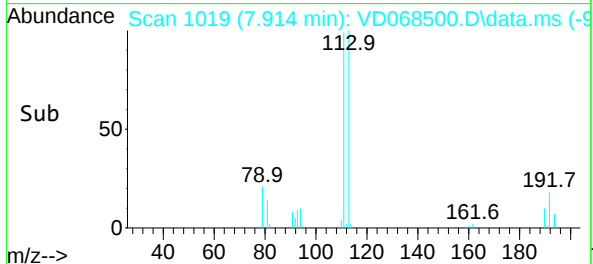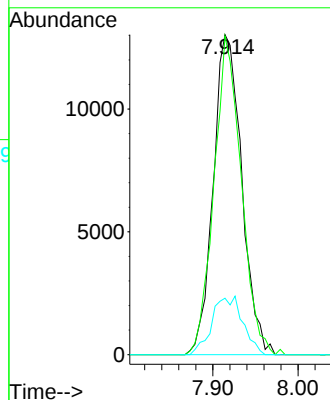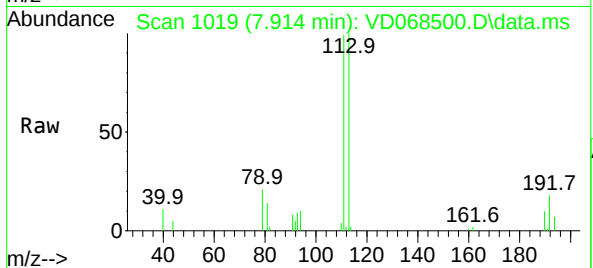

#36

1,1-Dichloropropene

Concen: 4.28 ug/l

RT: 7.979 min Scan# 1030

Delta R.T. -0.135 min

Lab File: VD068500.D

Acq: 02 Mar 2021 17:06




Tgt Ion: 75 Resp: 3553


Ion Ratio Lower Upper

75 100

110 4.2 19.4 58.2#


77 0.0 25.3 37.9#

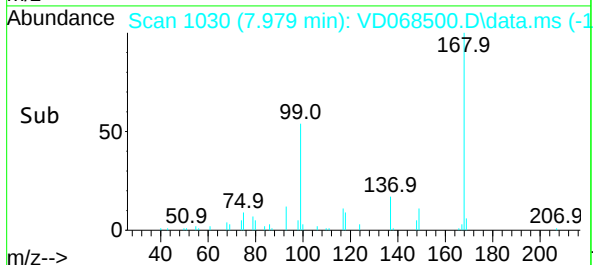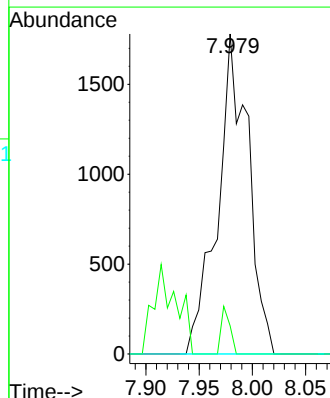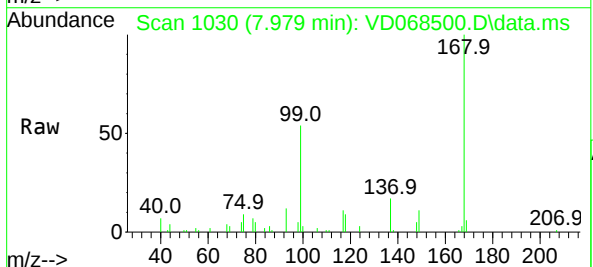






#38
Carbon Tetrachloride
Concen: 6.09 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.117 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06


Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221





Tgt Ion:117 Resp: 4752
Ion Ratio Lower Upper
117 100
119 0.0 77.3 115.9#
121 0.0 24.7 37.1#




#50
Toluene-d8
Concen: 50.25 ug/l
RT: 10.344 min Scan# 1432
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06




Tgt Ion: 98 Resp: 105297
Ion Ratio Lower Upper
98 100
100 66.2 53.0 79.4

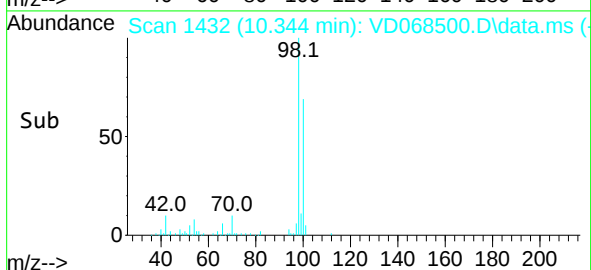






#55
1,1,2-Trichloroethane
Concen: 2.75 ug/l
RT: 10.767 min Scan# 1504
Delta R.T. -0.035 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221



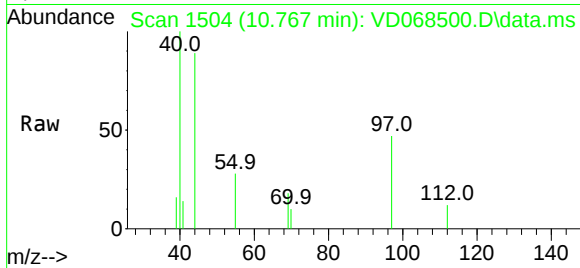



Tgt Ion	Ratio	Lower	Upper
97	100		
83	0.0	61.8	92.6#
85	0.0	42.2	63.2#
99	0.0	48.3	72.5#

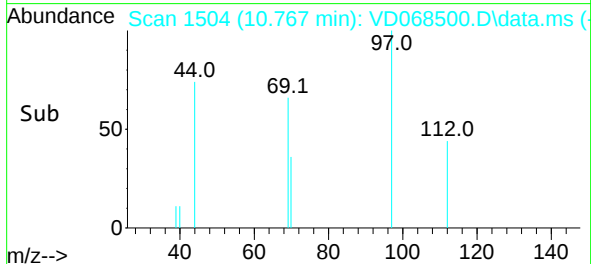

#59
2-Hexanone
Concen: 8.06 ug/l
RT: 10.949 min Scan# 1535
Delta R.T. -0.035 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion	Ratio	Lower	Upper
43	100		
58	0.0	31.0	93.0#


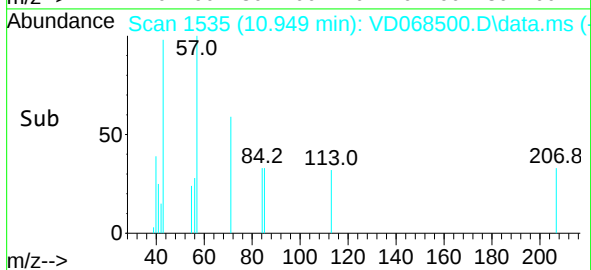

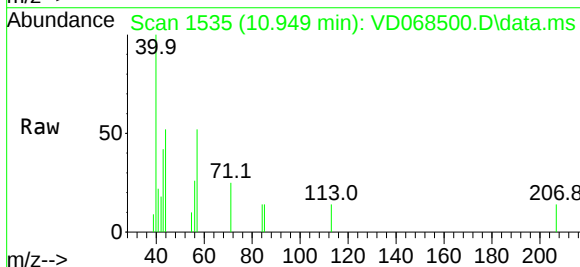


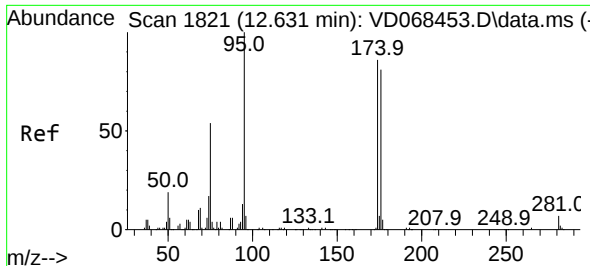

#62
4-Bromofluorobenzene
Concen: 66.94 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06




Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221


Tgt Ion:	95	Resp:	45206
Ion Ratio	Lower	Upper	
95	100		
174	85.1	0.0	172.4
176	81.3	0.0	168.4

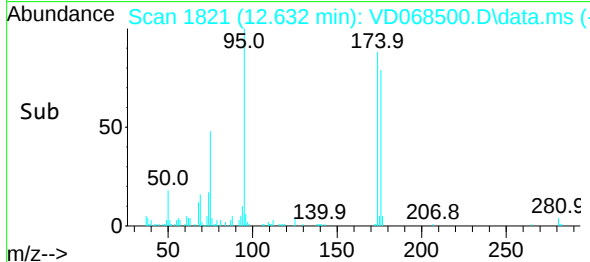

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion:	117	Resp:	90796
Ion Ratio	Lower	Upper	
117	100		
82	54.2	41.4	62.0
119	30.3	26.1	39.1


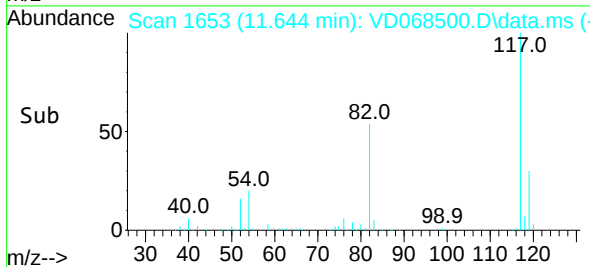

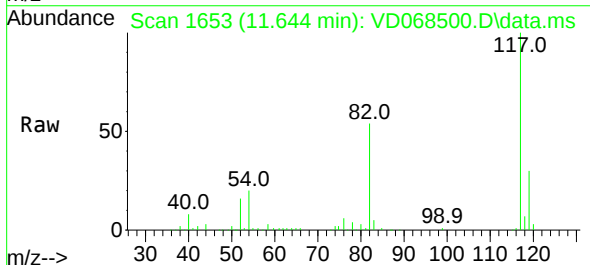


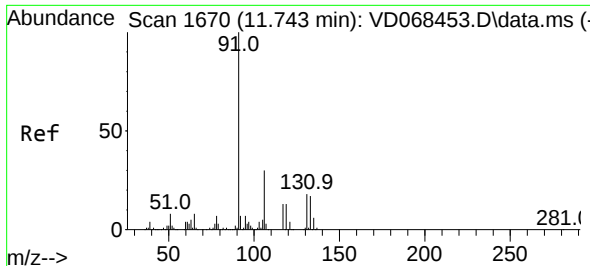

#67
Ethyl Benzene
Concen: 4.37 ug/l
RT: 11.749 min Scan# 1671
Delta R.T. 0.006 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06




Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221


Tgt Ion: 91 Resp: 14413
Ion Ratio Lower Upper
91 100
106 37.1 25.9 38.9

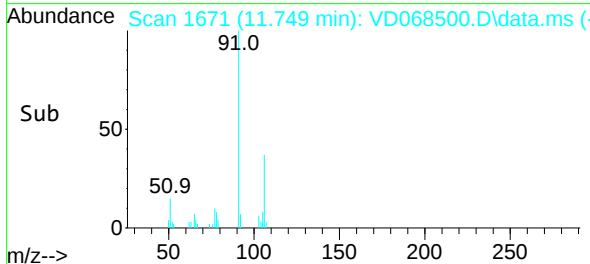

#68
m/p-Xylenes
Concen: 22.25 ug/l
RT: 11.849 min Scan# 1688
Delta R.T. -0.006 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion:106 Resp: 27887
Ion Ratio Lower Upper
106 100
91 208.3 159.1 238.7


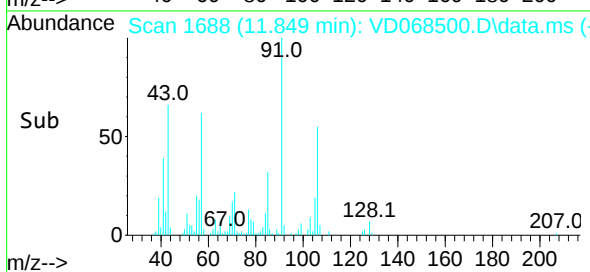

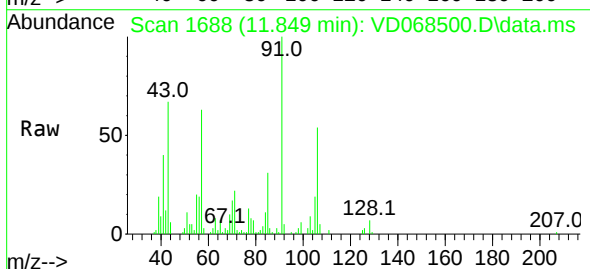




#69
o-Xylene
Concen: 22.81 ug/l
RT: 12.179 min Scan# 1744
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06




Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221


Tgt Ion:106 Resp: 26339
Ion Ratio Lower Upper
106 100
91 211.0 108.7 325.9

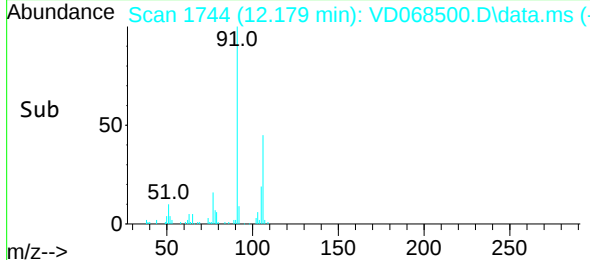

#71
Bromoform
Concen: 1.49 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.271 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion:173 Resp: 485
Ion Ratio Lower Upper
173 100
175 0.0 24.6 73.8#
254 0.0 0.0 0.0


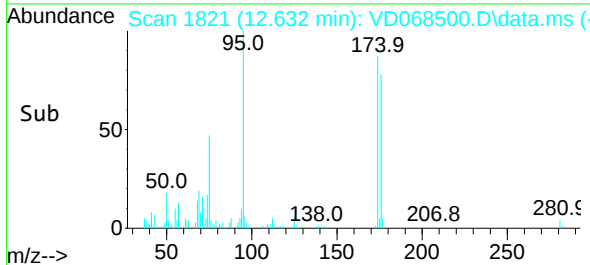

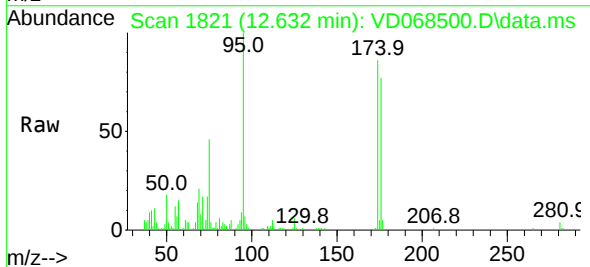


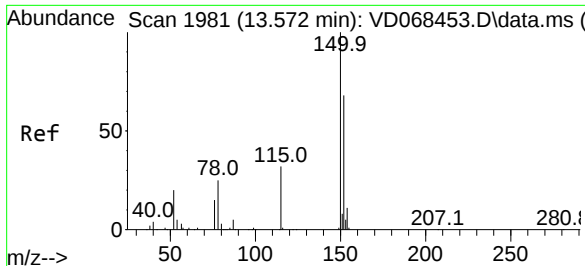

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.579 min Scan# 1982
Delta R.T. 0.007 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06




Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221


Tgt Ion:152 Resp: 51981
Ion Ratio Lower Upper
152 100
115 55.9 28.9 86.8
150 152.9 0.0 344.4

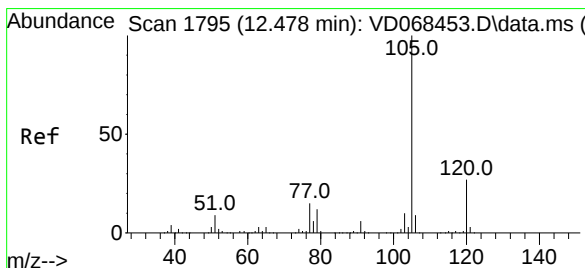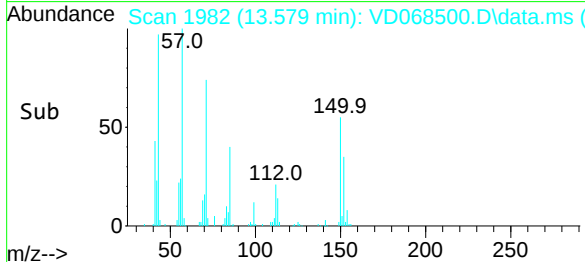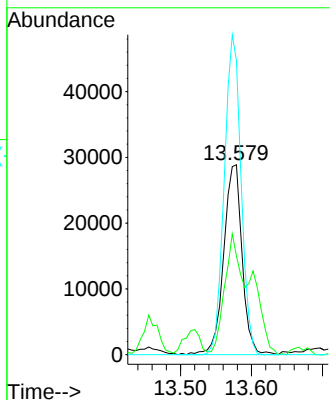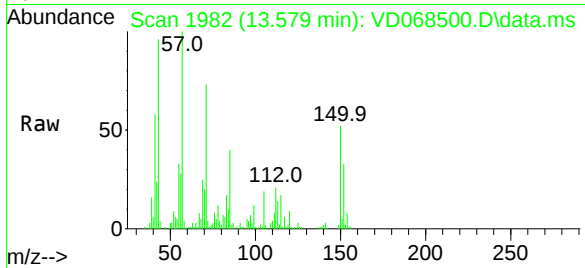

#73
Isopropylbenzene
Concen: 4.91 ug/l
RT: 12.479 min Scan# 1795
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06


Tgt Ion:105 Resp: 18948
Ion Ratio Lower Upper
105 100
120 26.2 13.2 39.6

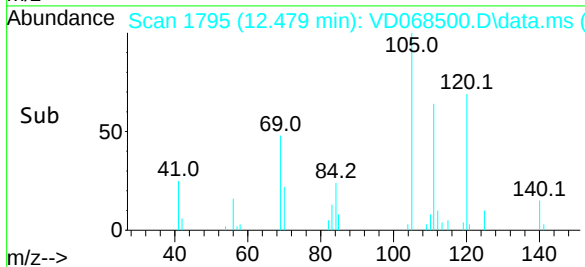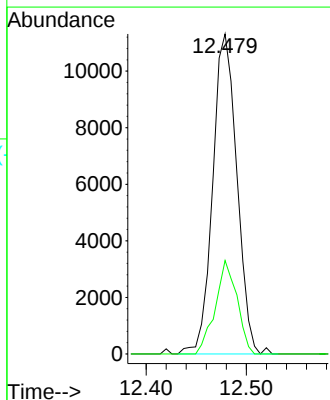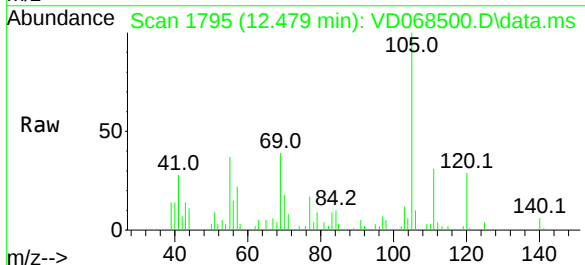






#74
N-amy1 acetate
Concen: 23.26 ug/l
RT: 12.267 min Scan# 1759
Delta R.T. -0.023 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221



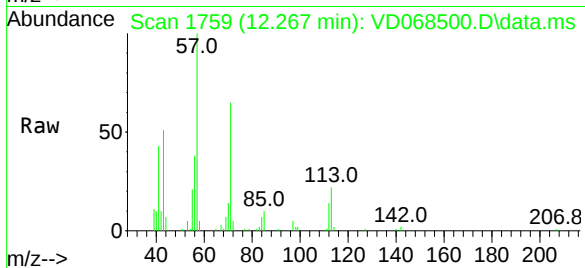



Tgt Ion:	43	Resp:	15276
Ion Ratio	100	Lower	Upper
70	20.4	41.8	62.8#
55	45.7	24.2	36.4#
61	0.0	21.7	32.5#

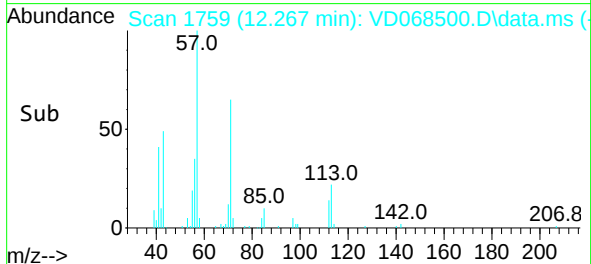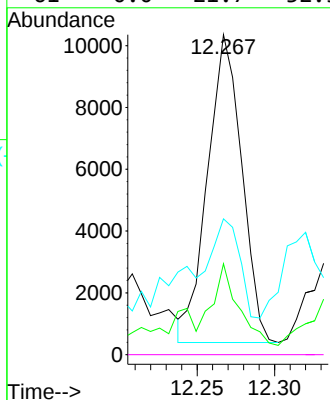

#75
1,1,2,2-Tetrachloroethane
Concen: 5.94 ug/l
RT: 12.667 min Scan# 1827
Delta R.T. -0.064 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06


Tgt Ion:	83	Resp:	3941
Ion Ratio	100	Lower	Upper
131	0.0	5.8	17.4#
85	0.0	32.4	97.2#

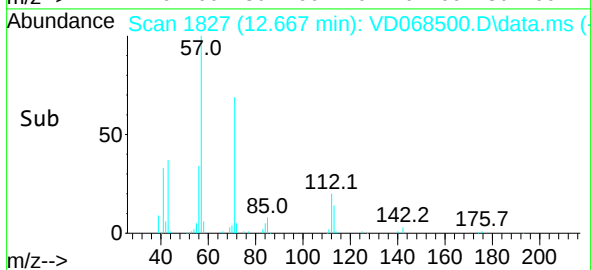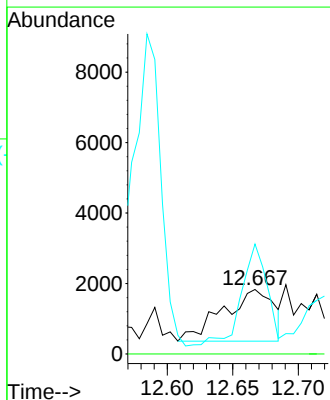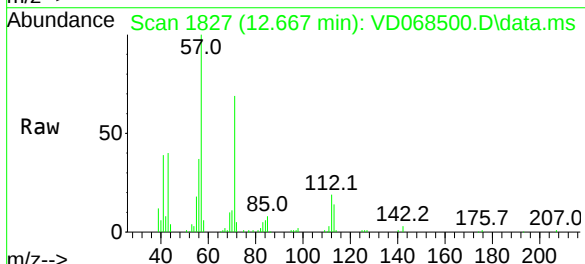



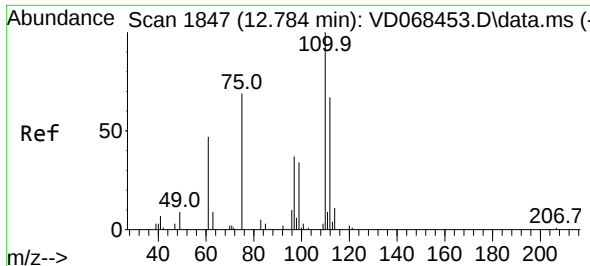


#76
1,2,3-Trichloropropane
Concen: 3.93 ug/l
RT: 12.885 min Scan# 1864
Delta R.T. 0.101 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221







Tgt Ion: 75 Resp: 1813
Ion Ratio Lower Upper
75 100
77 1592.8 0.0 0.0#

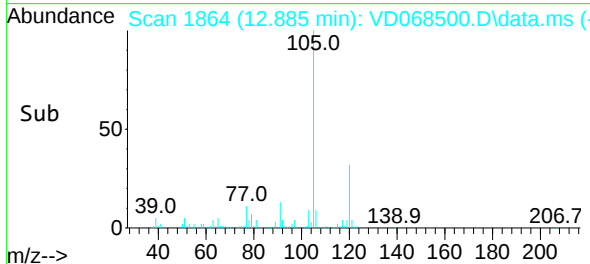

#78
n-propylbenzene
Concen: 18.19 ug/l
RT: 12.820 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion: 91 Resp: 83784
Ion Ratio Lower Upper
91 100
120 24.1 12.0 36.0


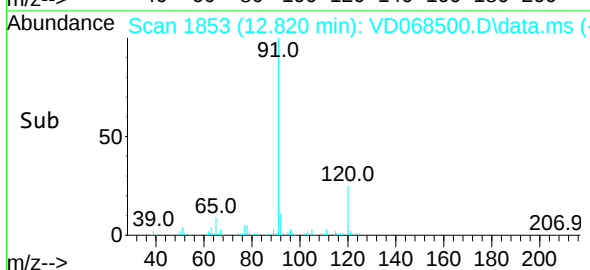

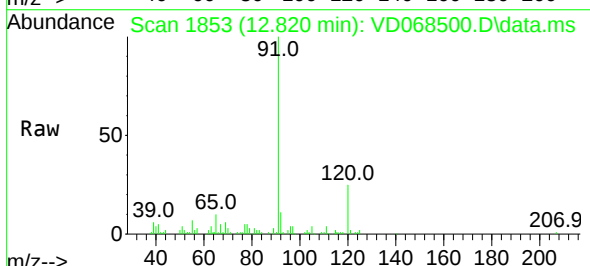




#79
2-Chlorotoluene
Concen: 11.54 ug/l
RT: 12.885 min Scan# 1864
Delta R.T. -0.023 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06




Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221


Tgt Ion: 91 Resp: 29499
Ion Ratio Lower Upper
91 100
126 0.0 17.8 53.5#

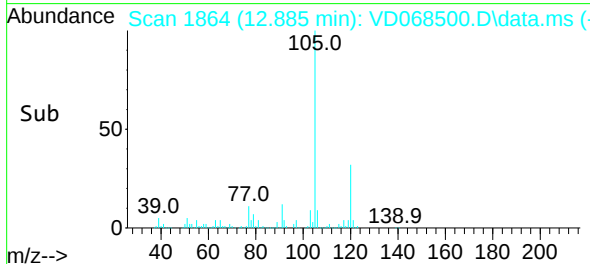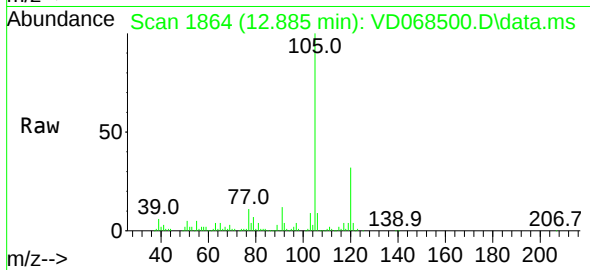

#80
1,3,5-Trimethylbenzene
Concen: 64.32 ug/l
RT: 12.961 min Scan# 1877
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion:105 Resp: 203248
Ion Ratio Lower Upper
105 100
120 48.2 24.2 72.6




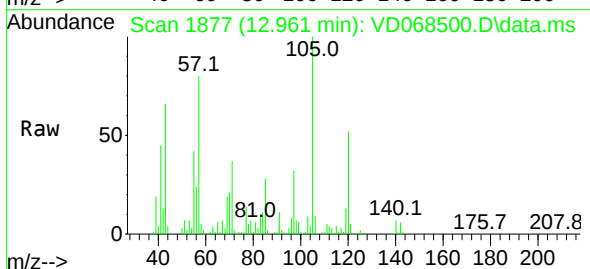




#81
trans-1,4-Dichloro-2-butene
Concen: 109.65 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.106 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06




Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221


Tgt Ion: 75 Resp: 21682
Ion Ratio Lower Upper
75 100
53 0.8 70.2 105.2#
89 0.0 40.3 60.5#

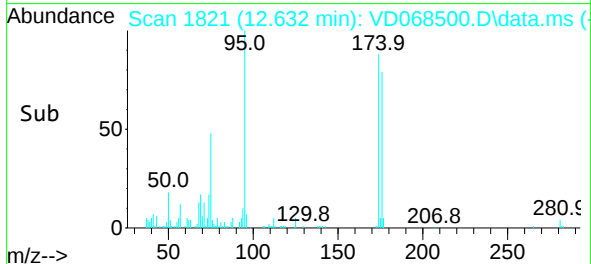

#82
4-Chlorotoluene
Concen: 7.79 ug/l
RT: 12.955 min Scan# 1876
Delta R.T. -0.047 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion: 91 Resp: 20960
Ion Ratio Lower Upper
91 100
126 1.5 17.7 53.1#


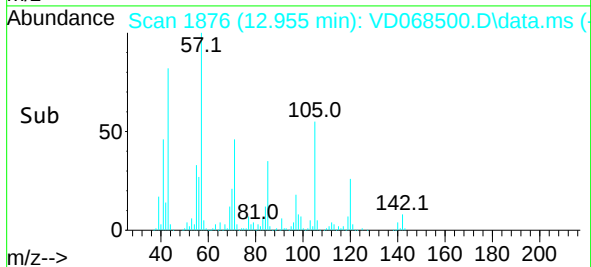

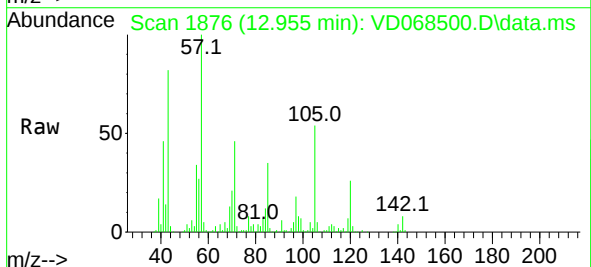


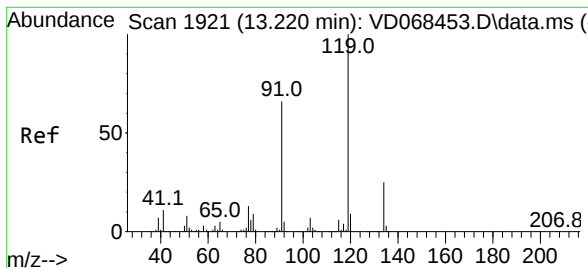

#83
tert-Butylbenzene
Concen: 32.51 ug/l
RT: 13.267 min Scan# 1929
Delta R.T. 0.047 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06




Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221


Tgt Ion:119 Resp: 87464
Ion Ratio Lower Upper
119 100
91 77.9 31.1 93.5
134 0.0 13.3 39.8#

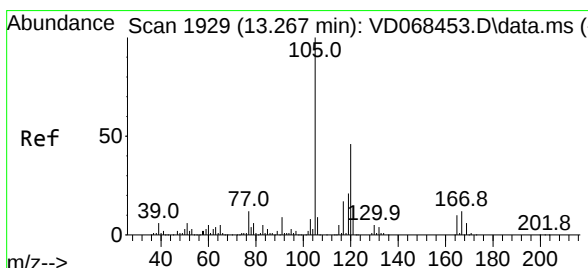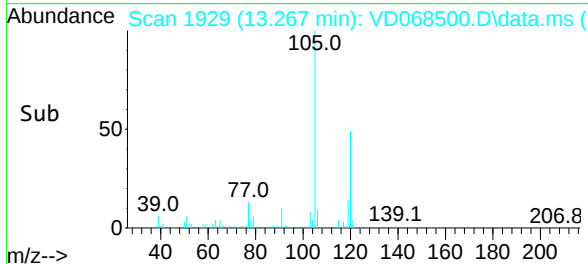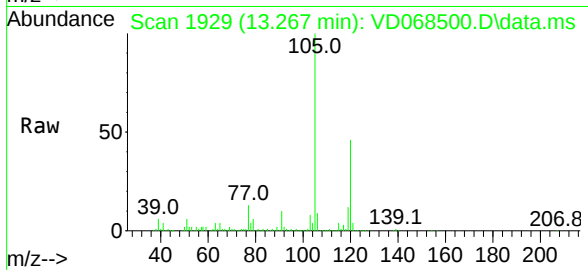

#84
1,2,4-Trimethylbenzene
Concen: 215.89 ug/l
RT: 13.267 min Scan# 1929
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion:105 Resp: 683184
Ion Ratio Lower Upper
105 100
120 46.4 22.4 67.0


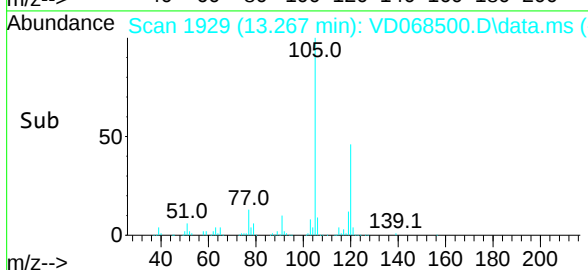

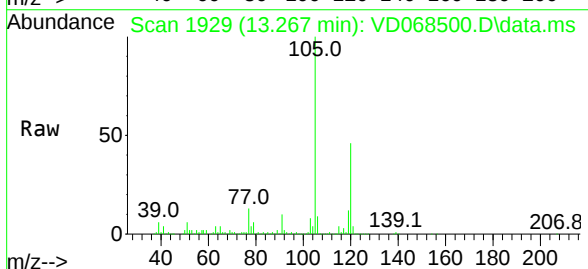




#85
 sec-Butylbenzene
 Concen: 20.79 ug/l
 RT: 13.396 min Scan# 1951
 Delta R.T. 0.000 min
 Lab File: VD068500.D
 Acq: 02 Mar 2021 17:06




Instrument :
 MSVOA_D
 ClientSampleId :
 PR-01-030221


Tgt Ion:105 Resp: 79017
 Ion Ratio Lower Upper
 105 100
 134 28.0 10.3 30.9

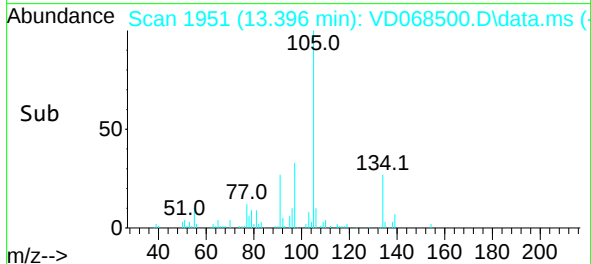

#86
 p-Isopropyltoluene
 Concen: 21.20 ug/l
 RT: 13.514 min Scan# 1971
 Delta R.T. 0.000 min
 Lab File: VD068500.D
 Acq: 02 Mar 2021 17:06

Tgt Ion:119 Resp: 73122
 Ion Ratio Lower Upper
 119 100
 134 26.4 12.9 38.7
 91 22.4 11.7 35.0


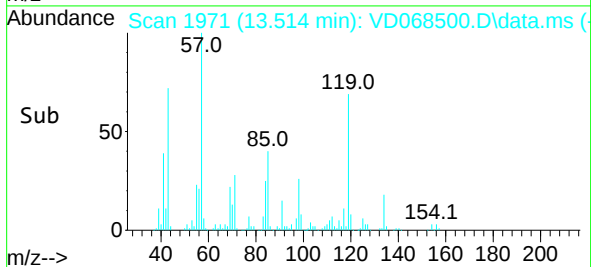

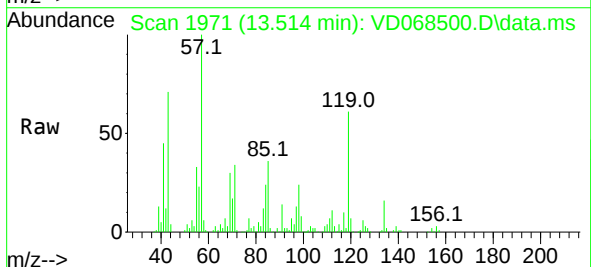




#89
n-Butylbenzene
Concen: 40.60 ug/l
RT: 13.838 min Scan# 2026
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06




Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221


Tgt Ion: 91 Resp: 135088
Ion Ratio Lower Upper
91 100
92 61.2 27.2 81.6
134 0.0 13.9 41.7#

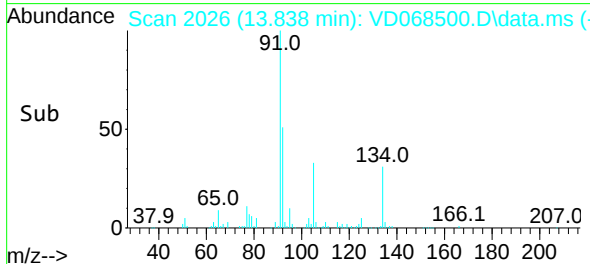

#90
Hexachloroethane
Concen: 70.68 ug/l
RT: 14.114 min Scan# 2073
Delta R.T. 0.006 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion: 117 Resp: 48463
Ion Ratio Lower Upper
117 100
201 0.0 39.5 118.5#


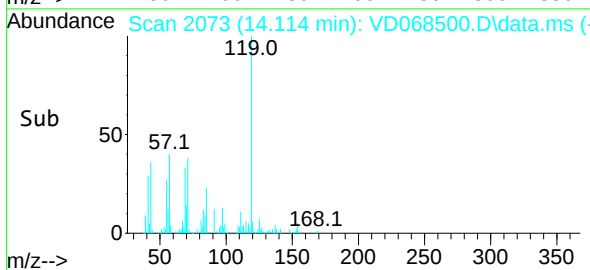

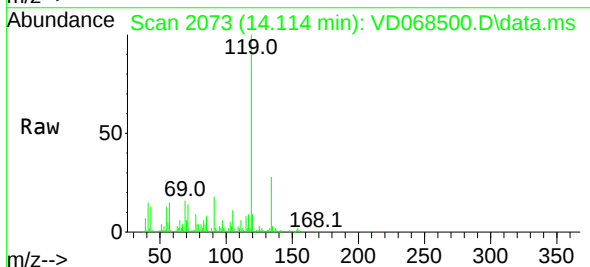


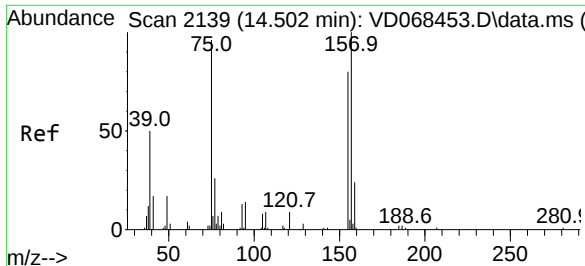

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 18.35 ug/l
 RT: 14.520 min Scan# 2142
 Delta R.T. 0.018 min
 Lab File: VD068500.D
 Acq: 02 Mar 2021 17:06




Instrument :
 MSVOA_D
 ClientSampleId :
 PR-01-030221


Tgt Ion: 75 Resp: 2145
 Ion Ratio Lower Upper
 75 100
 155 120.7 48.0 144.2
 157 0.0 65.0 194.8#

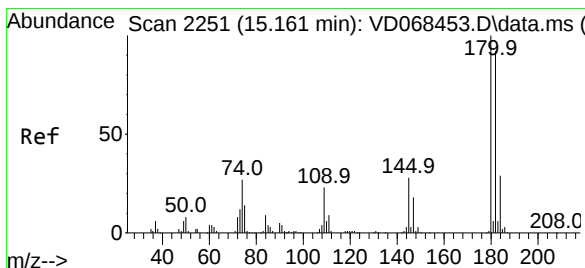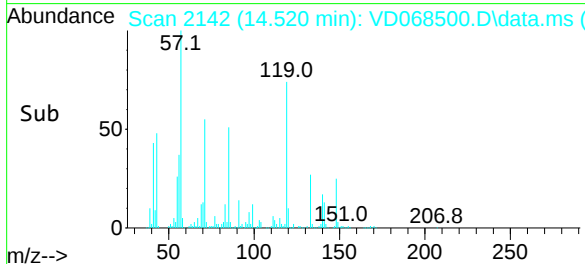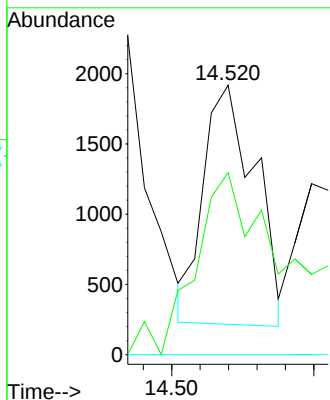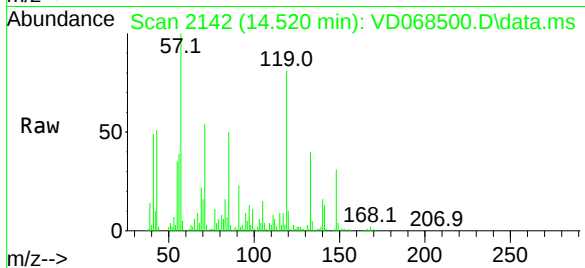

#93
 1,2,4-Trichlorobenzene
 Concen: 1.72 ug/l
 RT: 15.149 min Scan# 2249
 Delta R.T. -0.011 min
 Lab File: VD068500.D
 Acq: 02 Mar 2021 17:06

Tgt Ion: 180 Resp: 1933
 Ion Ratio Lower Upper
 180 100
 182 289.1 46.8 140.4#
 145 5310.6 15.2 45.5#


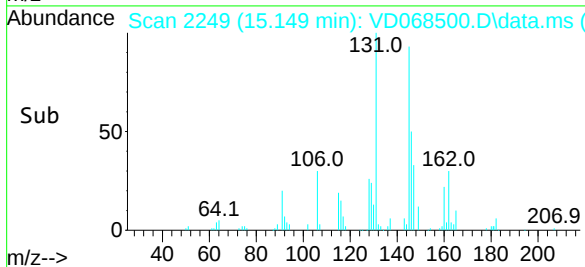
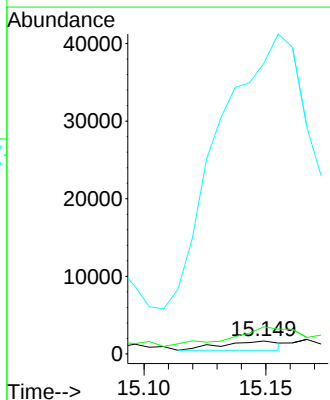
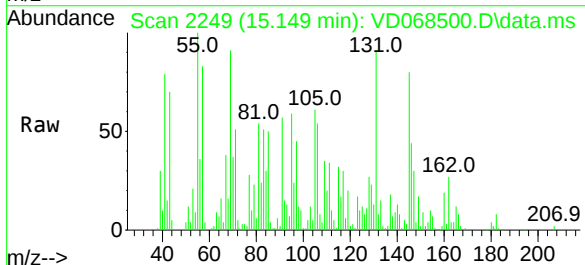


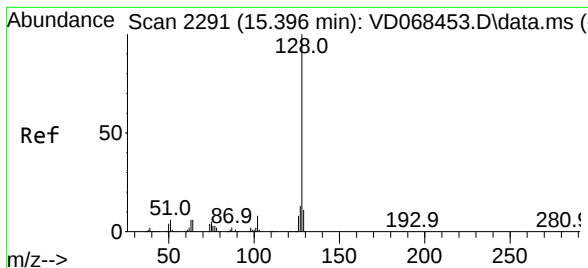

#95
Naphthalene
Concen: 84.03 ug/l
RT: 15.396 min Scan# 2291
Delta R.T. 0.000 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Instrument :
MSVOA_D
ClientSampleId :
PR-01-030221

Tgt Ion:128 Resp: 171279
Ion Ratio Lower Upper
128 100
127 9.8 10.2 15.2#
129 8.7 8.8 13.2#

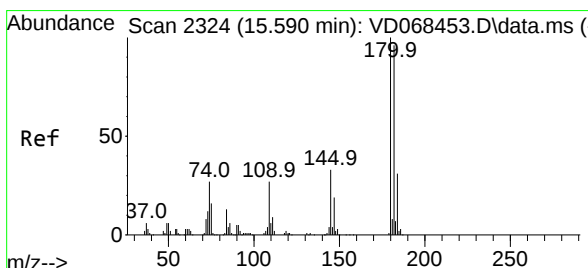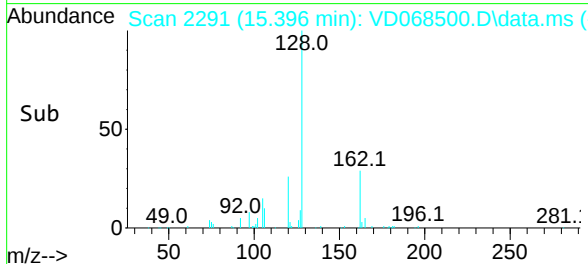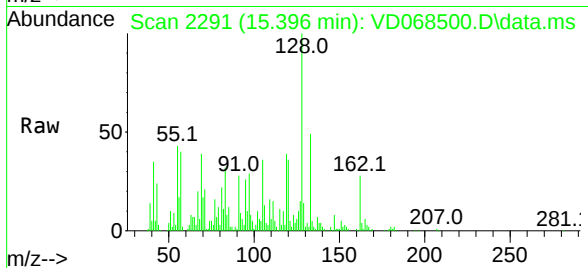

#96
1,2,3-Trichlorobenzene
Concen: 3.96 ug/l
RT: 15.614 min Scan# 2328
Delta R.T. 0.024 min
Lab File: VD068500.D
Acq: 02 Mar 2021 17:06

Tgt Ion:180 Resp: 3863
Ion Ratio Lower Upper
180 100
182 63.9 48.3 144.8
145 0.0 16.7 50.1#

