

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030223\
 Data File : VD075436.D
 Acq On : 02 Mar 2023 11:32
 Operator : KP/SY
 Sample : VD0302SBL03
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK105

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Title : SFAM01.0

Signal : TIC: VD075436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.734	14	25	41	rBV	673800	1419605	100.00%	16.913%
2	2.281	112	118	125	rBV	159711	238952	16.83%	2.847%
3	2.805	201	207	216	rVB	125805	238238	16.78%	2.838%
4	3.381	302	305	306	rBV2	971	708	0.05%	0.008%
5	3.517	326	328	330	rBV2	707	751	0.05%	0.009%
6	3.534	330	331	333	rVB	828	458	0.03%	0.005%
7	3.740	363	366	368	rVB2	869	860	0.06%	0.010%
8	3.834	381	382	385	rVB	677	515	0.04%	0.006%
9	3.922	387	397	409	rBV	128181	329354	23.20%	3.924%
10	4.087	423	425	426	rVB	1057	444	0.03%	0.005%
11	4.275	455	457	459	rBV	709	628	0.04%	0.007%
12	4.340	464	468	469	rBV2	813	915	0.06%	0.011%
13	4.364	470	472	473	rVB	1176	592	0.04%	0.007%
14	4.799	539	546	547	rBV	7803	10423	0.73%	0.124%
15	4.934	566	569	571	rBV2	945	1229	0.09%	0.015%
16	5.046	586	588	590	rVB	836	531	0.04%	0.006%
17	5.252	621	623	625	rBV2	766	632	0.04%	0.008%
18	5.305	628	632	633	rBV	605	604	0.04%	0.007%
19	5.405	646	649	650	rBV2	689	737	0.05%	0.009%
20	5.534	669	671	674	rBV2	594	568	0.04%	0.007%
21	5.611	682	684	685	rBV	1016	518	0.04%	0.006%
22	5.628	685	687	689	rVB2	775	557	0.04%	0.007%
23	5.658	689	692	693	rBV2	601	582	0.04%	0.007%
24	5.828	717	721	722	rBV3	2174	2656	0.19%	0.032%
25	5.922	734	737	739	rBV2	1020	1095	0.08%	0.013%
26	6.016	751	753	755	rBV	985	917	0.06%	0.011%
27	6.052	758	759	761	rVV	883	675	0.05%	0.008%
28	6.075	761	763	766	rVV2	802	889	0.06%	0.011%
29	6.252	789	793	794	rBV	593	671	0.05%	0.008%
30	6.458	826	828	829	rBV	702	432	0.03%	0.005%
31	6.528	837	840	842	rVB	593	550	0.04%	0.007%
32	6.552	842	844	851	rBV3	834	1359	0.10%	0.016%
33	6.993	911	919	925	rBV	17309	46262	3.26%	0.551%
34	7.240	957	961	962	rBV	653	712	0.05%	0.008%
35	7.334	975	977	979	rBV2	635	534	0.04%	0.006%
36	7.422	989	992	995	rBV	649	956	0.07%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030223\
 Data File : VD075436.D
 Acq On : 02 Mar 2023 11:32
 Operator : KP/SY
 Sample : VD0302SBL03
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK105

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Title : SFAM01.0

37	7.569	1008	1017	1028	rBV	156215	392349	27.64%	4.674%
38	7.793	1053	1055	1057	rBV2	775	543	0.04%	0.006%
39	7.881	1066	1070	1071	rBV3	1469	1452	0.10%	0.017%
40	8.040	1096	1097	1100	rBV	688	744	0.05%	0.009%
41	8.205	1115	1125	1142	rBV2	344198	977968	68.89%	11.652%
42	8.528	1176	1180	1184	rBV2	870	1619	0.11%	0.019%
43	8.781	1214	1223	1233	rBV	318454	641950	45.22%	7.648%
44	9.010	1258	1262	1263	rBV2	1548	1427	0.10%	0.017%
45	9.216	1289	1297	1306	rBV	195521	411470	28.98%	4.902%
46	9.363	1320	1322	1325	rBV2	765	871	0.06%	0.010%
47	9.410	1328	1330	1332	rVB2	937	762	0.05%	0.009%
48	9.434	1332	1334	1336	rBV2	651	507	0.04%	0.006%
49	9.652	1369	1371	1374	rBV2	801	695	0.05%	0.008%
50	9.693	1376	1378	1380	rBV2	620	483	0.03%	0.006%
51	9.934	1417	1419	1420	rBV	851	815	0.06%	0.010%
52	9.981	1420	1427	1436	rVV	106182	194885	13.73%	2.322%
53	10.104	1446	1448	1451	rBV2	845	1023	0.07%	0.012%
54	10.275	1469	1477	1486	rBV	429904	790024	55.65%	9.412%
55	10.528	1514	1520	1531	rBV2	65755	115971	8.17%	1.382%
56	10.669	1536	1544	1553	rBV	42444	80212	5.65%	0.956%
57	10.810	1565	1568	1569	rBV2	1912	1452	0.10%	0.017%
58	10.881	1574	1580	1591	rBV	67389	116390	8.20%	1.387%
59	10.993	1598	1599	1600	rBV	1073	509	0.04%	0.006%
60	11.028	1600	1605	1613	rVB3	13881	24545	1.73%	0.292%
61	11.128	1621	1622	1629	rBV3	1311	1946	0.14%	0.023%
62	11.346	1657	1659	1660	rBV2	1122	739	0.05%	0.009%
63	11.410	1665	1670	1676	rVB2	9151	15424	1.09%	0.184%
64	11.587	1692	1700	1713	rVV	429402	736052	51.85%	8.769%
65	11.687	1714	1717	1722	rVB3	2395	3279	0.23%	0.039%
66	11.804	1731	1737	1741	rVB4	4450	7953	0.56%	0.095%
67	11.975	1764	1766	1767	rBV	628	498	0.04%	0.006%
68	11.987	1767	1768	1769	rVV	1287	547	0.04%	0.007%
69	12.234	1808	1810	1813	rBV2	1035	970	0.07%	0.012%
70	12.398	1836	1838	1839	rBV	865	593	0.04%	0.007%
71	12.434	1839	1844	1849	rVB5	4762	8896	0.63%	0.106%
72	12.581	1864	1869	1875	rVB3	19377	30753	2.17%	0.366%
73	12.657	1875	1882	1889	rBV	141050	242504	17.08%	2.889%
74	12.734	1894	1895	1896	rBV	1132	557	0.04%	0.007%
75	12.763	1897	1900	1904	rVV2	3414	4259	0.30%	0.051%
76	12.851	1913	1915	1919	rVB2	2738	2585	0.18%	0.031%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030223\
 Data File : VD075436.D
 Acq On : 02 Mar 2023 11:32
 Operator : KP/SY
 Sample : VD0302SBL03
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK105

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Title : SFAM01.0

77	12.881	1919	1920	1921	rBV	1030	522	0.04%	0.006%
78	12.904	1921	1924	1928	rVB4	3166	5044	0.36%	0.060%
79	12.981	1936	1937	1939	rBV	952	665	0.05%	0.008%
80	13.098	1956	1957	1959	rBV	989	589	0.04%	0.007%
81	13.175	1965	1970	1973	rBV3	2398	3772	0.27%	0.045%
82	13.210	1974	1976	1983	rVB4	3281	4792	0.34%	0.057%
83	13.310	1991	1993	1994	rVB	954	449	0.03%	0.005%
84	13.463	2014	2019	2023	rVV3	5684	9283	0.65%	0.111%
85	13.522	2023	2029	2038	rVB	391670	648132	45.66%	7.722%
86	13.816	2072	2079	2088	rBV	329322	563705	39.71%	6.716%
87	13.922	2095	2097	2100	rBV2	1097	1420	0.10%	0.017%
88	13.945	2100	2101	2102	rBV	1262	556	0.04%	0.007%
89	14.057	2114	2120	2126	rVV2	8514	14932	1.05%	0.178%
90	14.122	2129	2131	2132	rBV	887	595	0.04%	0.007%
91	14.445	2184	2186	2187	rBV2	977	693	0.05%	0.008%
92	14.487	2191	2193	2194	rBV	905	623	0.04%	0.007%
93	14.763	2238	2240	2247	rVB5	3216	4228	0.30%	0.050%
94	15.098	2295	2297	2303	rVB5	2995	4434	0.31%	0.053%
95	15.645	2389	2390	2392	rBV	1360	654	0.05%	0.008%
96	15.763	2409	2410	2414	rBV2	1075	833	0.06%	0.010%
97	16.016	2450	2453	2455	rBV2	1758	1744	0.12%	0.021%
98	16.269	2494	2496	2497	rBV	1122	669	0.05%	0.008%
99	16.310	2500	2503	2506	rBV2	1300	2014	0.14%	0.024%
100	16.669	2562	2564	2565	rBV2	1076	723	0.05%	0.009%




Sum of corrected areas: 8393401

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030223\
Data File : VD075436.D
Acq On : 02 Mar 2023 11:32
Operator : KP/SY
Sample : VD0302SBL03
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK105

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

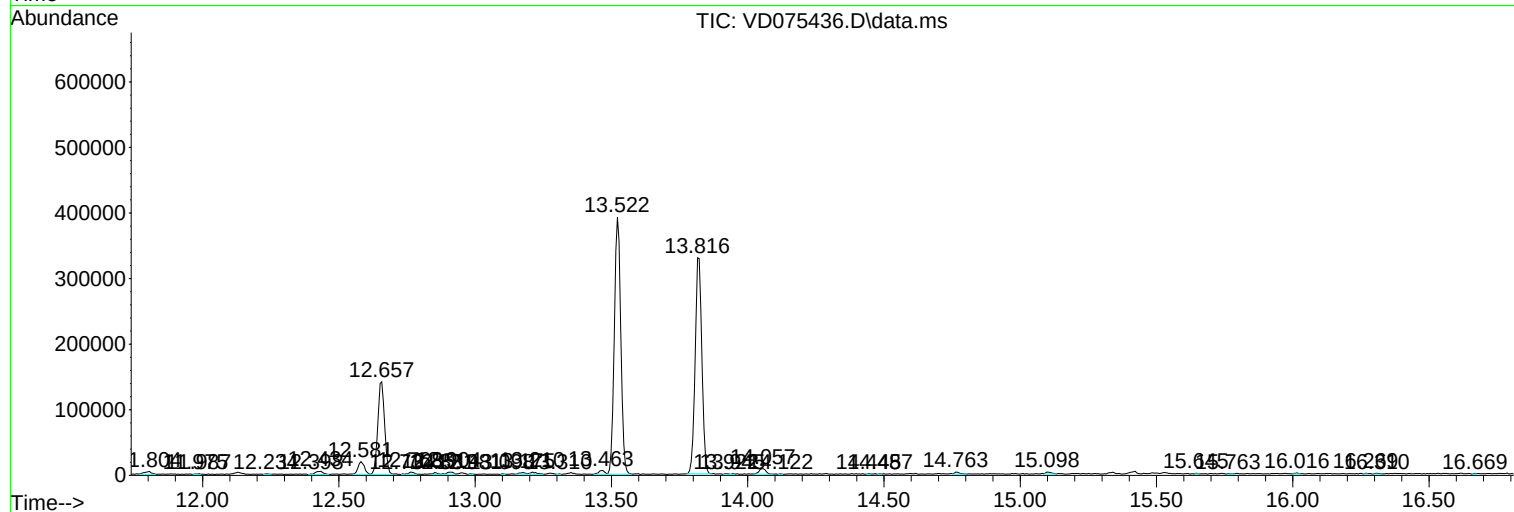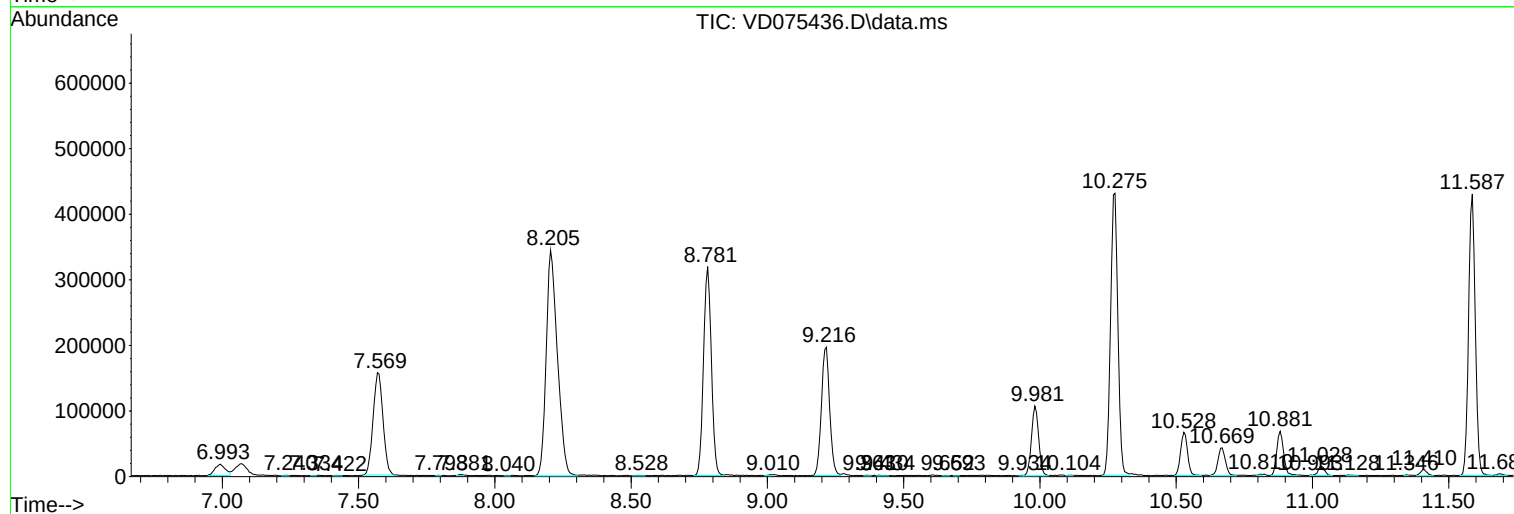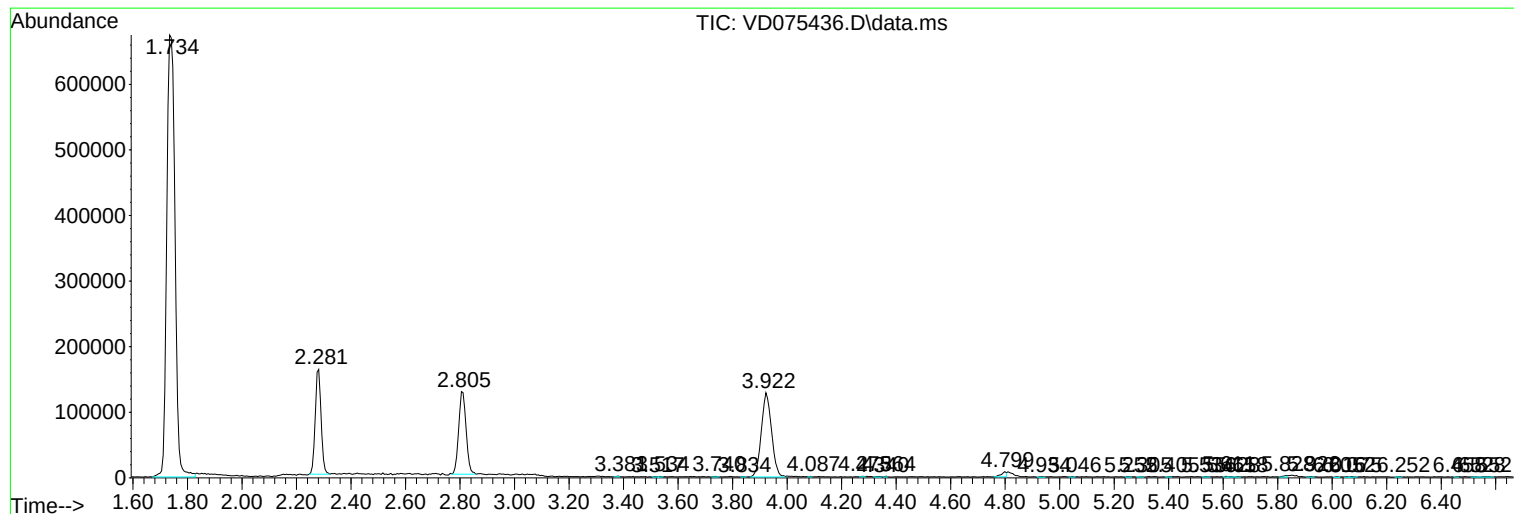

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030223\
Data File : VD075436.D
Acq On : 02 Mar 2023 11:32
Operator : KP/SY
Sample : VD0302SBL03
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK105

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030223\
Data File : VD075436.D
Acq On : 02 Mar 2023 11:32
Operator : KP/SY
Sample : VD0302SBL03
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK105

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------