

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD030320\
 Data File : VD065397.D
 Acq On : 03 Mar 2020 16:31
 Operator : VA/SY
 Sample : L1775-01
 Misc : 7.71G/5.00ml/MSVOA D/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CR-1

Quant Time: Mar 04 05:47:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D021820S.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 19 03:26:54 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	542614	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	928113	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	848090	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	385904	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.34	65	272045	55.73	ug/l	0.00
Spiked Amount						
			Recovery	=	111.46%	
35) Dibromofluoromethane	7.92	113	293713	51.90	ug/l	0.00
Spiked Amount						
			Recovery	=	103.80%	
50) Toluene-d8	10.34	98	1129723	52.22	ug/l	0.00
Spiked Amount						
			Recovery	=	104.44%	
62) 4-Bromofluorobenzene	12.64	95	341281	49.80	ug/l	0.00
Spiked Amount						
			Recovery	=	99.60%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD030320\
Data File : VD065397.D
Acq On : 03 Mar 2020 16:31
Operator : VA/SY
Sample : L1775-01
Misc : 7.71G/5.00ml/MSVOA D/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CR-1

Quant Time: Mar 04 05:47:33 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D021820S.M
Quant Title : SW846 8260
QLast Update : Wed Feb 19 03:26:54 2020
Response via : Initial Calibration

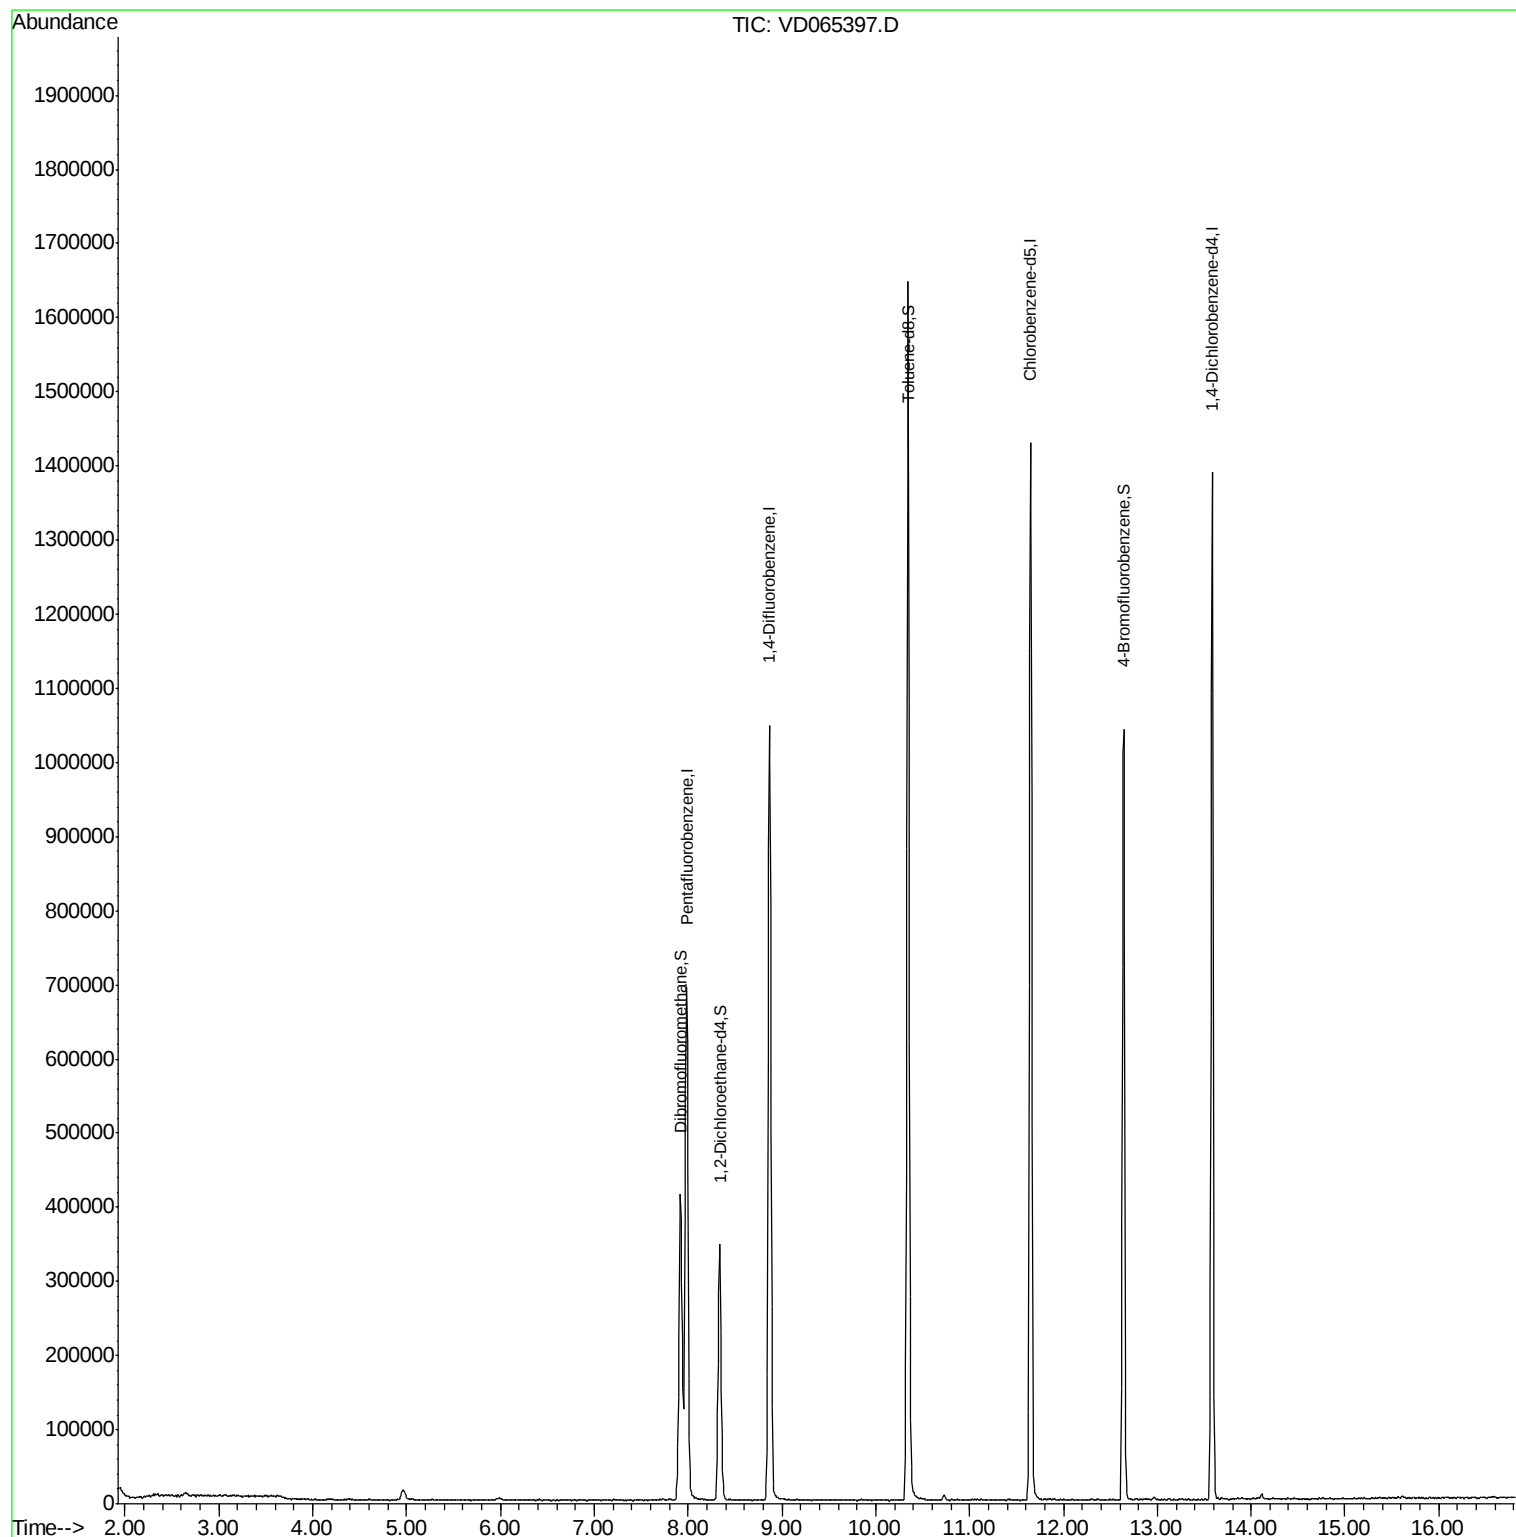

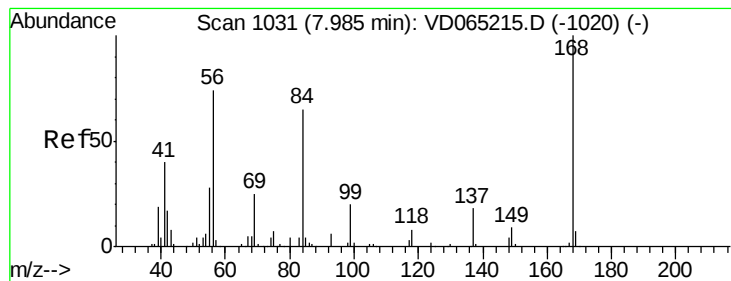

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VD065397.D

Acq: 03 Mar 2020 16:31

Instrument :

MSVOA_D

ClientSampleId :


CR-1

Tot Ion:168 Resp: 542614

Ion Ratio Lower Upper




168 100

99 52.1 41.4 62.2

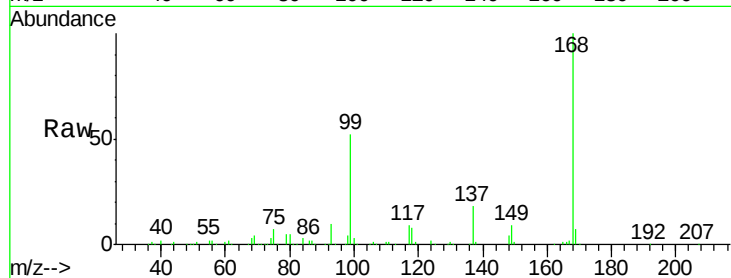

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

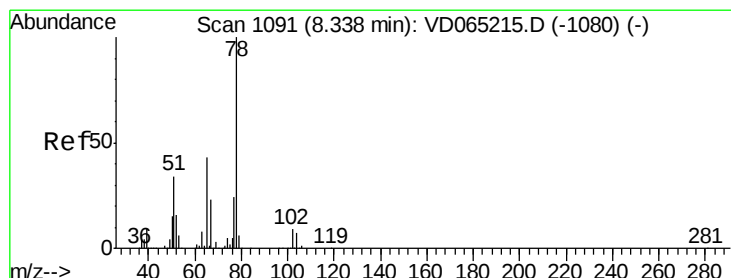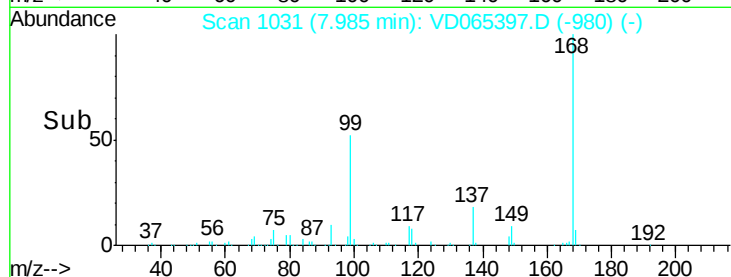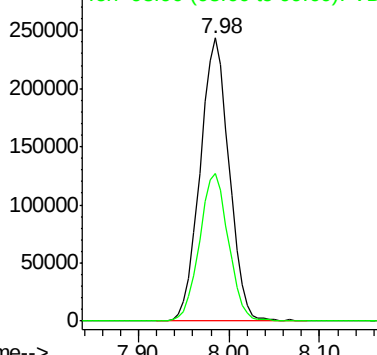

#33

1,2-Dichloroethane-d4

Concen: 55.731 ug/l

RT: 8.34 min Scan# 1091

Delta R.T. 0.00 min

Lab File: VD065397.D


Acq: 03 Mar 2020 16:31

Tgt Ion: 65 Resp: 272045

Ion Ratio Lower Upper



65 100


67 53.1 0.0 106.8

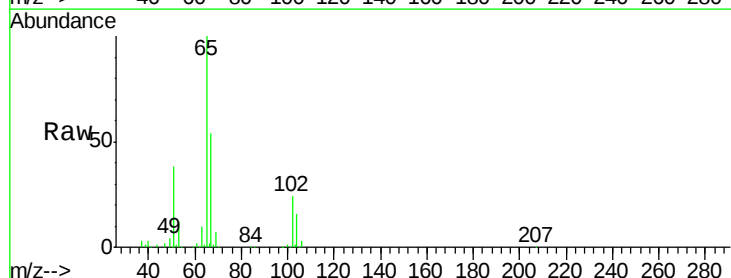

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

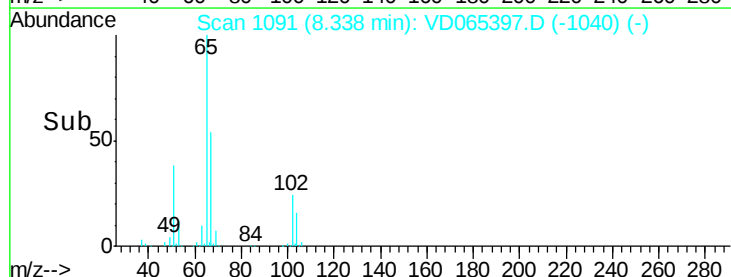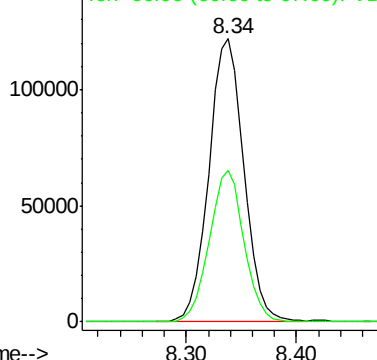

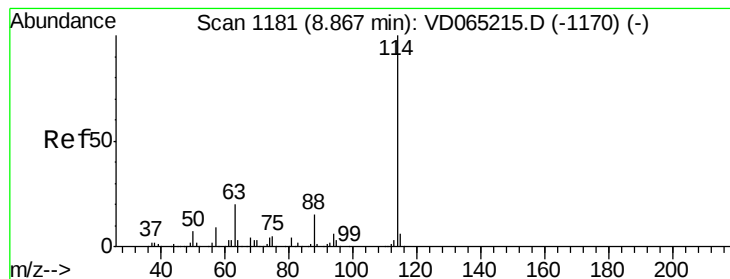

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.87 min Scan# 1181

Delta R.T. 0.00 min

Lab File: VD065397.D

Acq: 03 Mar 2020 16:31

Instrument :

MSVOA_D

ClientSampleId :

CR-1


Tot Ion:114 Resp: 928113

Ion Ratio Lower Upper

114 100

63 19.2 0.0 39.4

88 15.3 0.0 30.4

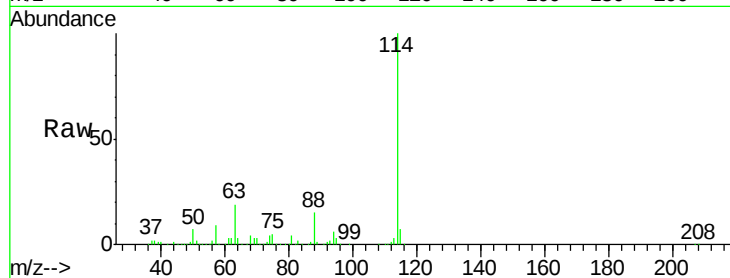

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

8.87

600000

500000

400000



300000

200000

100000

0

Time-->

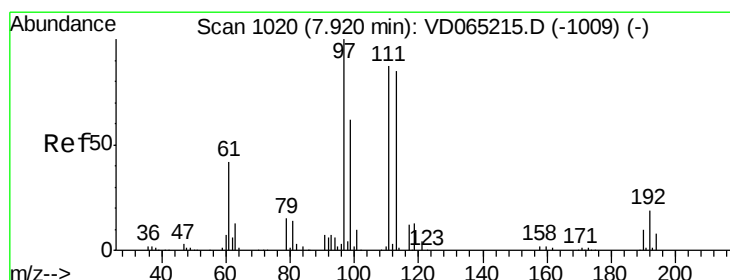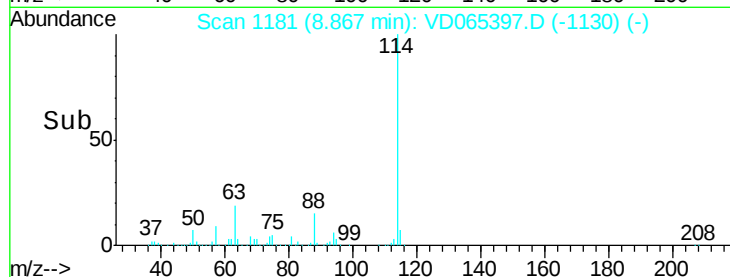

#35

Dibromofluoromethane

Concen: 51.901 ug/l

RT: 7.92 min Scan# 1020

Delta R.T. 0.00 min

Lab File: VD065397.D

Acq: 03 Mar 2020 16:31


Tgt Ion:113 Resp: 293713

Ion Ratio Lower Upper

113 100

111 102.8 82.9 124.3

192 21.8 17.3 25.9

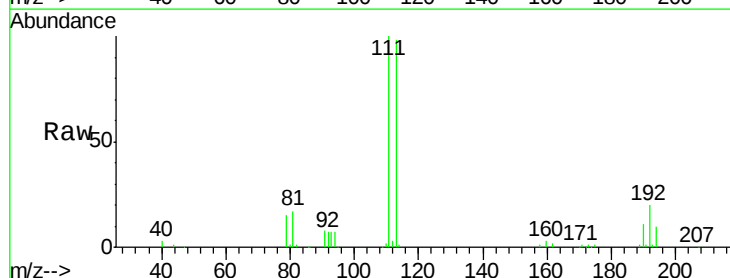

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

7.92


150000

100000

50000

0

Time-->




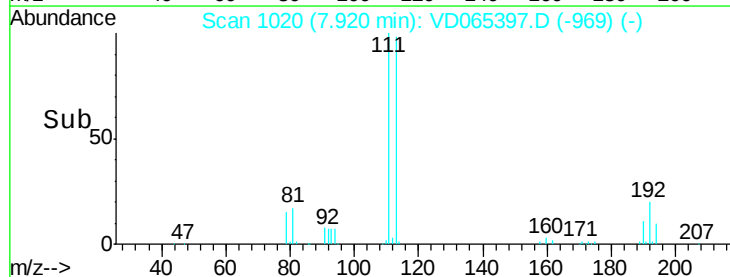




#50
Toluene-d8
Concen: 52.219 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. 0.00 min
Lab File: VD065397.D
Acq: 03 Mar 2020 16:31




Instrument :
MSVOA_D
ClientSampleId :
CR-1


Tot Ion: 98 Resp: 1129723
Ion Ratio Lower Upper
98 100
100 65.0 52.0 78.0

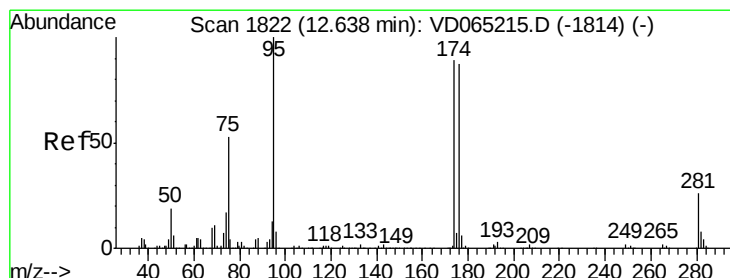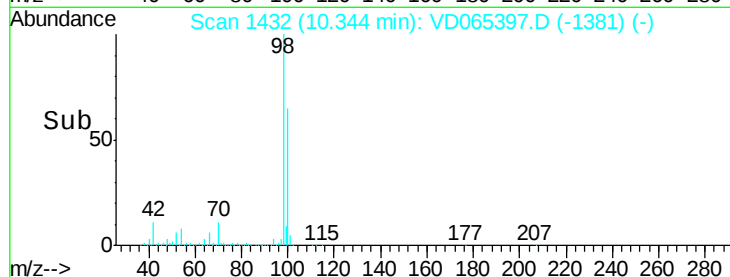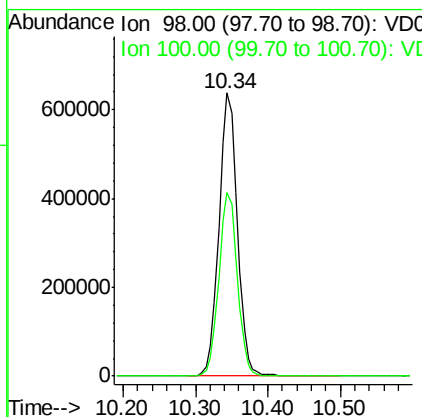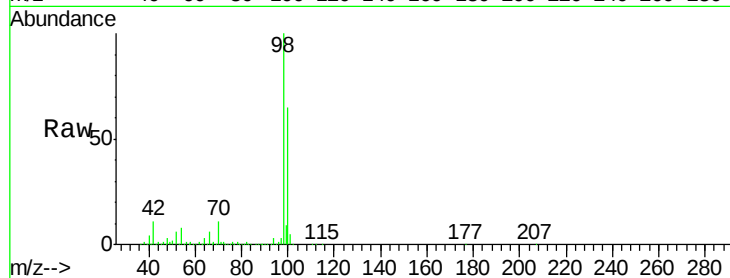

#62
4-Bromofluorobenzene
Concen: 49.796 ug/l
RT: 12.64 min Scan# 1823
Delta R.T. 0.01 min
Lab File: VD065397.D
Acq: 03 Mar 2020 16:31

Tgt Ion: 95 Resp: 341281
Ion Ratio Lower Upper
95 100
174 89.8 0.0 178.0
176 86.5 0.0 174.4


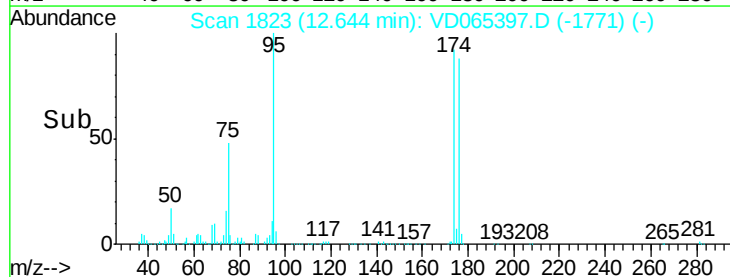
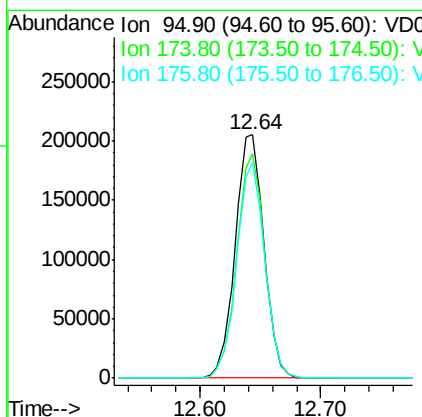
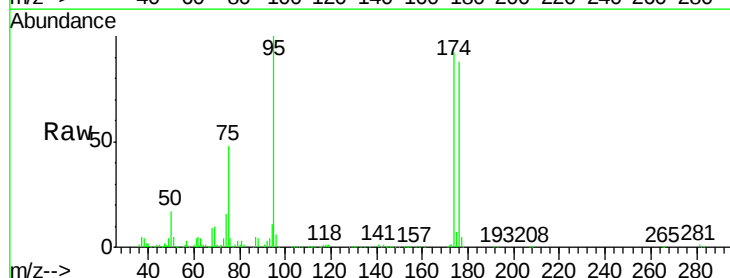


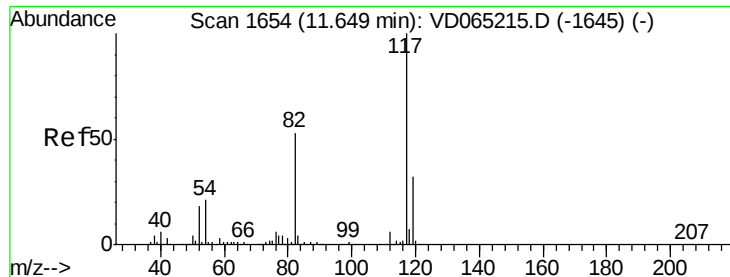

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD065397.D
Acq: 03 Mar 2020 16:31

Instrument :
MSVOA_D
ClientSampleId :
CR-1

Tot Ion:117 Resp: 848090
Ion Ratio Lower Upper
117 100
82 52.5 42.7 64.1
119 31.6 25.5 38.3

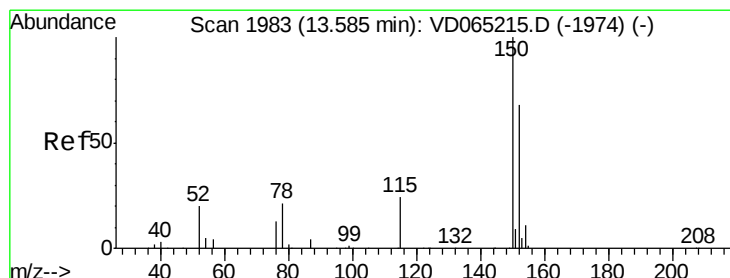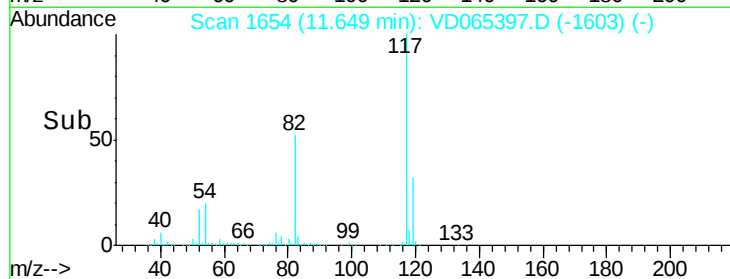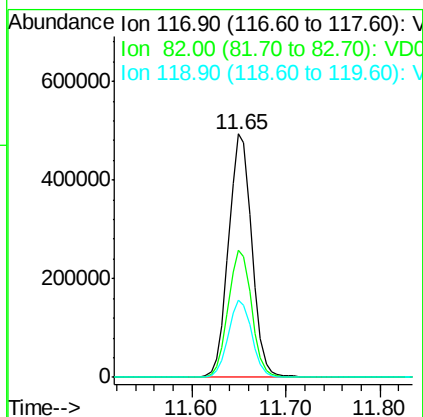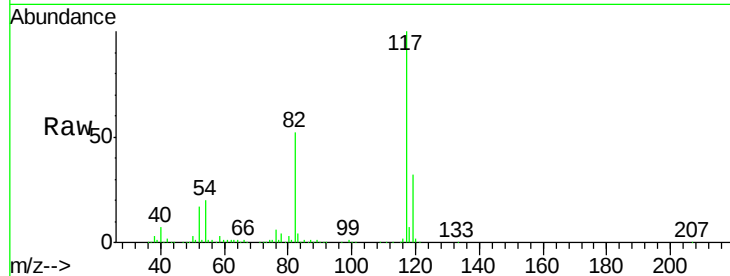

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1983
Delta R.T. 0.00 min
Lab File: VD065397.D
Acq: 03 Mar 2020 16:31

Tgt Ion:152 Resp: 385904
Ion Ratio Lower Upper
152 100
115 53.8 27.6 82.8
150 154.2 0.0 347.4

