

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030323\
 Data File : VD075443.D
 Acq On : 03 Mar 2023 10:00
 Operator : KP/SY
 Sample : VD0303SBL04
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Mar 03 23:24:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 03 23:23:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	300658	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117	269866	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	113510	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	143126	19.172	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	76.680%		
7) Chloroethane-d5	2.805	69	134173	20.769	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.080%		
11) 1,1-Dichloroethene-d2	3.922	63	105916	15.189	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	60.760%		
21) 2-Butanone-d5	6.987	46	31010	44.825	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	89.660%		
24) Chloroform-d	7.569	84	169777	21.547	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	86.200%		
26) 1,2-Dichloroethane-d4	8.228	65	75128	22.009	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	88.040%		
32) Benzene-d6	8.205	84	348912	21.771	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.080%		
36) 1,2-Dichloropropane-d6	9.210	67	101920	22.500	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	90.000%		
41) Toluene-d8	10.275	98	309248	21.151	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.600%		
43) trans-1,3-Dichloroprop...	10.528	79	39689	21.441	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	85.760%		
47) 2-Hexanone-d5	10.881	63	26142	40.005	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	80.000%		
56) 1,1,2,2-Tetrachloroeth...	12.657	84	80368	21.211	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	84.840%		
66) 1,2-Dichlorobenzene-d4	13.816	152	95458	24.042	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	96.160%		
Target Compounds						Qvalue
37) 1,2-Dichloropropane	9.210	63	10491	2.201	ug/L	# 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030323\
Data File : VD075443.D
Acq On : 03 Mar 2023 10:00
Operator : KP/SY
Sample : VD0303SBL04
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :

Quant Time: Mar 03 23:24:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 03 23:23:38 2023
Response via : Initial Calibration

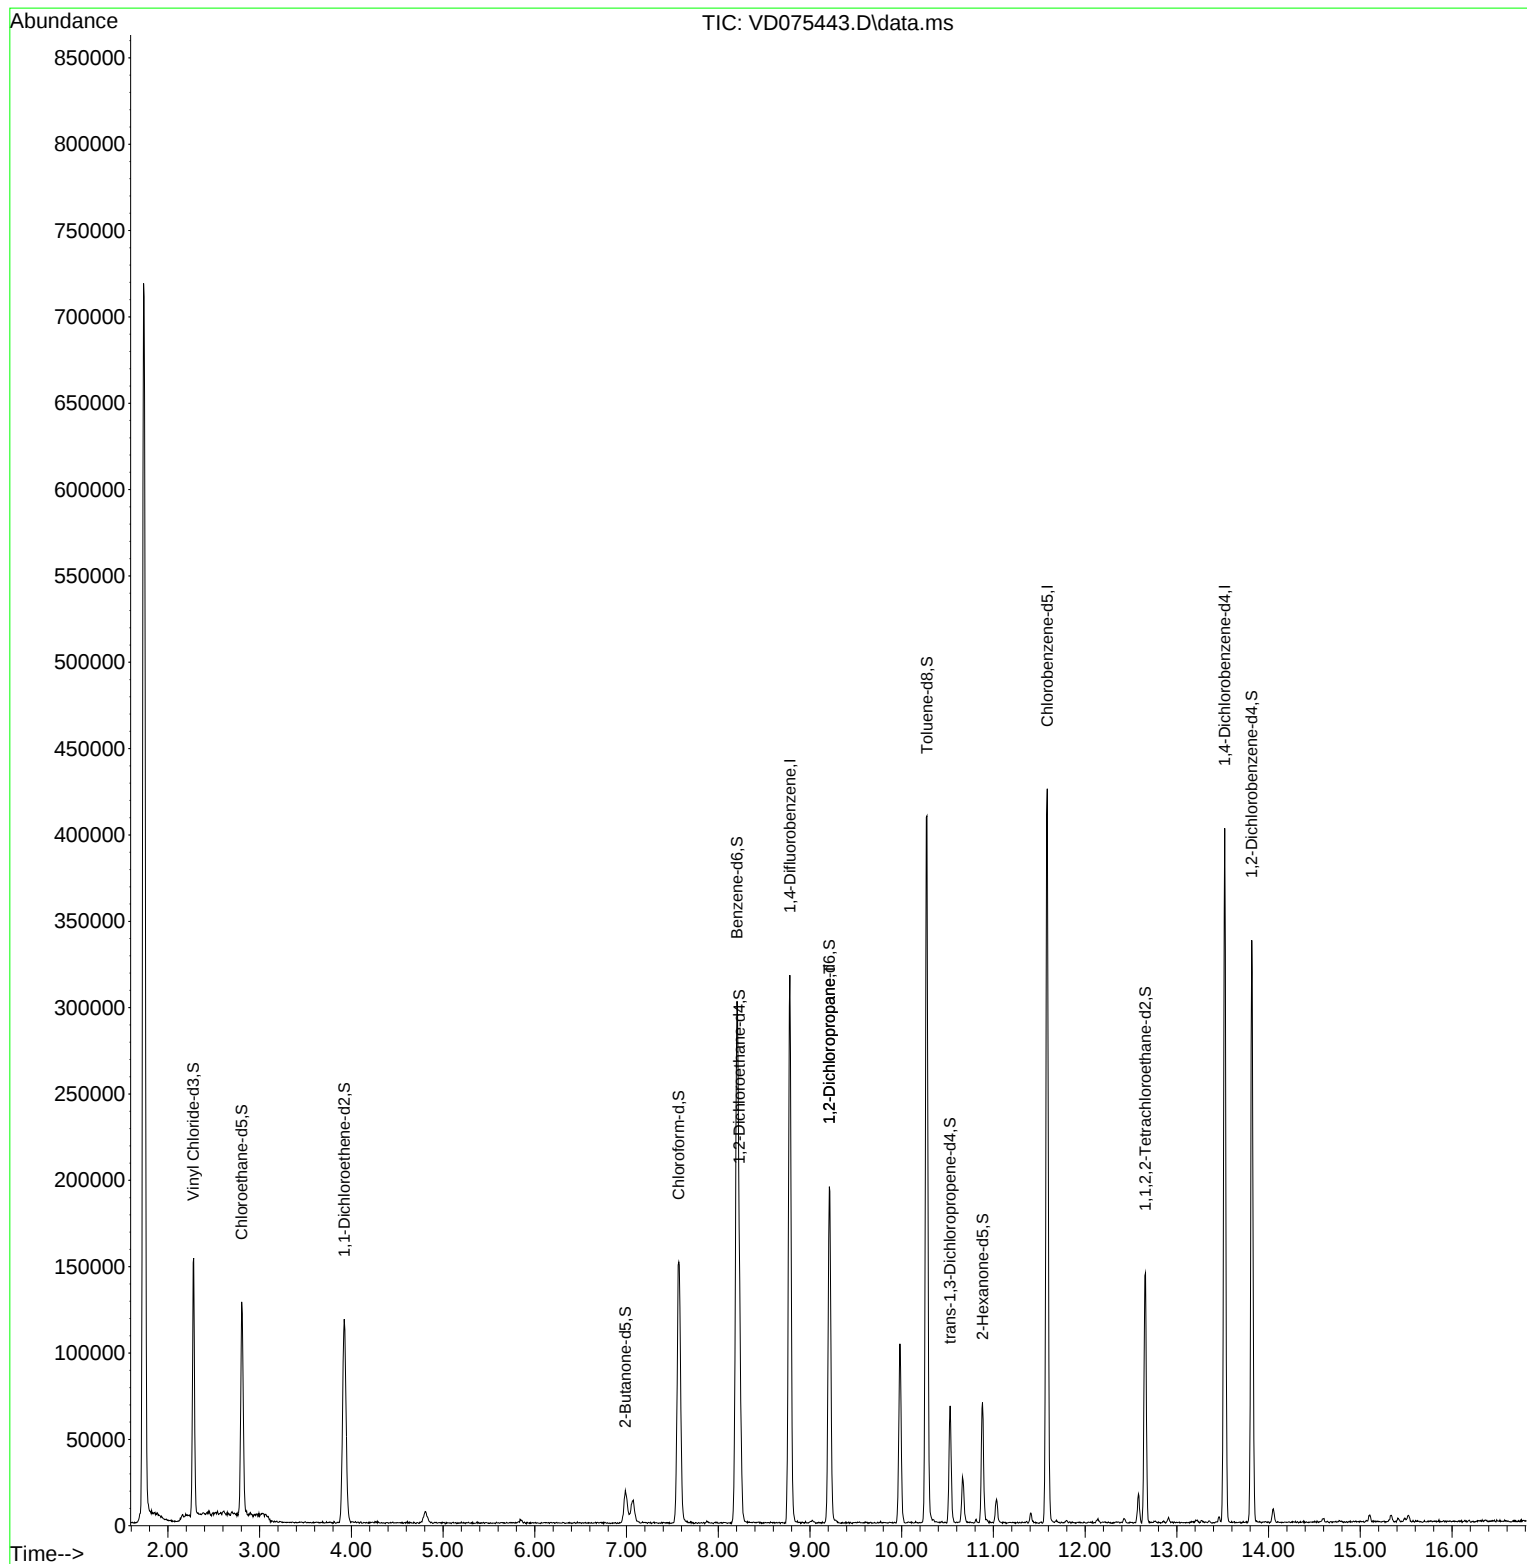

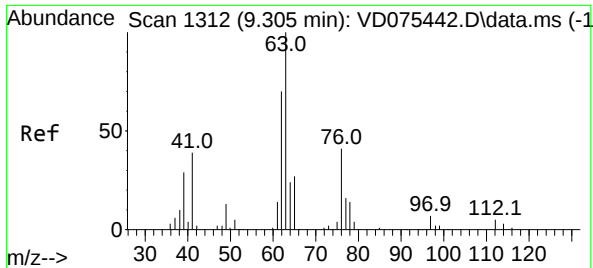

#37
 1,2-Dichloropropane
 Concen: 2.201 ug/L
 RT: 9.210 min Scan# 11
 Delta R.T. -0.094 min
 Lab File: VD075443.D
 Acq: 03 Mar 2023 10:00

Instrument :
 MSVOA_D
 ClientSampleId :

Tgt Ion: 63 Resp: 10491
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.8 5.6#

