


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD030419\
 Data File : VD060916.D
 Acq On : 4 Mar 2019 11:12
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030119S.M
 Title : SW846 8260
 Last Update : Sat Mar 02 01:28:28 2019

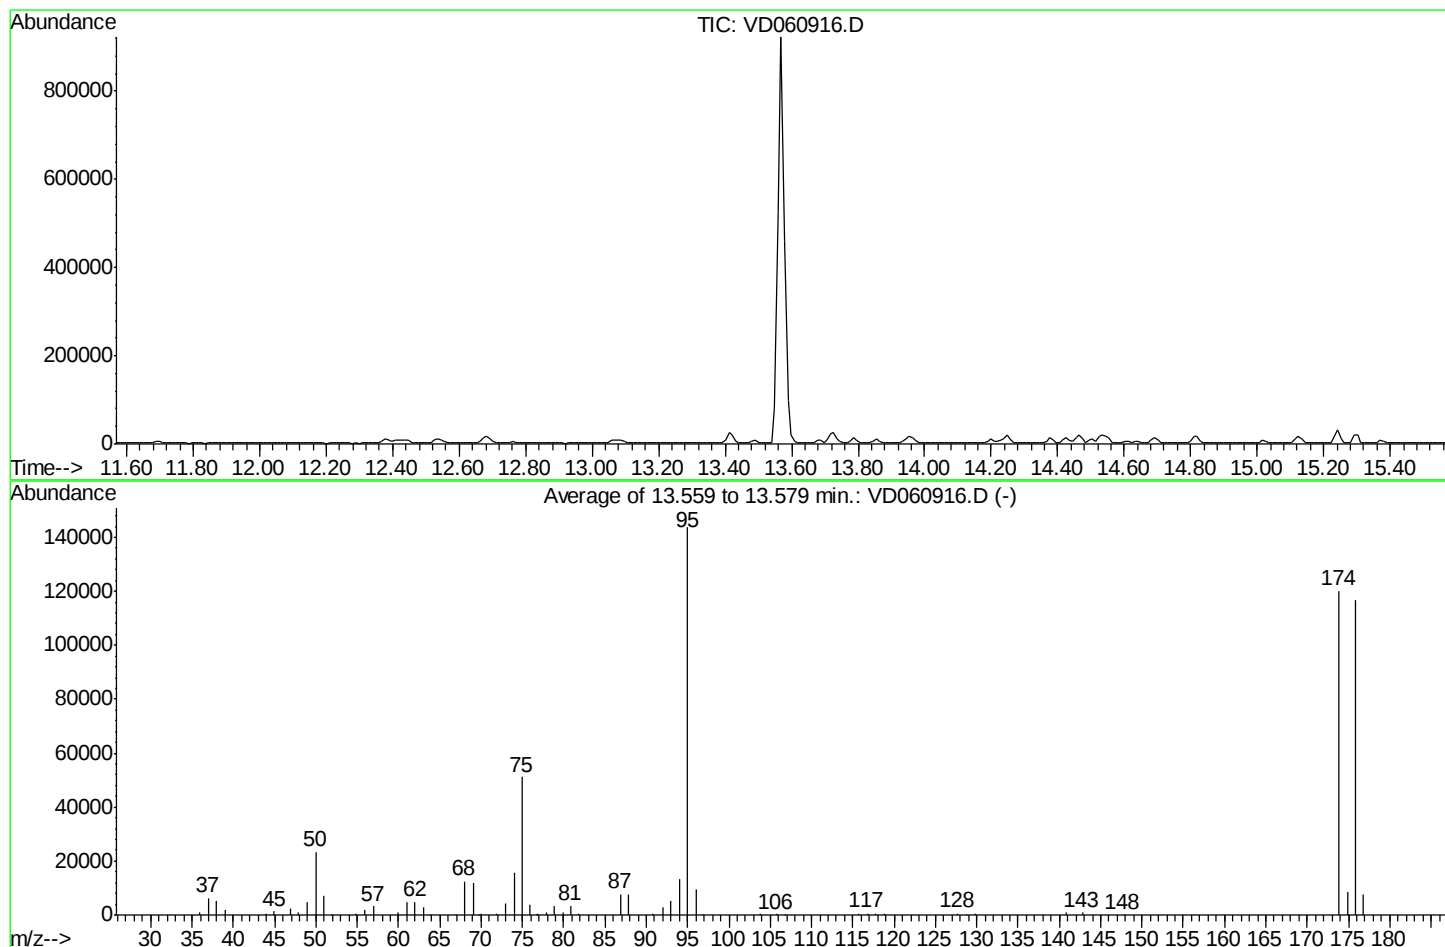

AutoFind: Scans 1233, 1234, 1235; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	23408	PASS
75	95	30	60	35.5	51053	PASS
95	95	100	100	100.0	143749	PASS
96	95	5	9	6.5	9322	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.6	120130	PASS
175	174	5	9	7.1	8516	PASS
176	174	95	101	97.2	116736	PASS
177	176	5	9	6.3	7404	PASS