



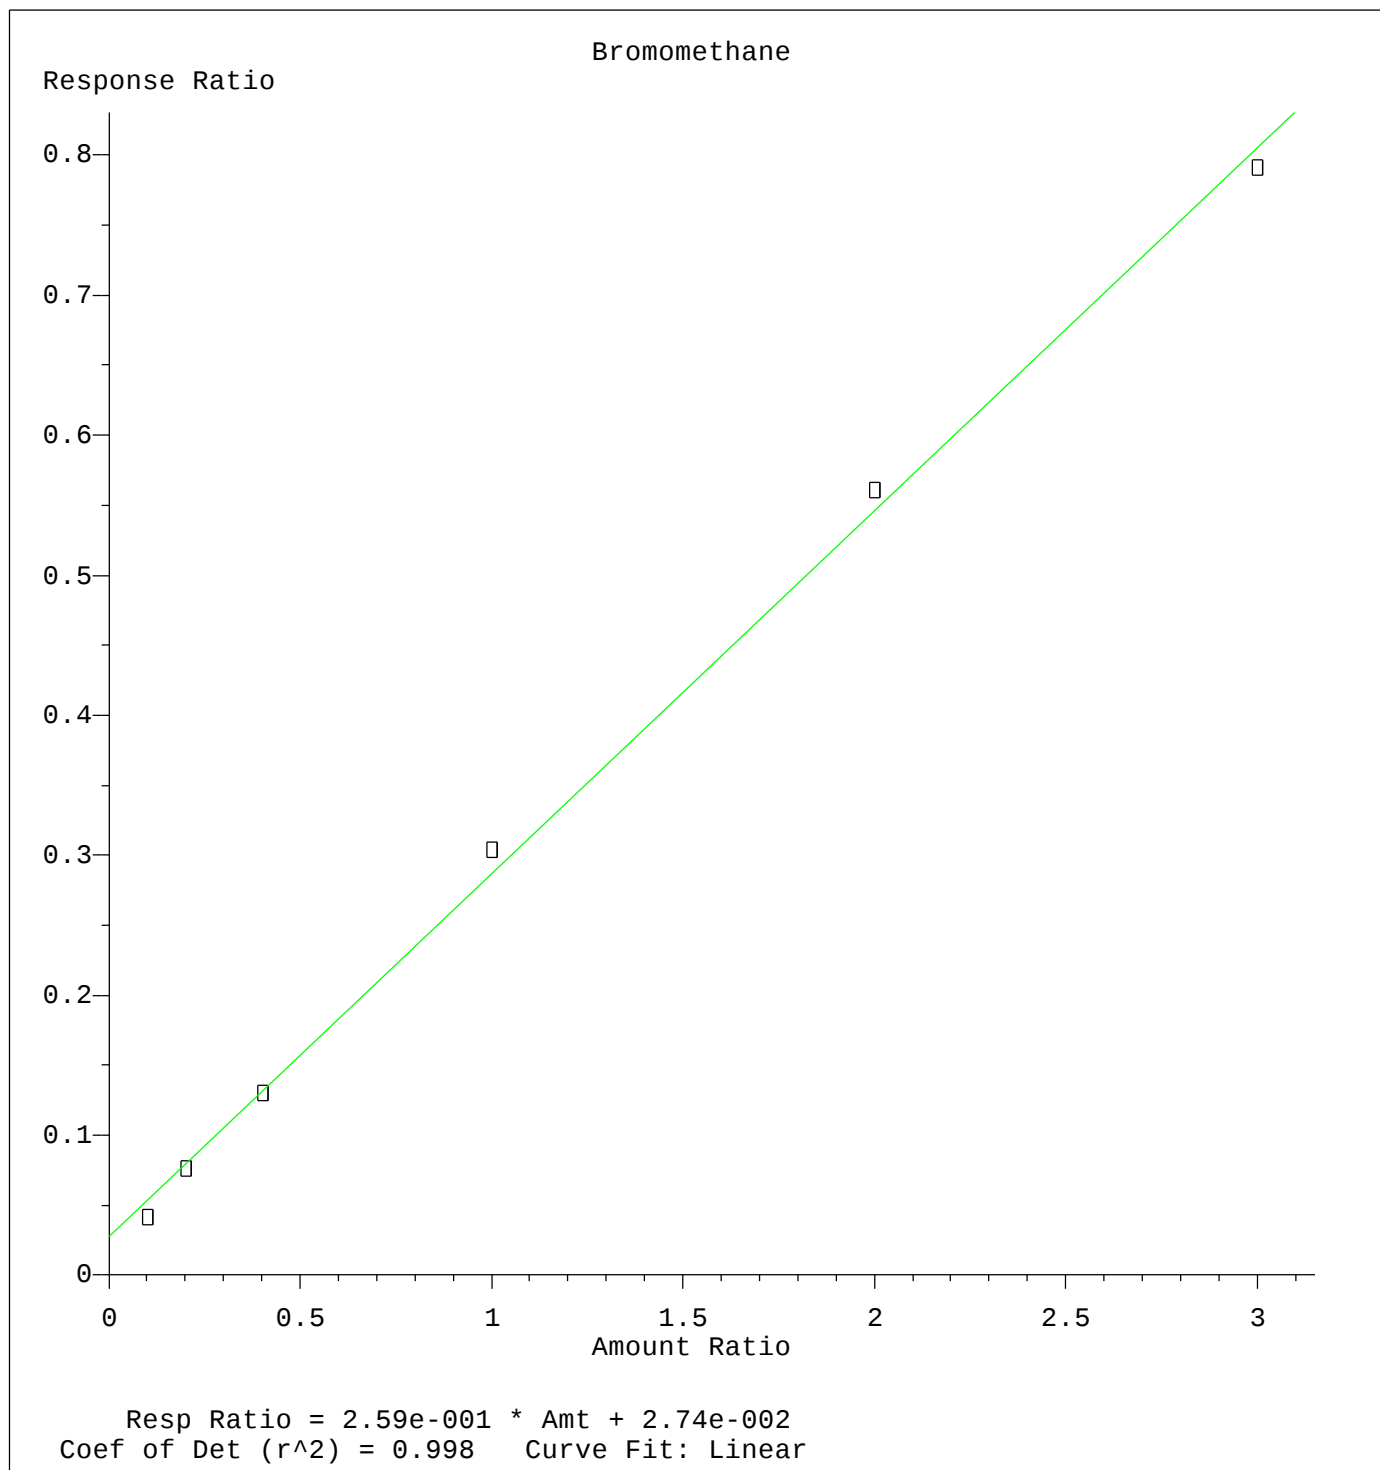

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030420S.M
Calibration Table Last Updated: Wed Mar 04 16:52:47 2020

Methylene Chloride

Response Ratio

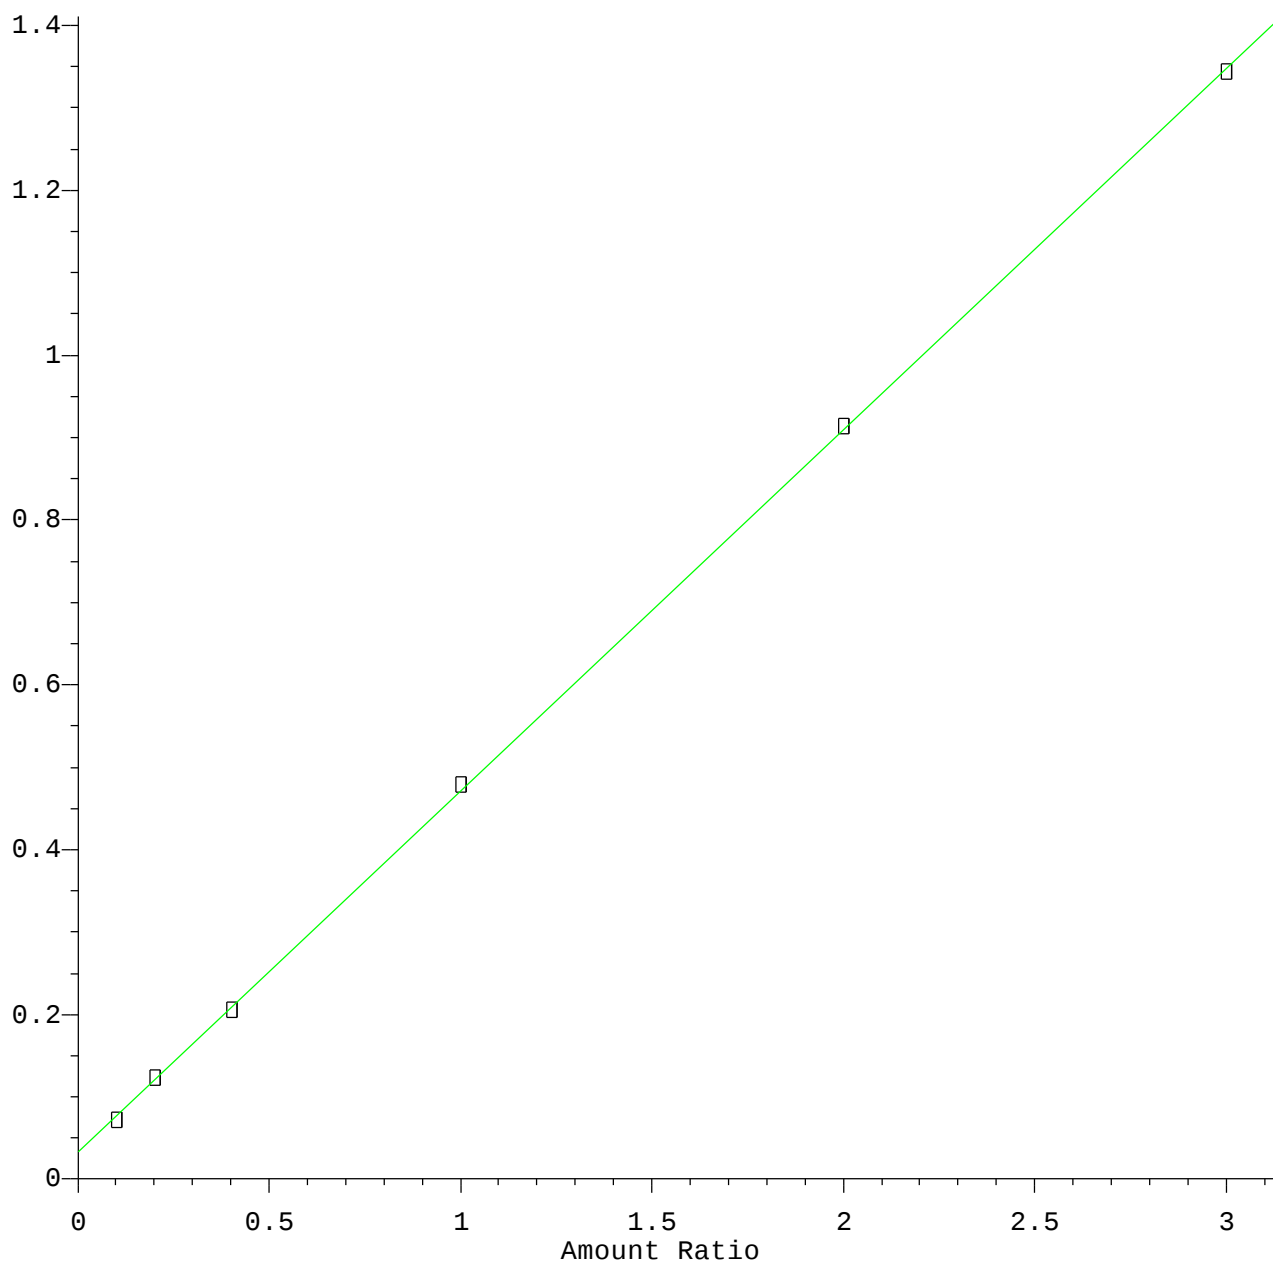


Resp Ratio = $4.38 \times 10^{-1} \times \text{Amt} + 3.26 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030420S.M
Calibration Table Last Updated: Wed Mar 04 16:52:47 2020

2-Chloroethyl Vinyl ether

Response Ratio

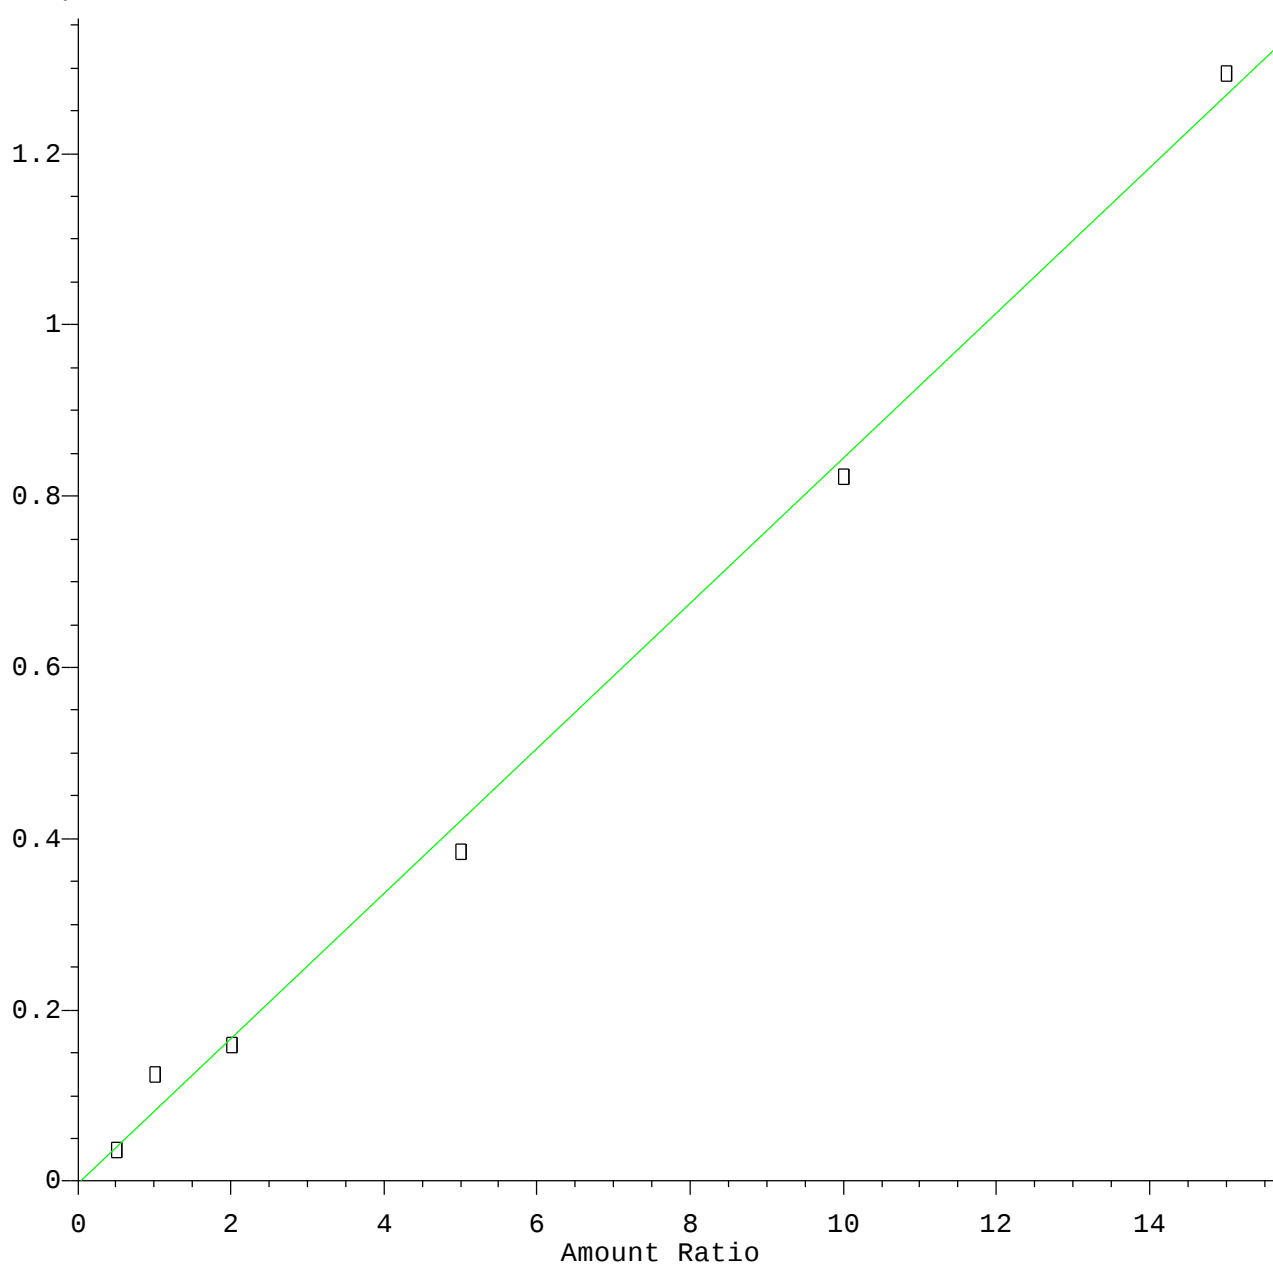


Resp Ratio = 8.48×10^{-2} * Amt - 3.70×10^{-3}
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030420S.M
Calibration Table Last Updated: Wed Mar 04 16:54:14 2020

Naphthalene

Response Ratio

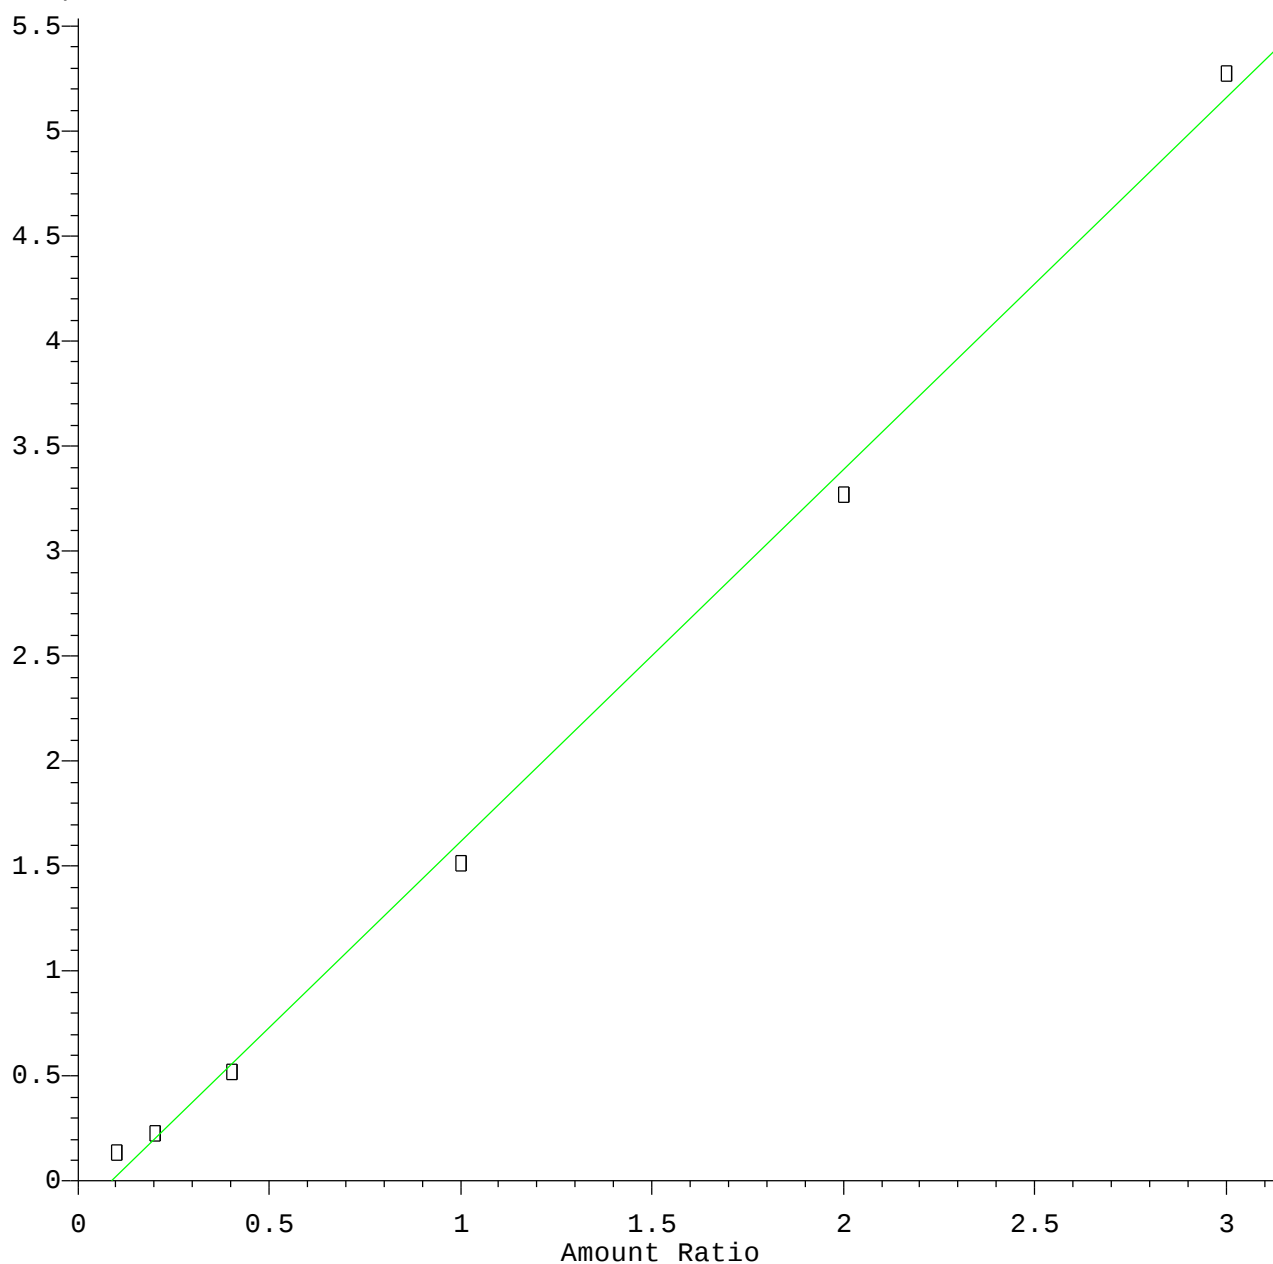


Resp Ratio = 1.77e+000 * Amt - 1.56e-001
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030420S.M
Calibration Table Last Updated: Wed Mar 04 16:54:14 2020

Methylene Chloride

Response Ratio

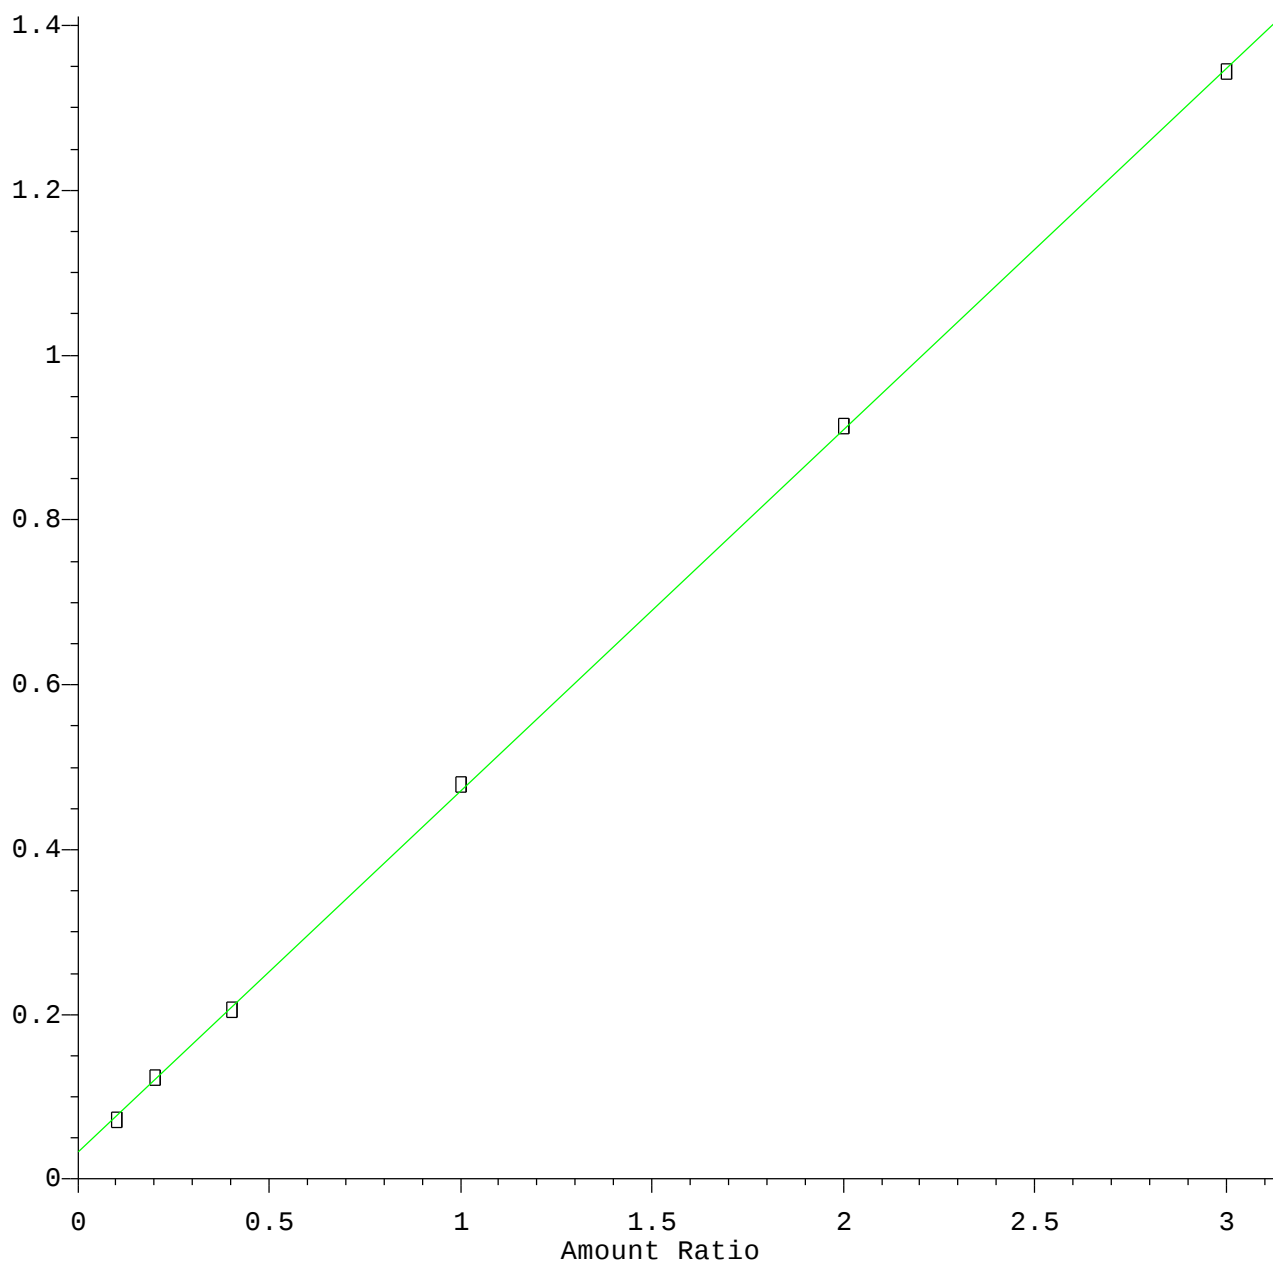

Resp Ratio = $4.38 \times 10^{-1} \times \text{Amt} + 3.26 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030420S.M
Calibration Table Last Updated: Wed Mar 04 16:52:47 2020