


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD030420\
 Data File : VD065403.D
 Acq On : 04 Mar 2020 09:22
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030420S.M
 Title : SW846 8260
 Last Update : Thu Mar 05 01:22:07 2020

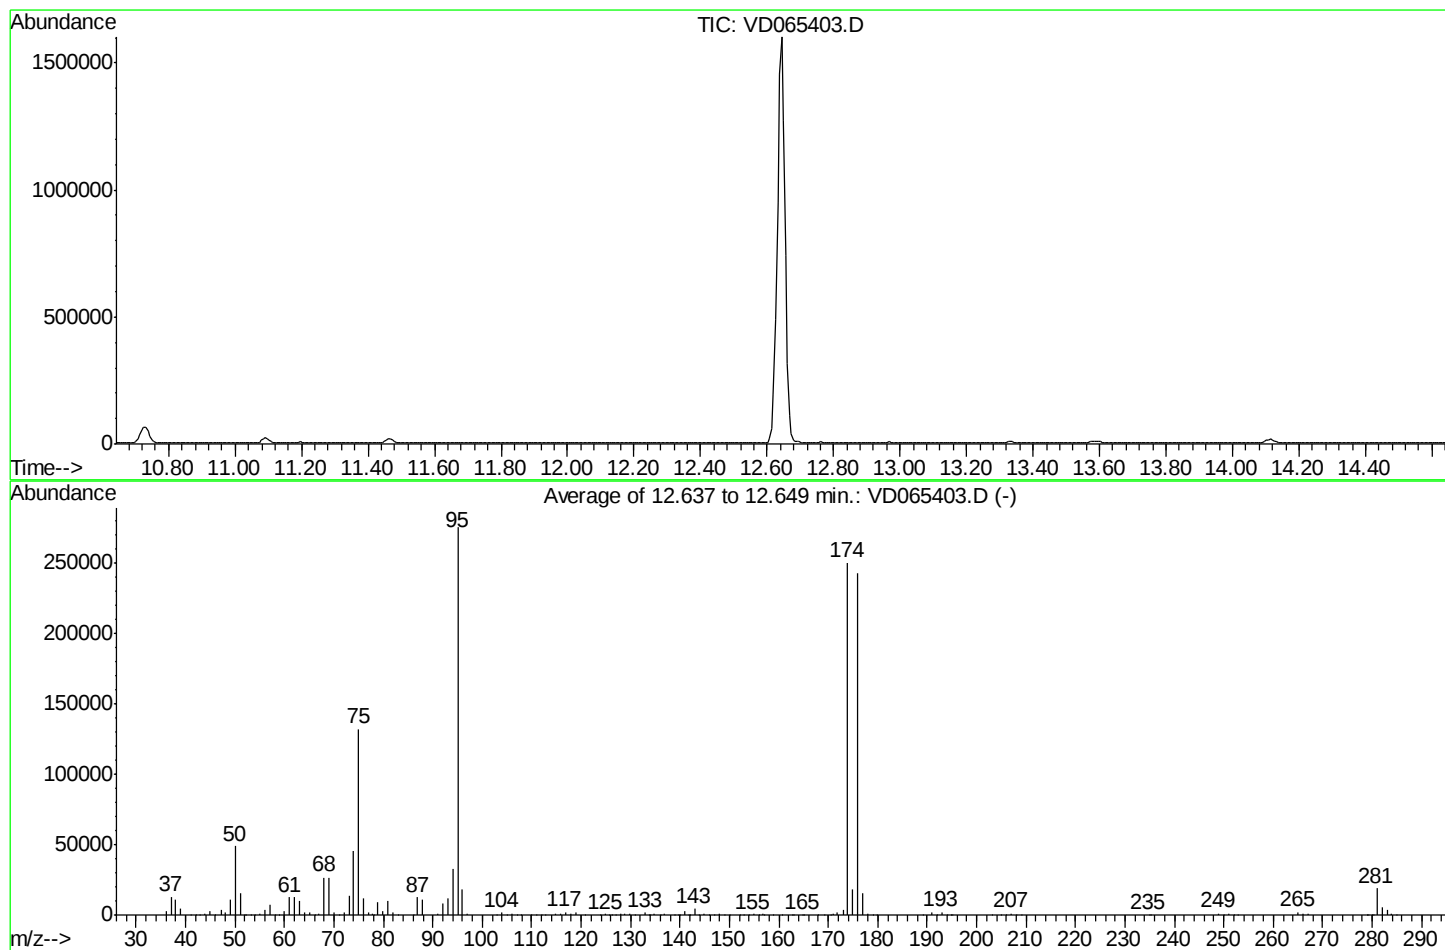

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	48888	PASS
75	95	30	60	48.0	131920	PASS
95	95	100	100	100.0	275008	PASS
96	95	5	9	6.7	18315	PASS
173	174	0.00	2	1.3	3269	PASS
174	95	50	100	90.8	249792	PASS
175	174	5	9	7.4	18605	PASS
176	174	95	101	97.2	242880	PASS
177	176	5	9	6.4	15427	PASS