
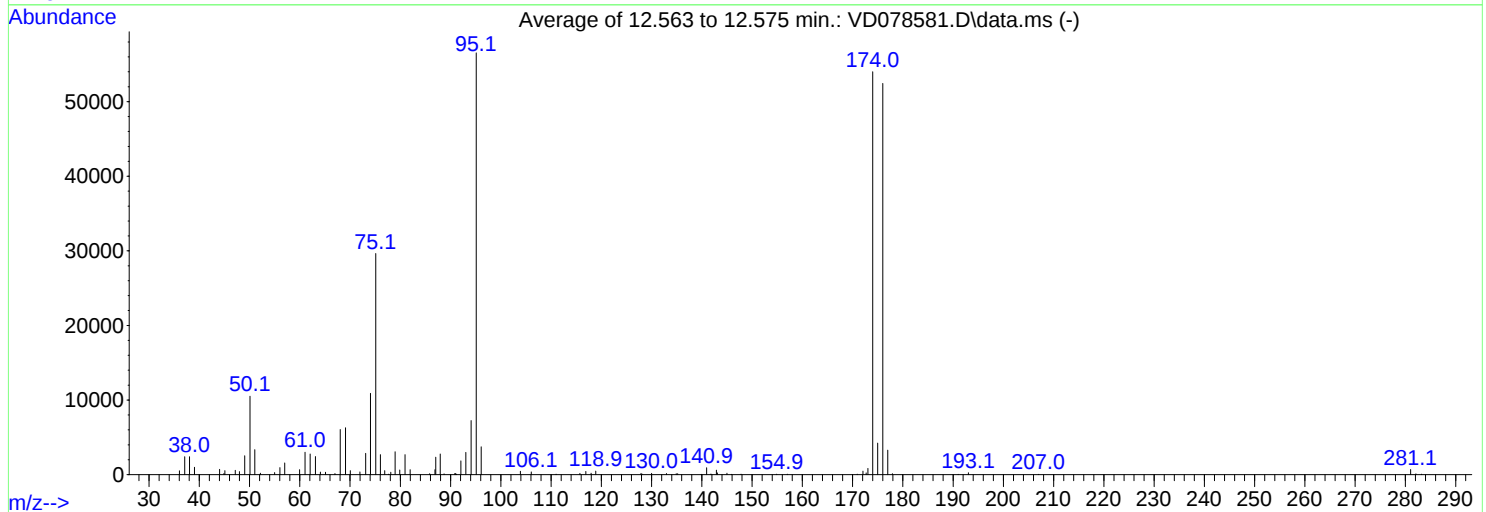


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030424\
Data File : VD078581.D
Acq On : 04 Mar 2024 09:18
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D030124S.M
Title : SW846 8260
Last Update : Sat Mar 02 03:50:17 2024

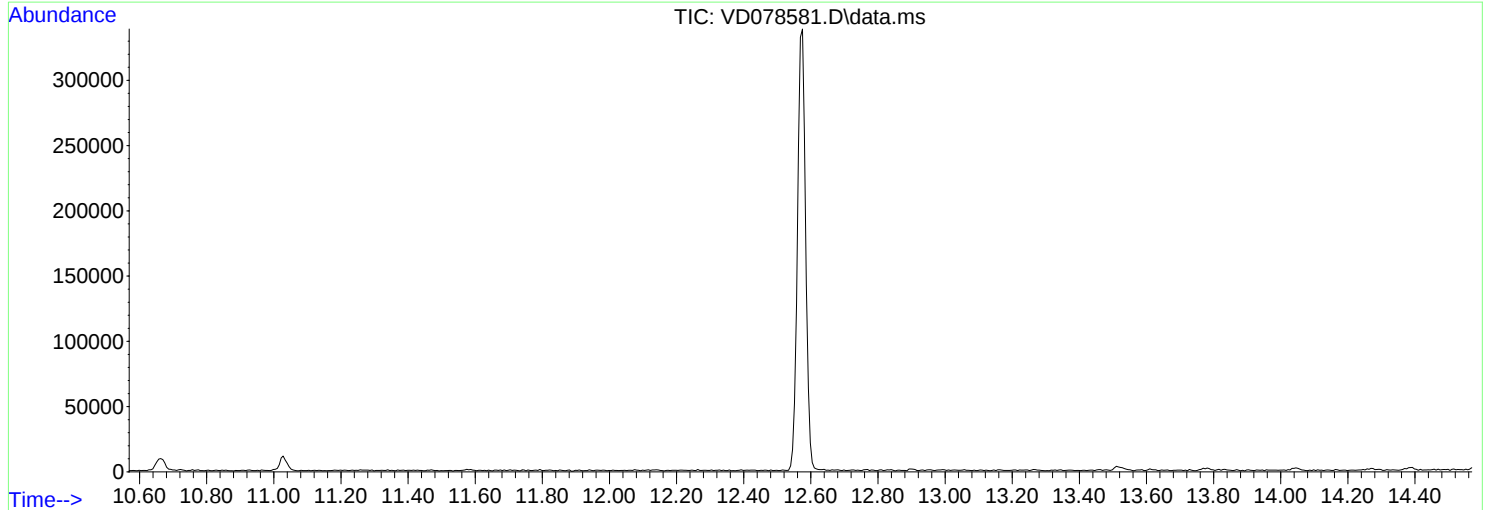

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	10502	PASS
75	95	30	60	52.4	29651	PASS
95	95	100	100	100.0	56544	PASS
96	95	5	9	6.6	3741	PASS
173	174	0.00	2	1.6	841	PASS
174	95	50	100	95.5	54019	PASS
175	174	5	9	7.8	4220	PASS
176	174	95	101	97.1	52440	PASS
177	176	5	9	6.2	3277	PASS