


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD030719\
 Data File : VD060967.D
 Acq On : 7 Mar 2019 14:02
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
 Title : SW846 8260
 Last Update : Fri Mar 08 02:35:39 2019

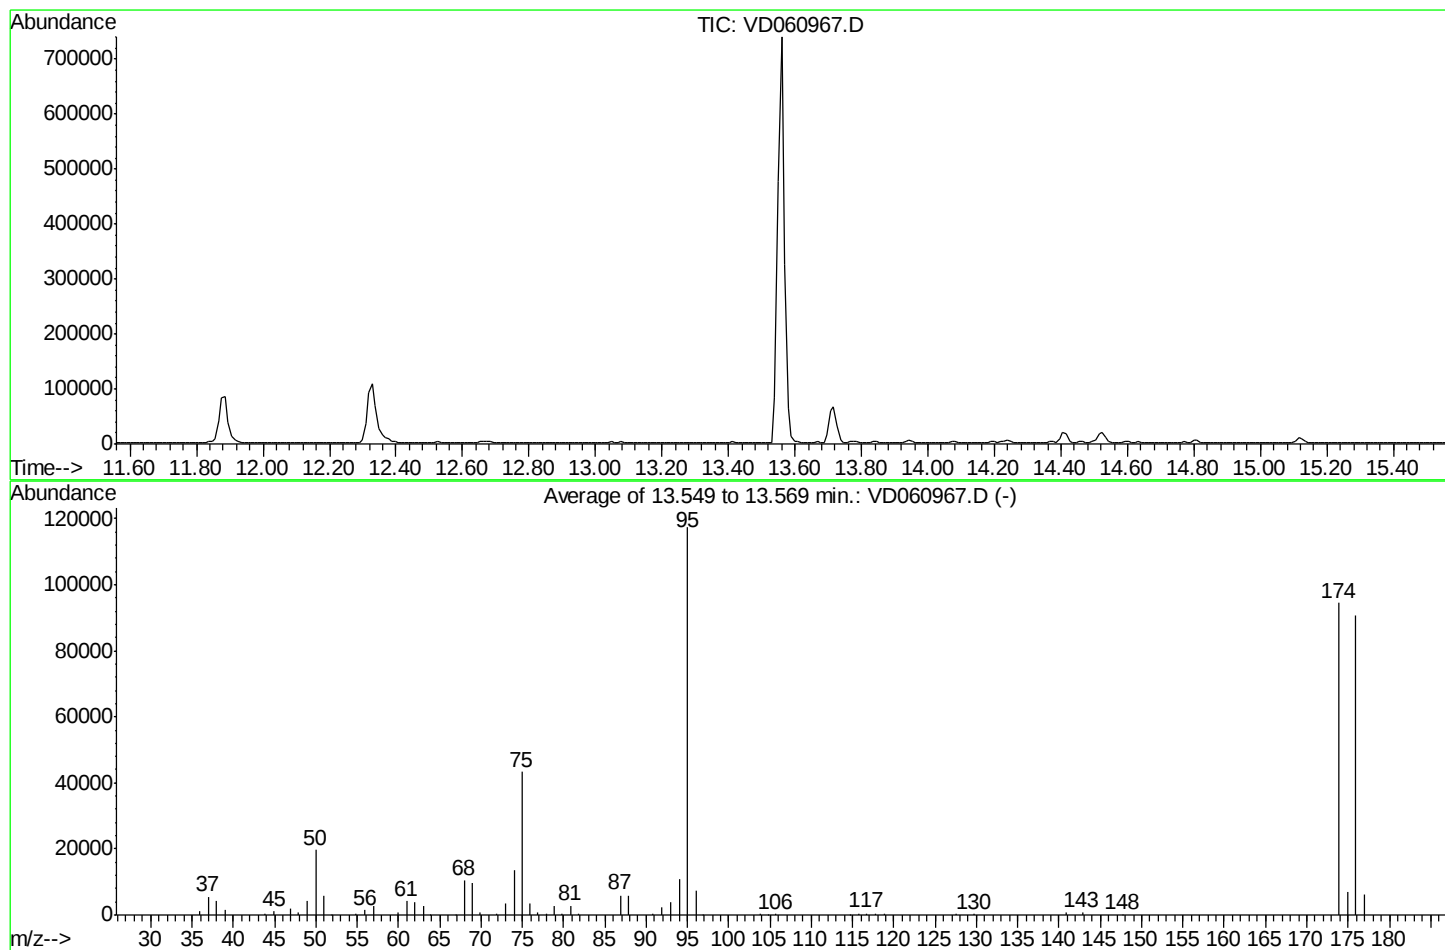

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	19596	PASS
75	95	30	60	36.9	43338	PASS
95	95	100	100	100.0	117373	PASS
96	95	5	9	6.3	7413	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.4	94410	PASS
175	174	5	9	7.3	6891	PASS
176	174	95	101	96.2	90848	PASS
177	176	5	9	6.6	6024	PASS