

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD030819\
 Data File : VD060994.D
 Acq On : 8 Mar 2019 20:08
 Operator : VA/AP
 Sample : K1807-17RE
 Misc : 5.10µ/5ml/MSVOA D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TP-9RE

Quant Time: Mar 08 23:08:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 08 02:35:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	µg/l	-7.04
34) 1,4-Difluorobenzene	0.00	114	0	0.00	µg/l	-8.21
63) Chlorobenzene-d5	0.00	117	0	0.00	µg/l	-12.36
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	µg/l	-14.51

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Recovery
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	µg/l	0.00%
Spiked Amount				50.000		
35) Dibromofluoromethane	0.00	113	0	0.00	µg/l	0.00%
Spiked Amount				50.000		
50) Toluene-d8	0.00	98	0	0.00	µg/l	0.00%
Spiked Amount				50.000		
62) 4-Bromofluorobenzene	0.00	95	0	0.00	µg/l	0.00%
Spiked Amount				50.000		


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD030819\
Data File : VD060994.D
Acq On : 8 Mar 2019 20:08
Operator : VA/AP
Sample : K1807-17RE
Misc : 5.10µ/5ml/MSVOA D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampled :
TP-9RE

Quant Time: Mar 08 23:08:03 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 08 02:35:39 2019
Response via : Initial Calibration


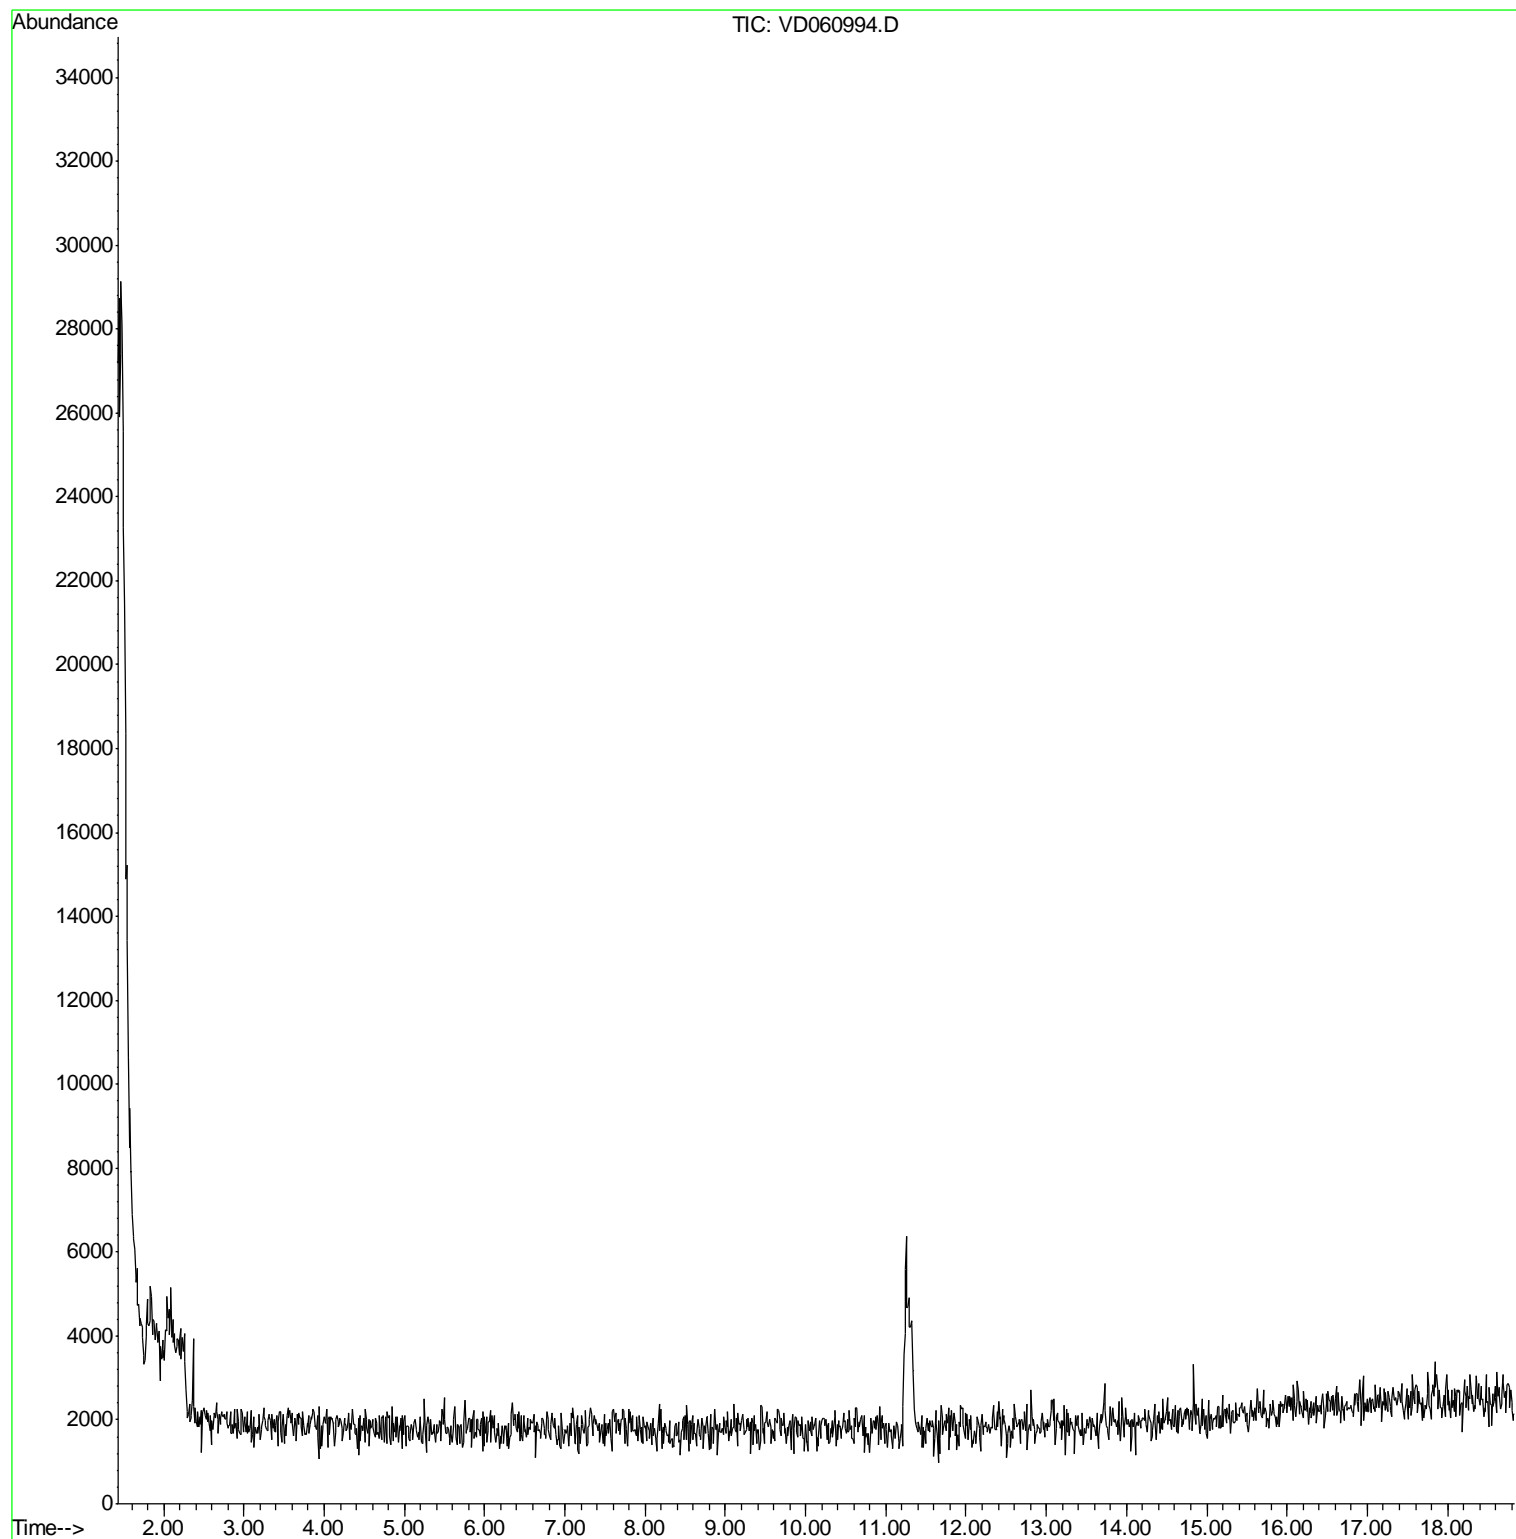


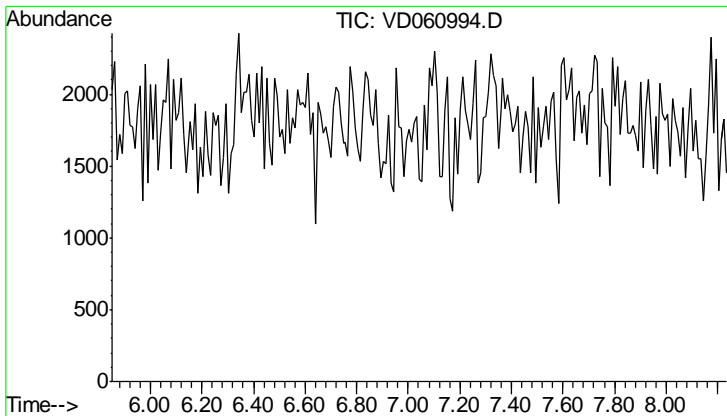

#1
 Pentafluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 7.04 min
 Lab File: VD060994.D
 Acq: 8 Mar 2019 20:08


Instrument :
 MSVOA_D
ClientSampled :
 TP-9RE


Tgt Ion	Exp Ratio
168	100
99	59.1

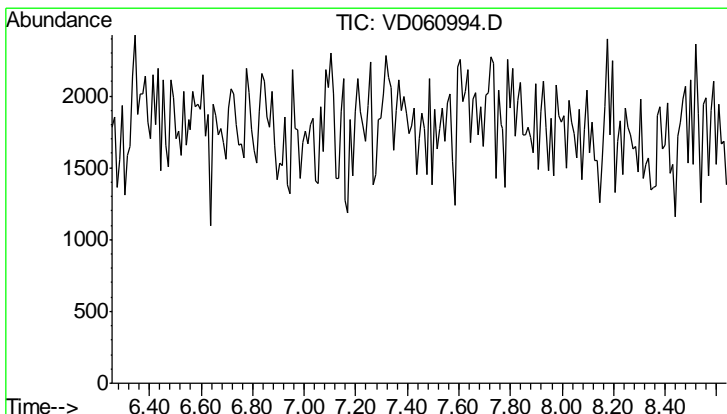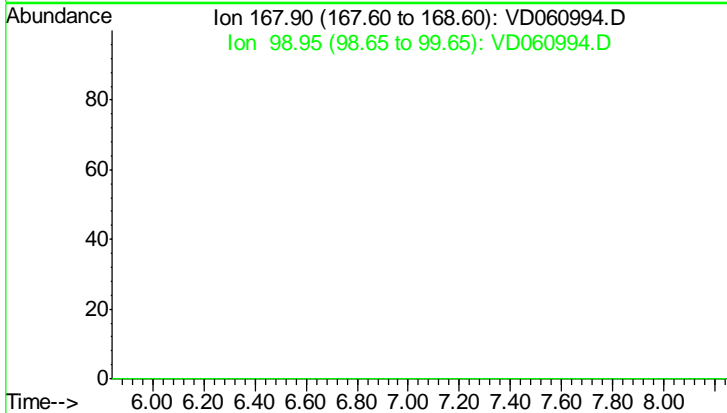

#33
 1,2-Dichloroethane-d4
 Concen: N.D. ug/l
 Expected RT: 7.45 min
 Lab File: VD060994.D
 Acq: 8 Mar 2019 20:08

Tgt Ion	Exp Ratio
65	100
67	52.6


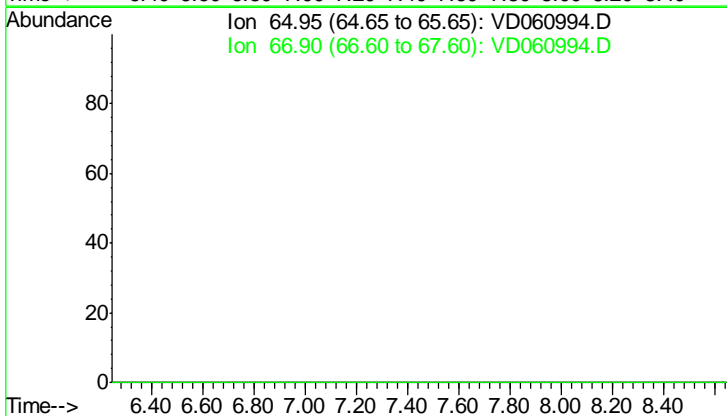


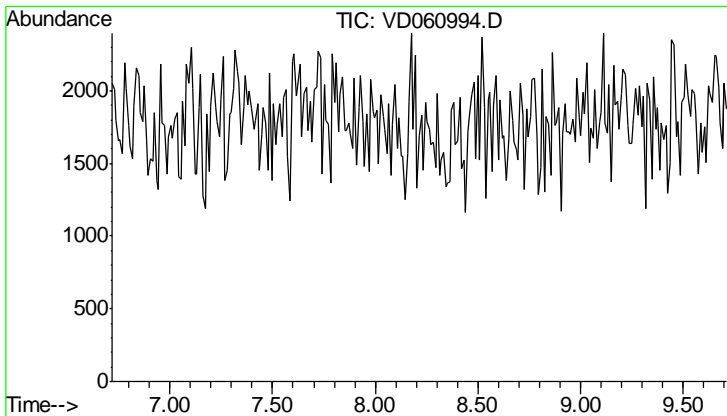

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.21 min
 Lab File: VD060994.D
 Acq: 8 Mar 2019 20:08


Instrument : MSVOA_D
 ClientSampled : TP-9RE


Tgt Ion	Exp Ratio
114	100
63	15.7
88	16.5

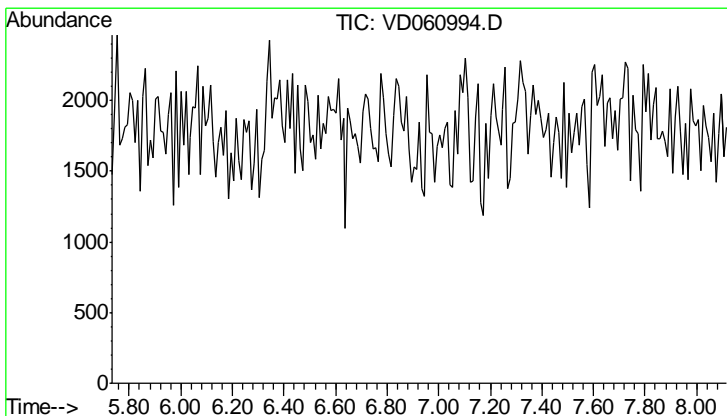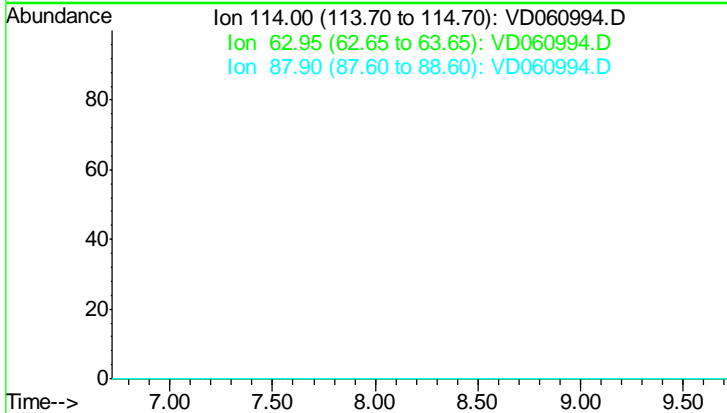

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 6.92 min
 Lab File: VD060994.D
 Acq: 8 Mar 2019 20:08

Tgt Ion	Exp Ratio
113	100
111	105.3
192	16.4


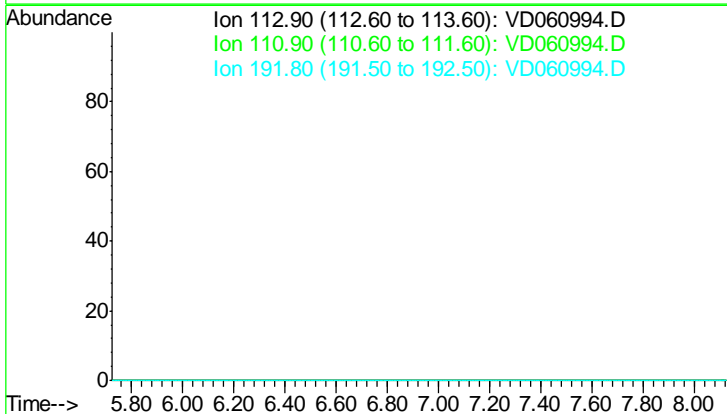


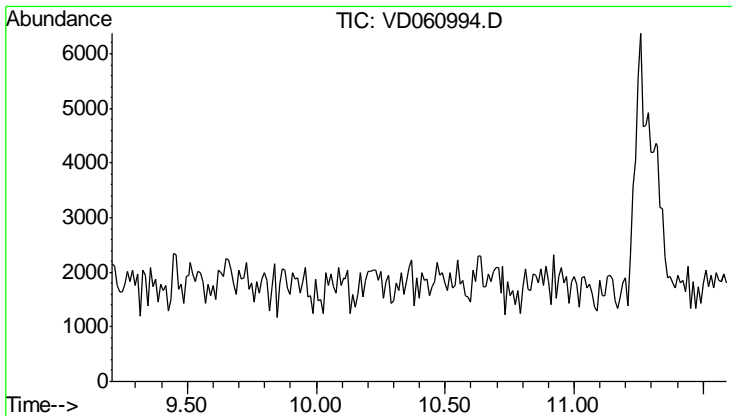

#50
 Toluene-d8
 Concen: N.D. ug/l
 Expected RT: 10.40 min
 Lab File: VD060994.D
 Acq: 8 Mar 2019 20:08


Instrument : MSVOA_D
 ClientSampled : TP-9RE


Tgt Ion: 98
 Sig Exp Ratio
 98 100
 100 71.8

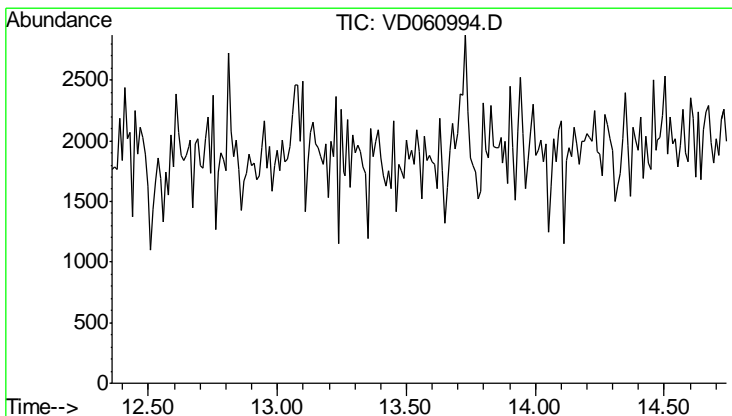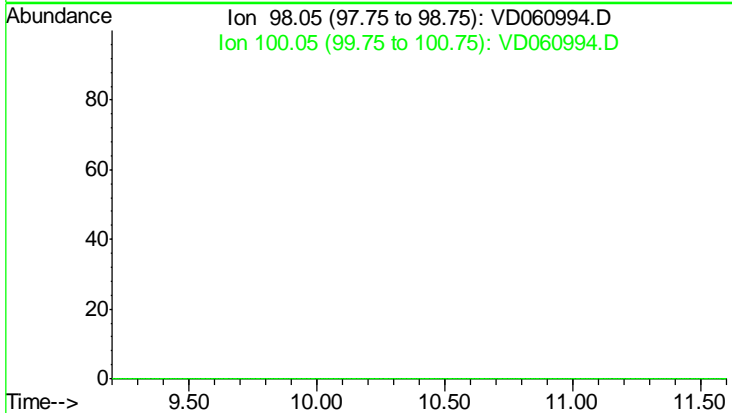

#62
 4-Bromofluorobenzene
 Concen: N.D. ug/l
 Expected RT: 13.55 min
 Lab File: VD060994.D
 Acq: 8 Mar 2019 20:08

Tgt Ion: 95
 Sig Exp Ratio
 95 100
 174 77.8
 176 76.9


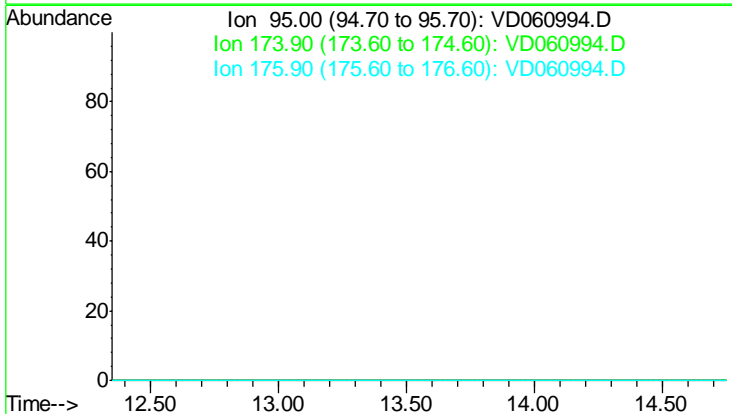


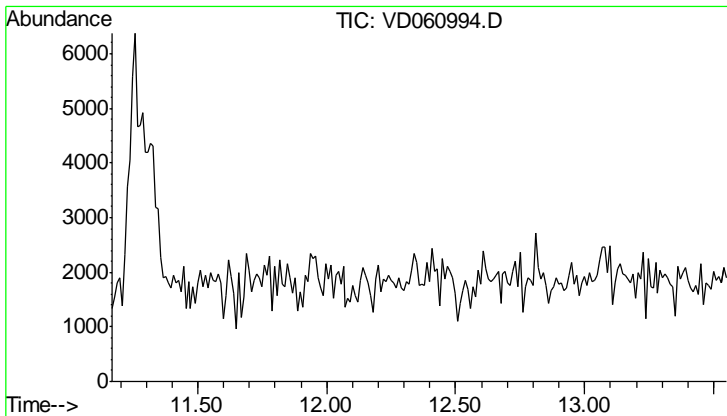

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 12.36 min
 Lab File: VD060994.D
 Acq: 8 Mar 2019 20:08

Instrument : MSVOA_D
 ClientSampled : TP-9RE

Tgt Ion	Exp Ratio
117	100
82	48.6
119	33.2

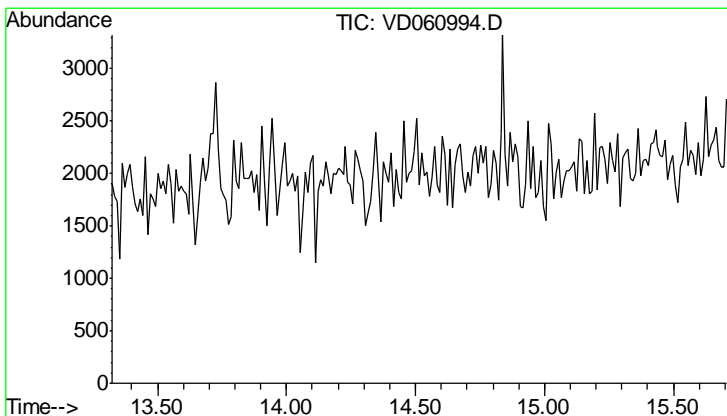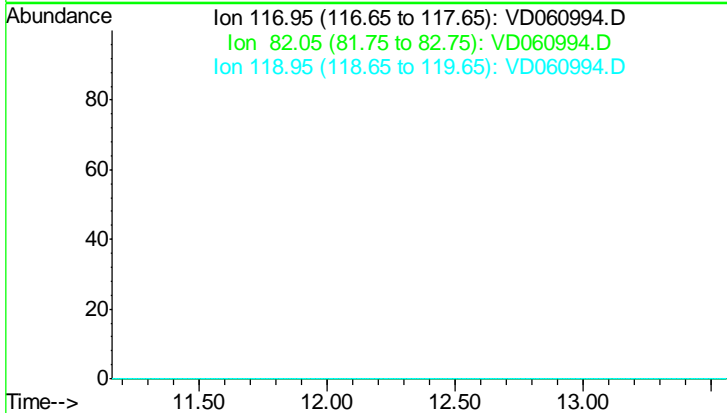

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 14.51 min
 Lab File: VD060994.D
 Acq: 8 Mar 2019 20:08

Tgt Ion	Exp Ratio
152	100
115	57.3
150	155.3

