

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030824\
 Data File : VD078614.D
 Acq On : 08 Mar 2024 10:53
 Operator : RP/MD
 Sample : VD0308SBL01
 Misc : 5.00G/5ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0308SBL01

Quant Time: Mar 09 02:31:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D030124S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 02 03:50:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	120066	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	214478	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	195404	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	85870	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	60471	50.807	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	101.620%
35) Dibromofluoromethane	7.799	113	65919	47.248	ug/l	-0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	94.500%
50) Toluene-d8	10.269	98	238049	43.910	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	87.820%
62) 4-Bromofluorobenzene	12.575	95	61157	39.496	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	79.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030824\
Data File : VD078614.D
Acq On : 08 Mar 2024 10:53
Operator : RP/MD
Sample : VD0308SBL01
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0308SBL01

Quant Time: Mar 09 02:31:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D030124S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 02 03:50:17 2024
Response via : Initial Calibration




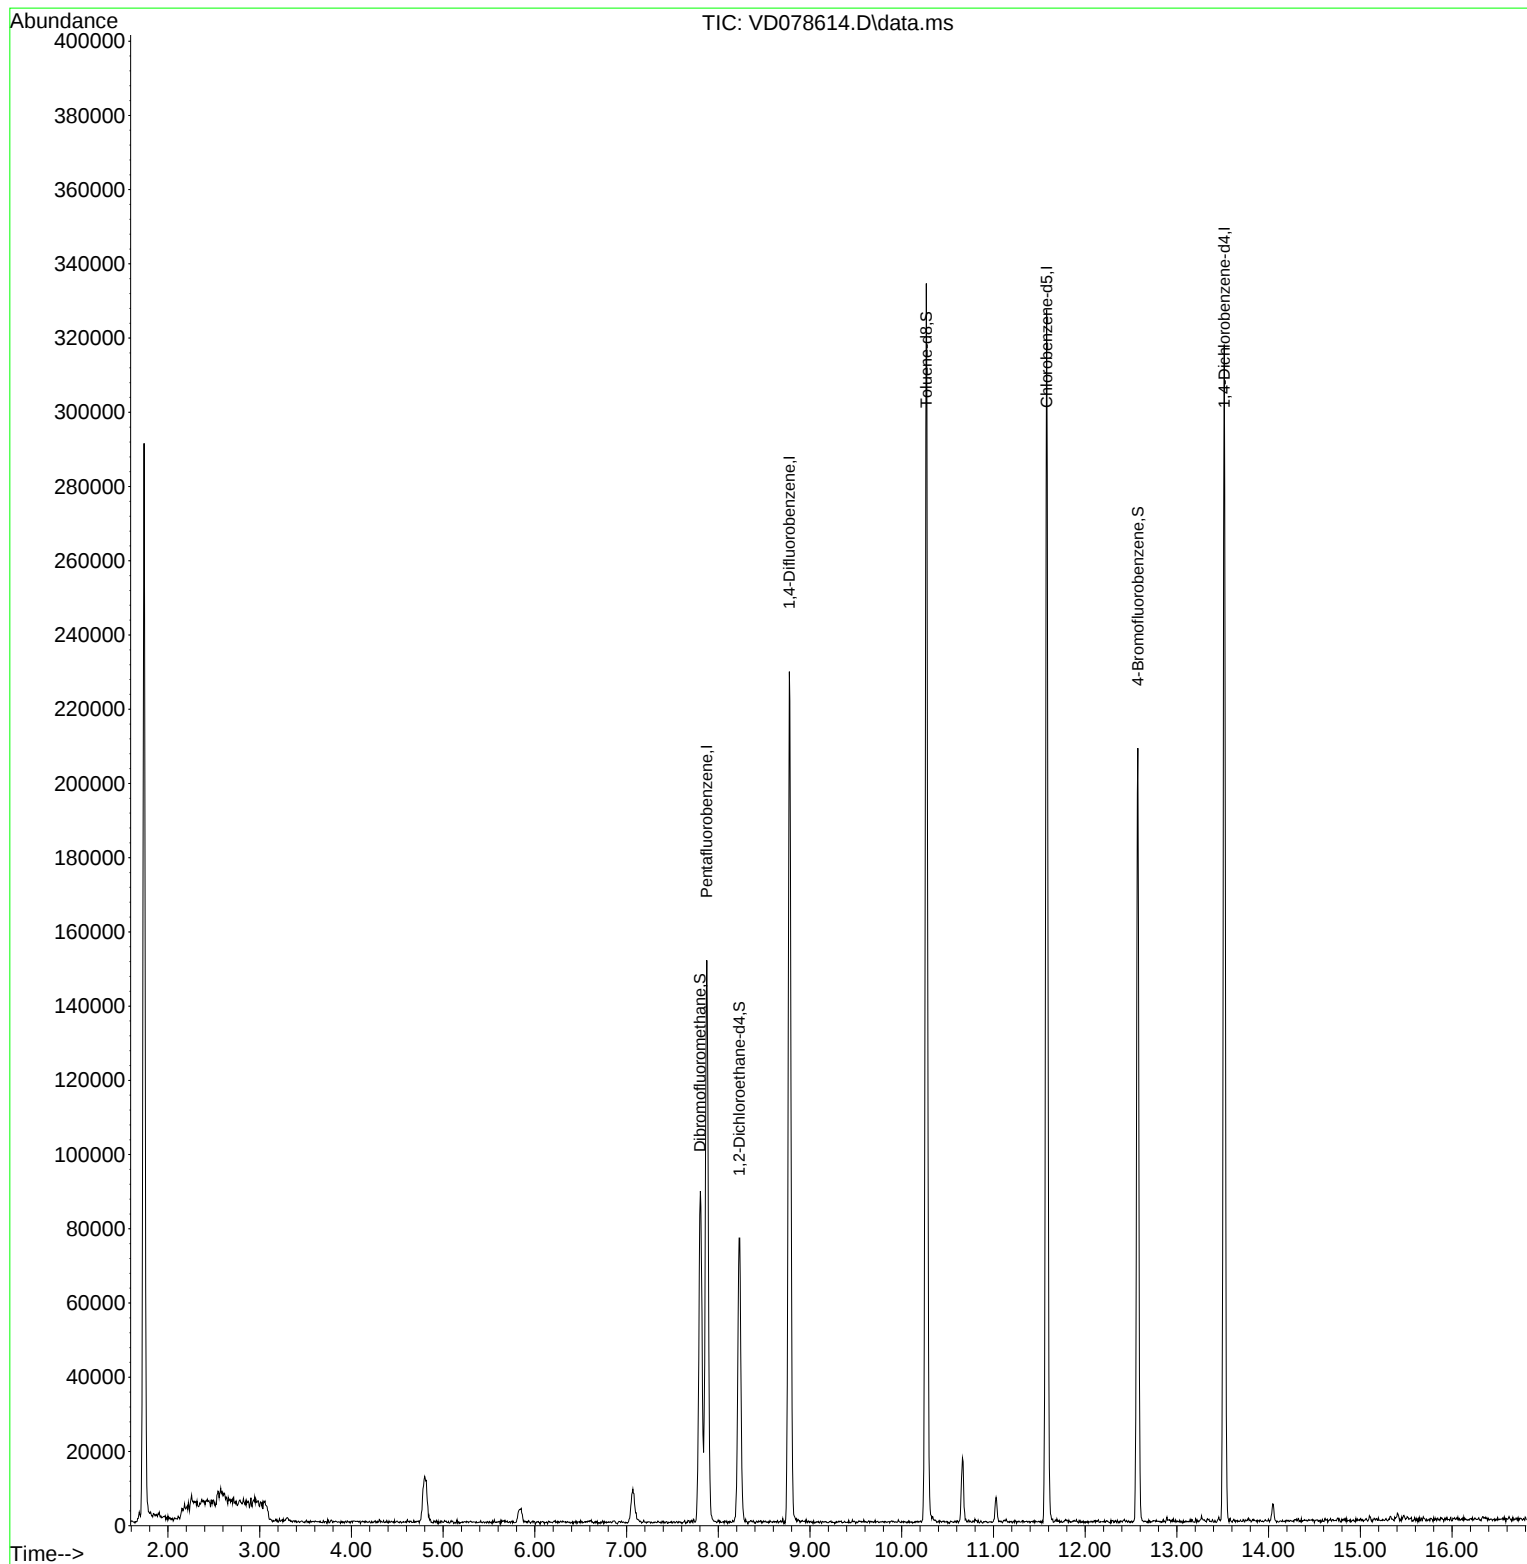


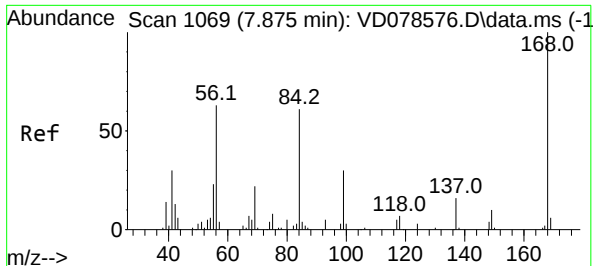

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1129
Delta R.T. 0.000 min
Lab File: VD078614.D
Acq: 08 Mar 2024 10:53




Instrument :
MSVOA_D
ClientSampleId :
VD0308SBL01


Tgt Ion:168 Resp: 120066
Ion Ratio Lower Upper
168 100
99 49.2 36.7 55.1

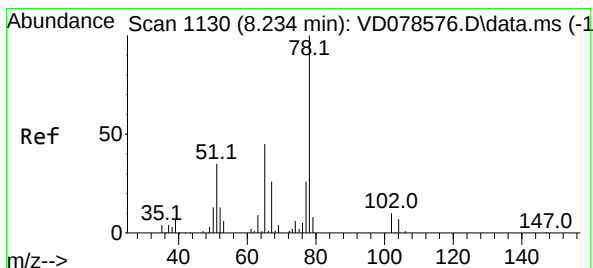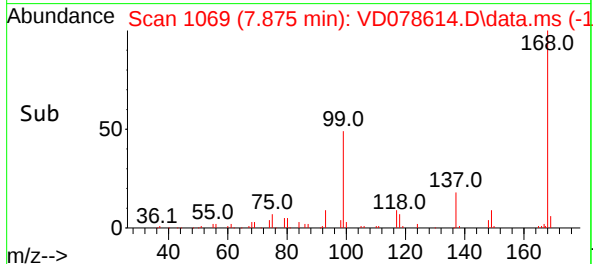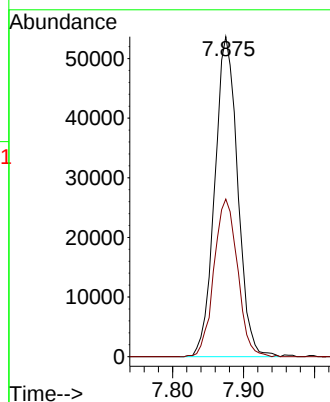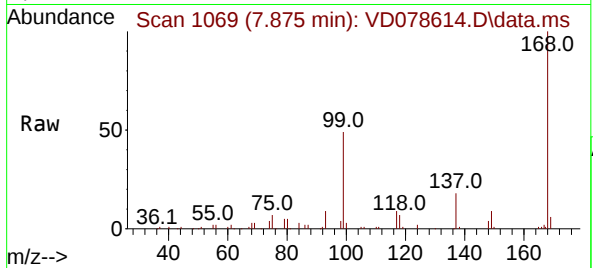

#33
1,2-Dichloroethane-d4
Concen: 50.807 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.006 min
Lab File: VD078614.D
Acq: 08 Mar 2024 10:53

Tgt Ion: 65 Resp: 60471
Ion Ratio Lower Upper
65 100
67 55.4 0.0 115.0

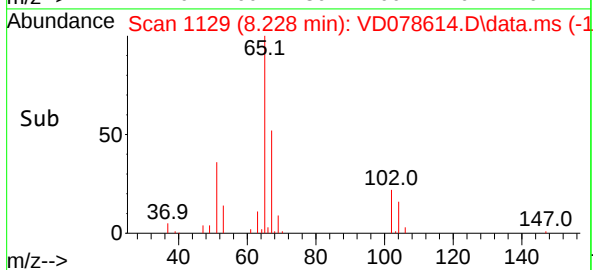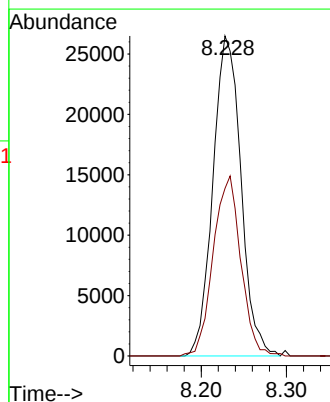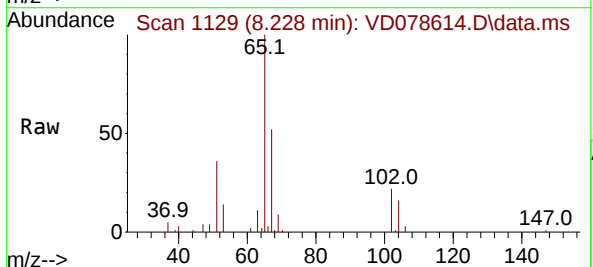

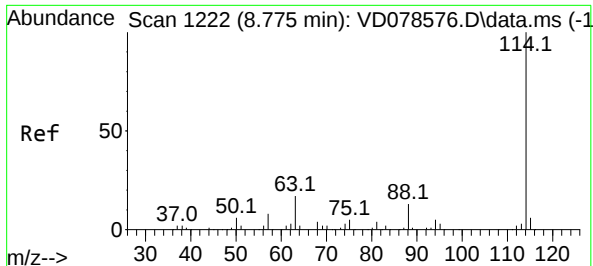

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 1

Delta R.T. 0.000 min

Lab File: VD078614.D

Acq: 08 Mar 2024 10:53

Instrument :

MSVOA_D

ClientSampleId :

VD0308SBL01





Tgt Ion:114 Resp: 214478

Ion Ratio Lower Upper

114 100

63 16.9 0.0 33.4

88 13.8 0.0 26.2

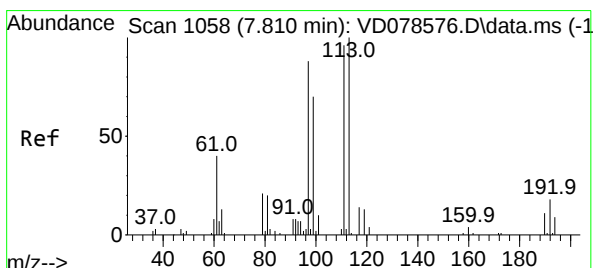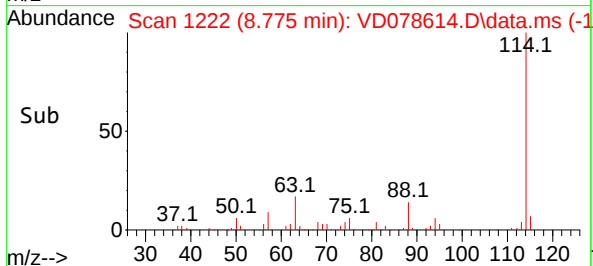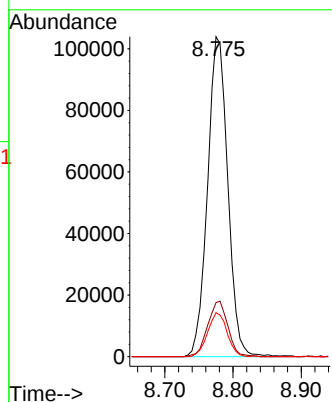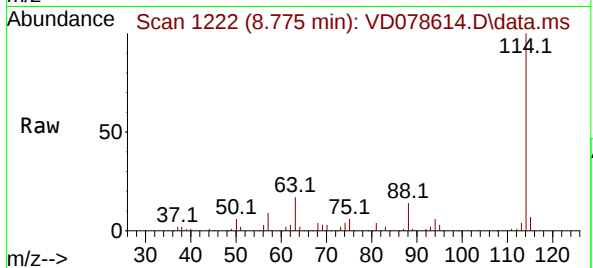

#35

Dibromofluoromethane

Concen: 47.248 ug/l

RT: 7.799 min Scan# 1056

Delta R.T. -0.012 min

Lab File: VD078614.D

Acq: 08 Mar 2024 10:53




Tgt Ion:113 Resp: 65919


Ion Ratio Lower Upper

113 100

111 103.0 84.7 127.1

192 19.3 16.8 25.2


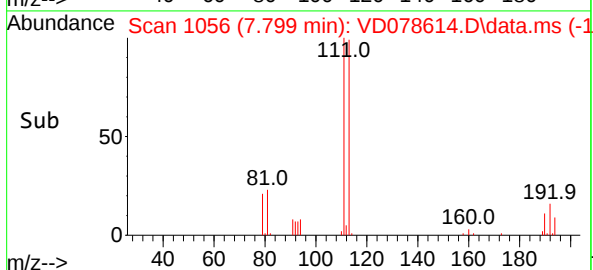
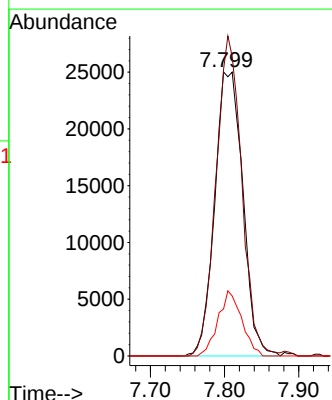
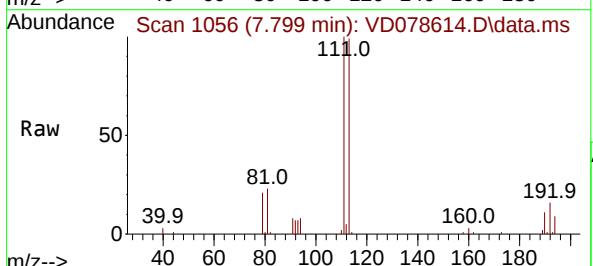


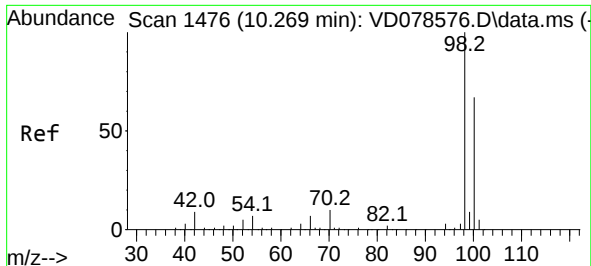

#50
Toluene-d8
Concen: 43.910 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD078614.D
Acq: 08 Mar 2024 10:53




Instrument :
MSVOA_D
ClientSampleId :
VD0308SBL01


Tgt Ion: 98 Resp: 238049
Ion Ratio Lower Upper
98 100
100 61.9 50.3 75.5

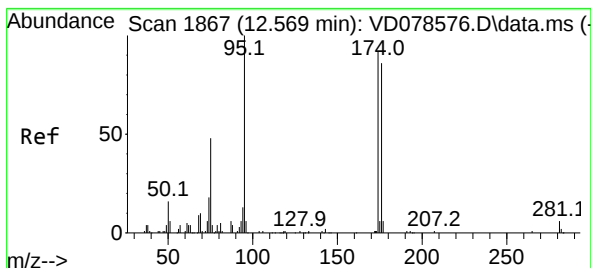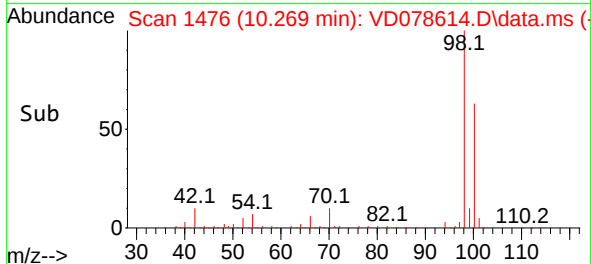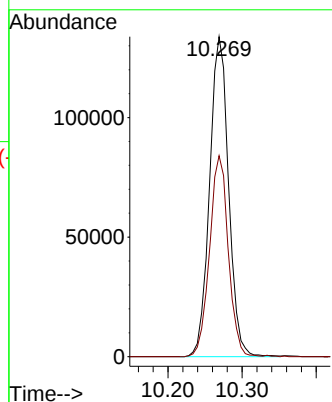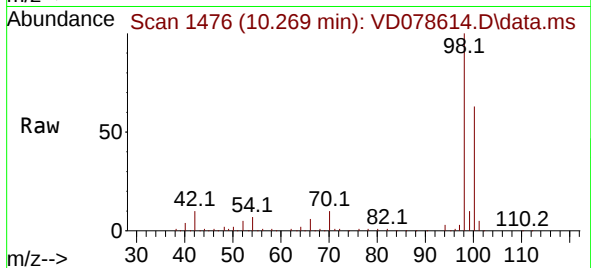

#62
4-Bromofluorobenzene
Concen: 39.496 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. 0.006 min
Lab File: VD078614.D
Acq: 08 Mar 2024 10:53

Tgt Ion: 95 Resp: 61157
Ion Ratio Lower Upper
95 100
174 94.7 0.0 201.8
176 88.6 0.0 191.8

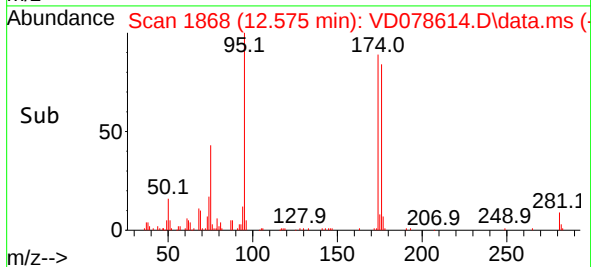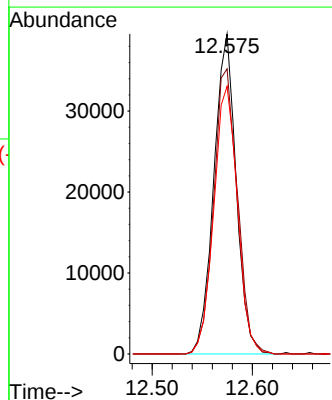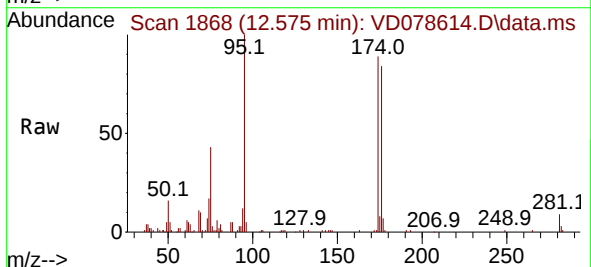

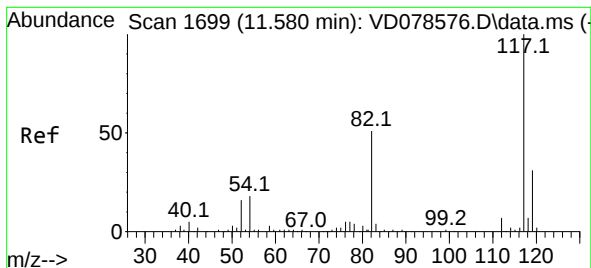

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.581 min Scan# 1

Delta R.T. 0.000 min

Lab File: VD078614.D

Acq: 08 Mar 2024 10:53

Instrument :

MSVOA_D

ClientSampleId :

VD0308SBL01





Tgt Ion:117 Resp: 195404

Ion Ratio Lower Upper

117 100

82 49.9 38.3 57.5

119 32.0 25.0 37.4

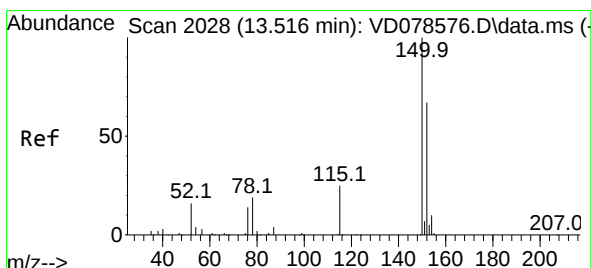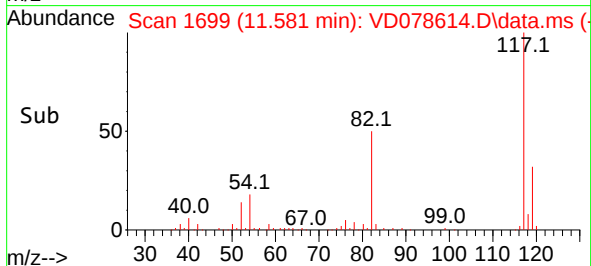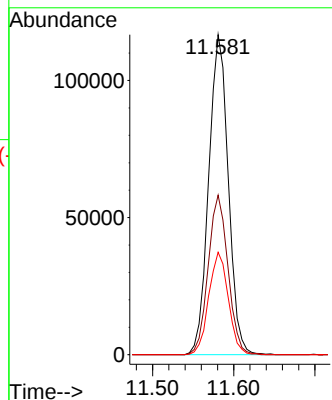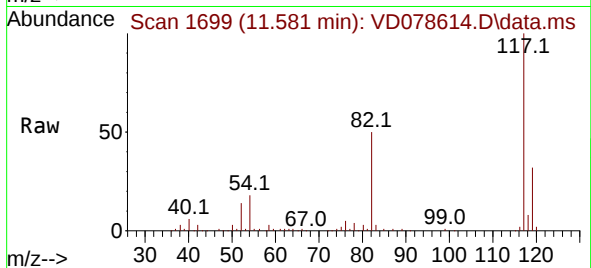

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.516 min Scan# 2028

Delta R.T. 0.000 min

Lab File: VD078614.D

Acq: 08 Mar 2024 10:53

Tgt Ion:152 Resp: 85870

Ion Ratio Lower Upper

152 100

115 53.3 27.1 81.3

150 159.6 0.0 353.6

