
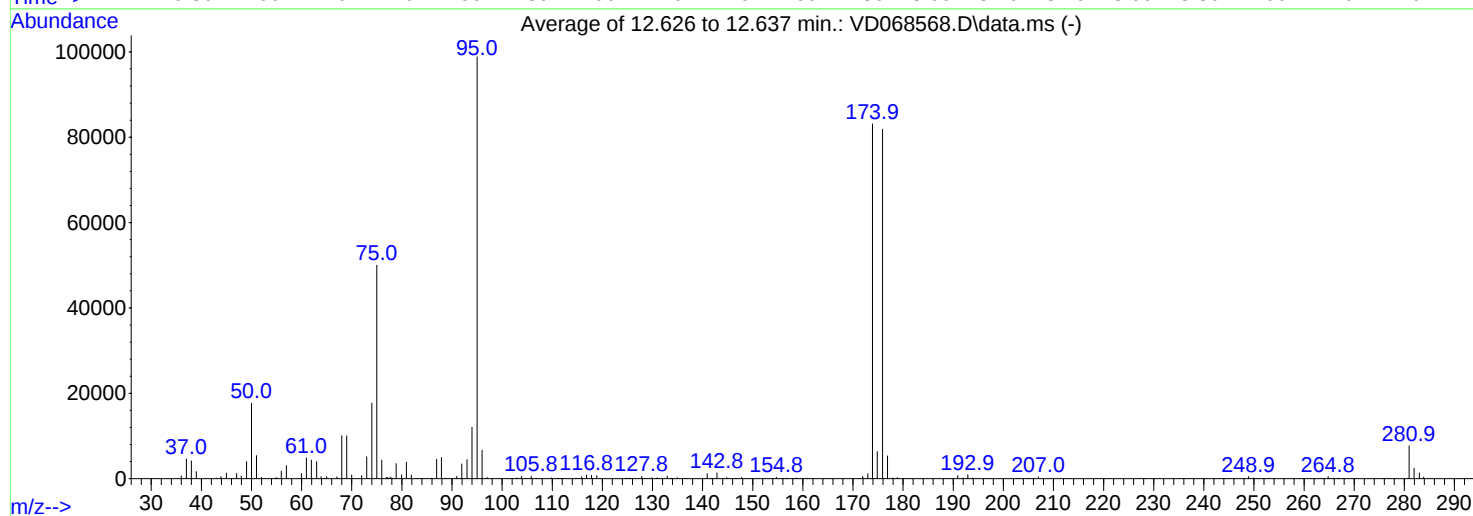


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD030921\  
 Data File : VD068568.D  
 Acq On : 09 Mar 2021 09:36  
 Operator : VA/SY  
 Sample : BFB  
 Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D022621S.M  
 Title : SW846 8260  
 Last Update : Fri Feb 26 14:04:14 2021

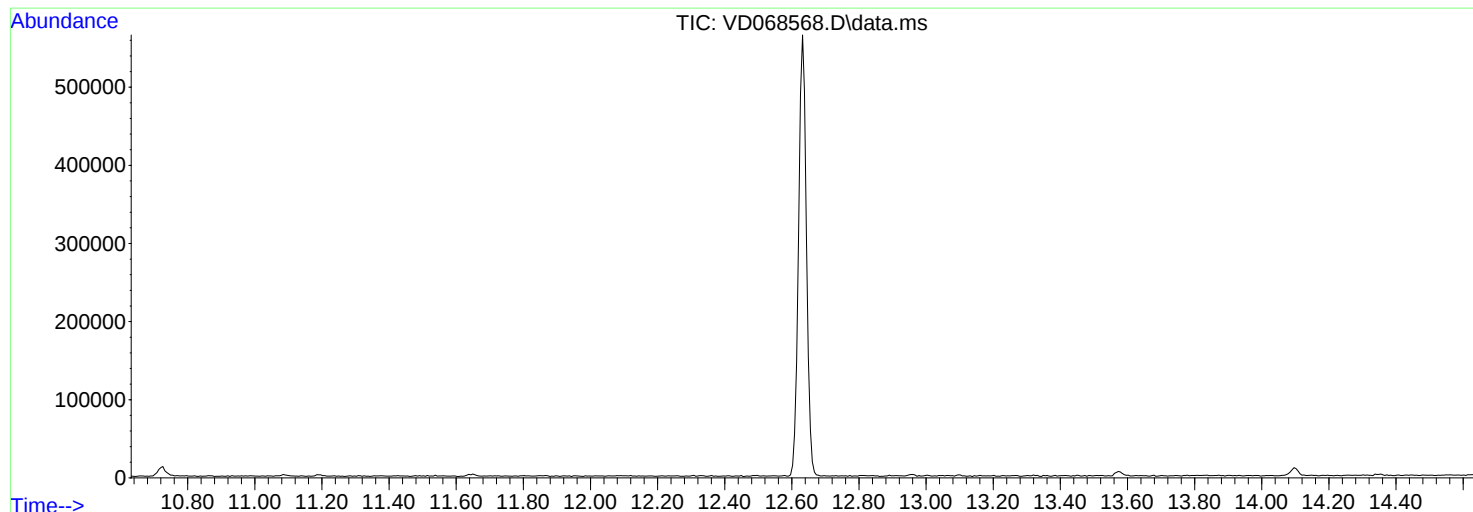

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 17.9         | 17677      | PASS                |
| 75             | 95              | 30              | 60              | 50.6         | 50035      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 98837      | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 6665       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.4          | 1181       | PASS                |
| 174            | 95              | 50              | 100             | 84.1         | 83109      | PASS                |
| 175            | 174             | 5               | 9               | 7.6          | 6323       | PASS                |
| 176            | 174             | 95              | 101             | 98.5         | 81880      | PASS                |
| 177            | 176             | 5               | 9               | 6.5          | 5336       | PASS                |