


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD031120\
Data File : VD065472.D
Acq On : 11 Mar 2020 10:21
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030420S.M
Title : SW846 8260
Last Update : Thu Mar 05 01:22:07 2020

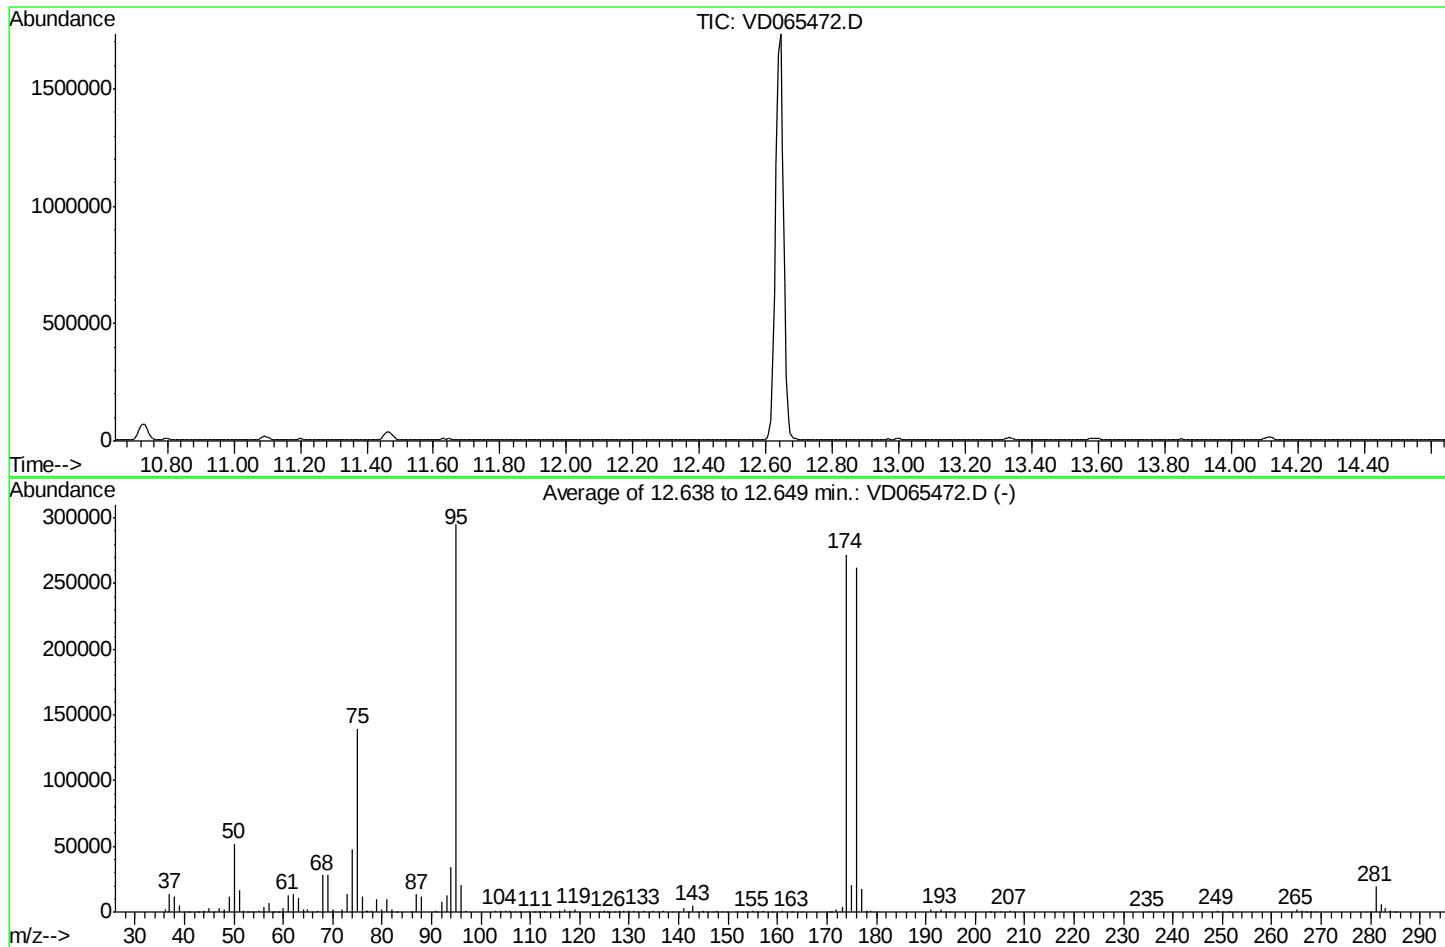

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	51970	PASS
75	95	30	60	47.3	139664	PASS
95	95	100	100	100.0	295146	PASS
96	95	5	9	6.9	20307	PASS
173	174	0.00	2	1.3	3464	PASS
174	95	50	100	92.3	272362	PASS
175	174	5	9	7.6	20648	PASS
176	174	95	101	96.4	262592	PASS
177	176	5	9	6.6	17328	PASS