
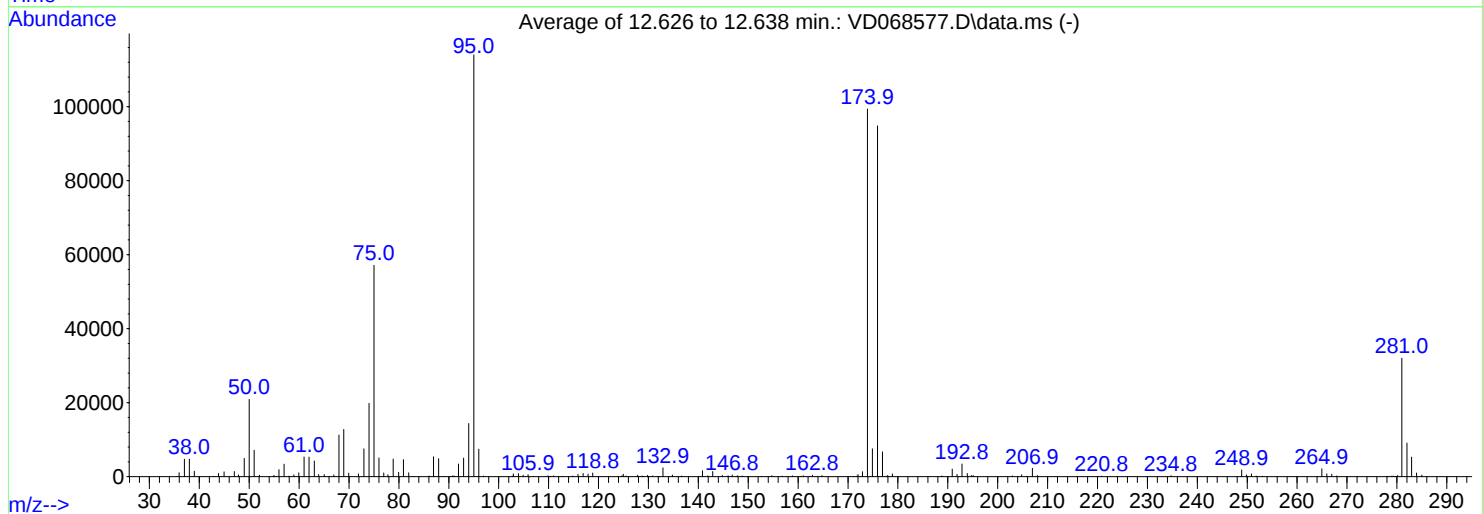


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031121\
Data File : VD068577.D
Acq On : 11 Mar 2021 09:04
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
Title : SW846 8260
Last Update : Fri Feb 26 14:04:14 2021

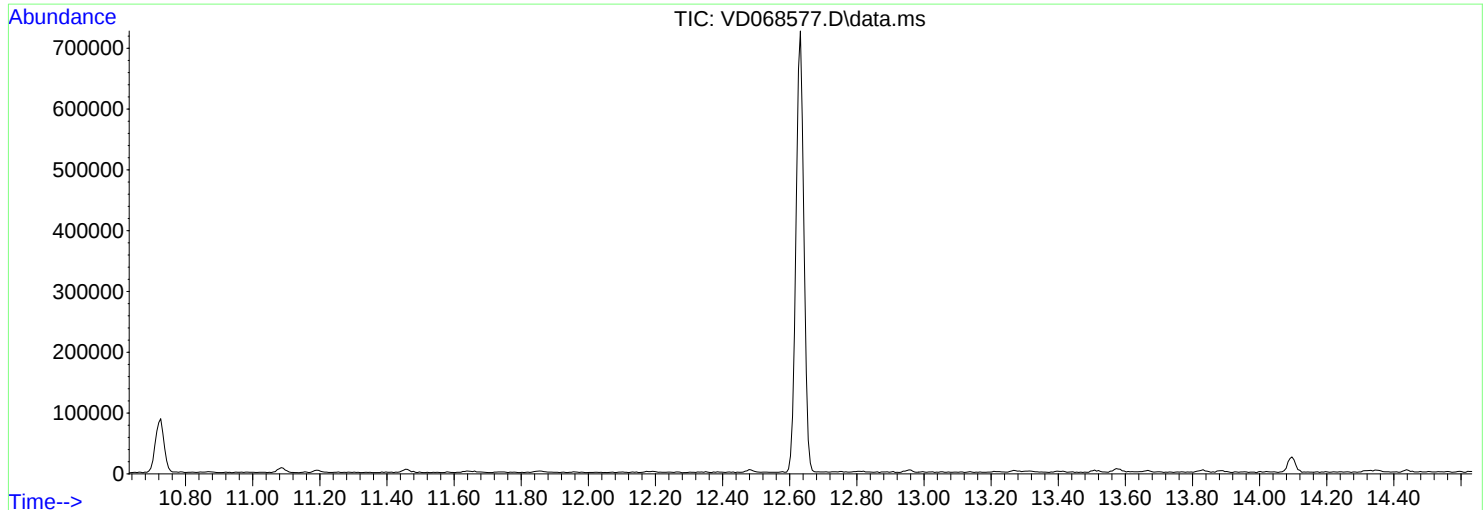

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	20891	PASS
75	95	30	60	50.1	57107	PASS
95	95	100	100	100.0	113997	PASS
96	95	5	9	6.5	7422	PASS
173	174	0.00	2	1.4	1359	PASS
174	95	50	100	87.2	99379	PASS
175	174	5	9	7.6	7517	PASS
176	174	95	101	95.4	94787	PASS
177	176	5	9	7.1	6686	PASS