


Methyl Iodide

Response Ratio

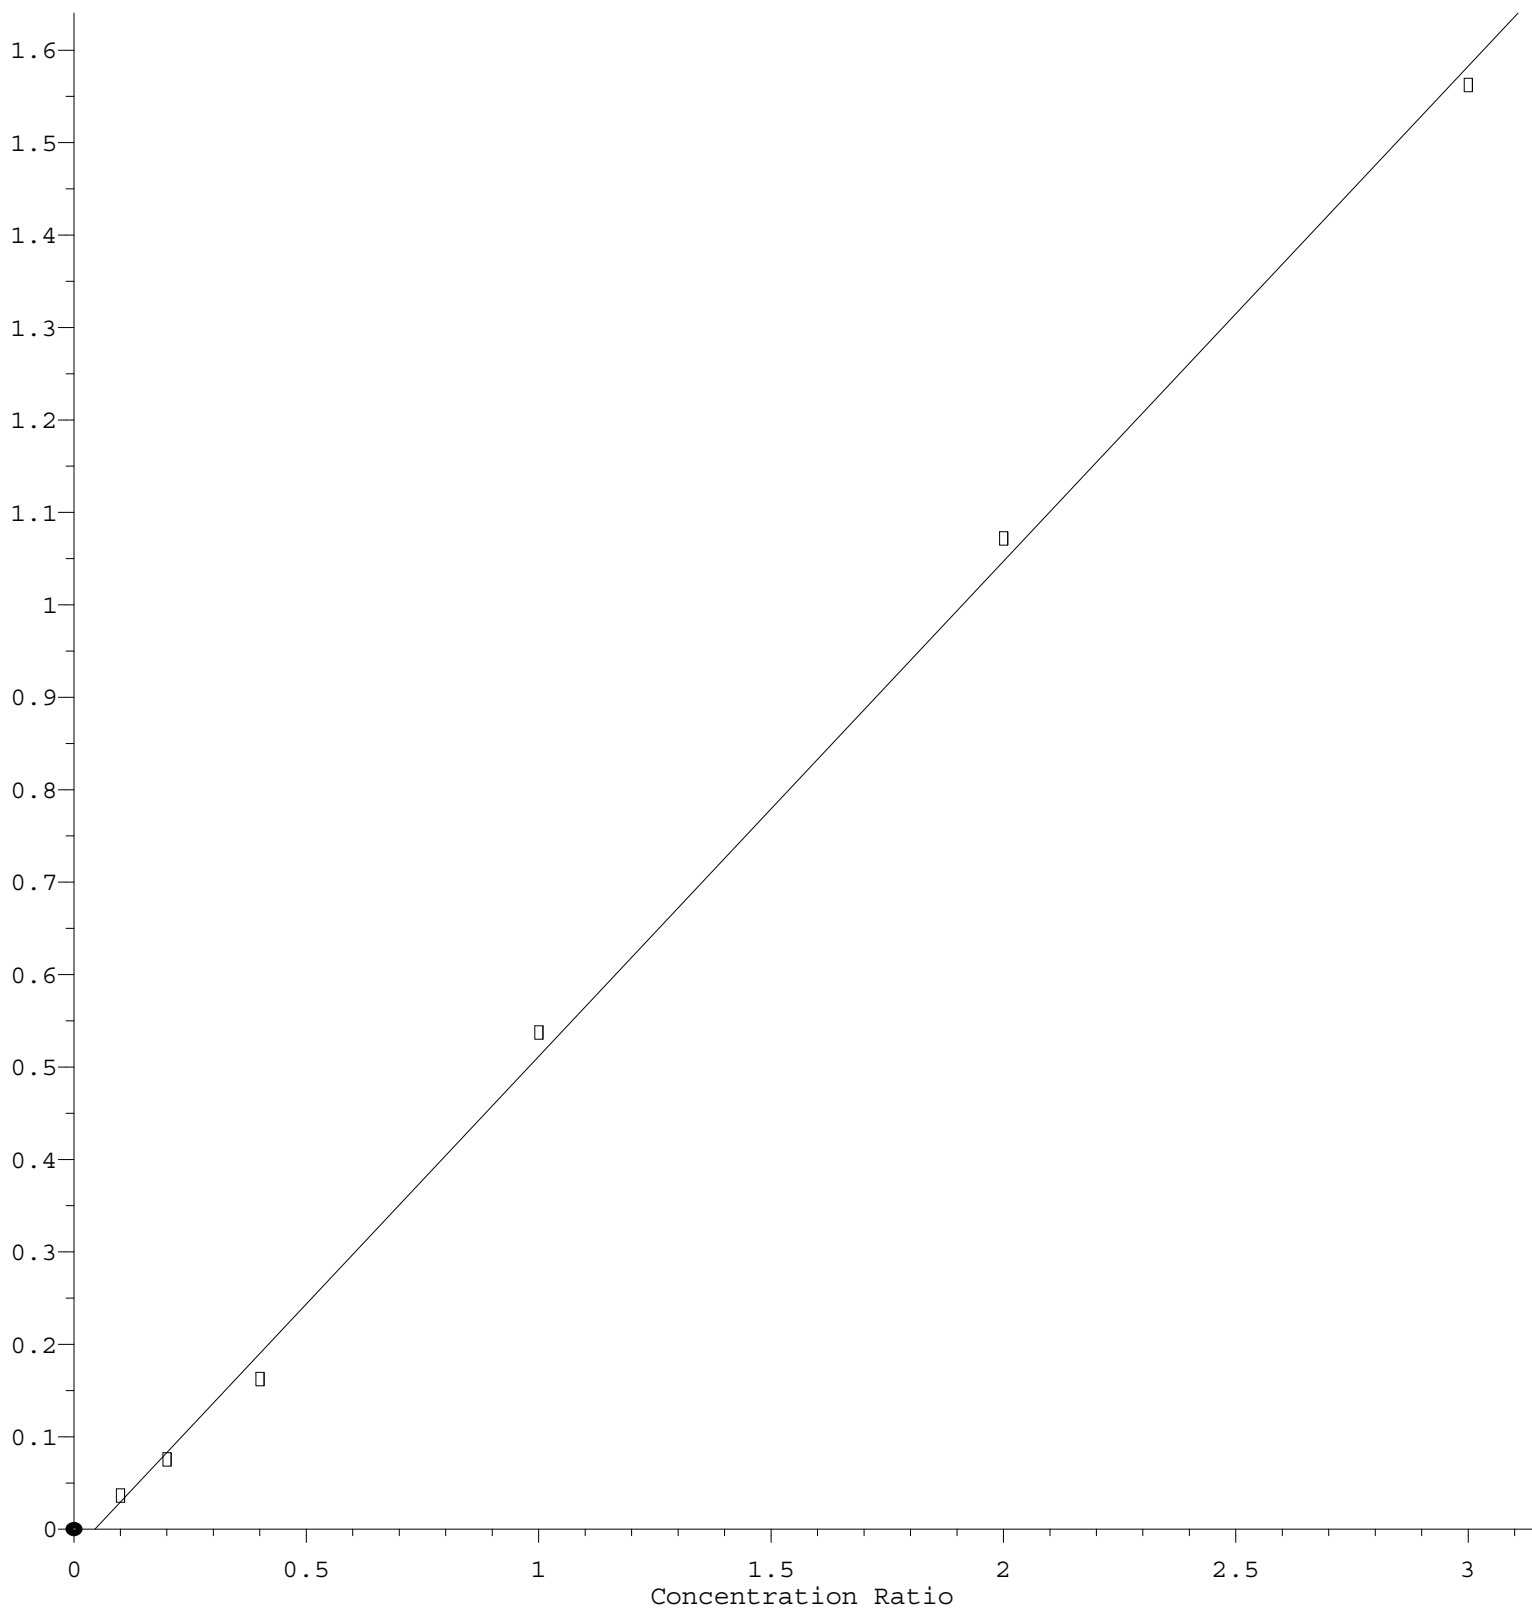

$$\text{Response} = 5.356\text{e-}001 * \text{Amt} - 2.385\text{e-}002$$


Coef of Det (r^2) = 0.998672 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D031122S.M

Calibration Table Last Updated: Mon Mar 14 05:18:06 2022

Carbon Disulfide

Response Ratio

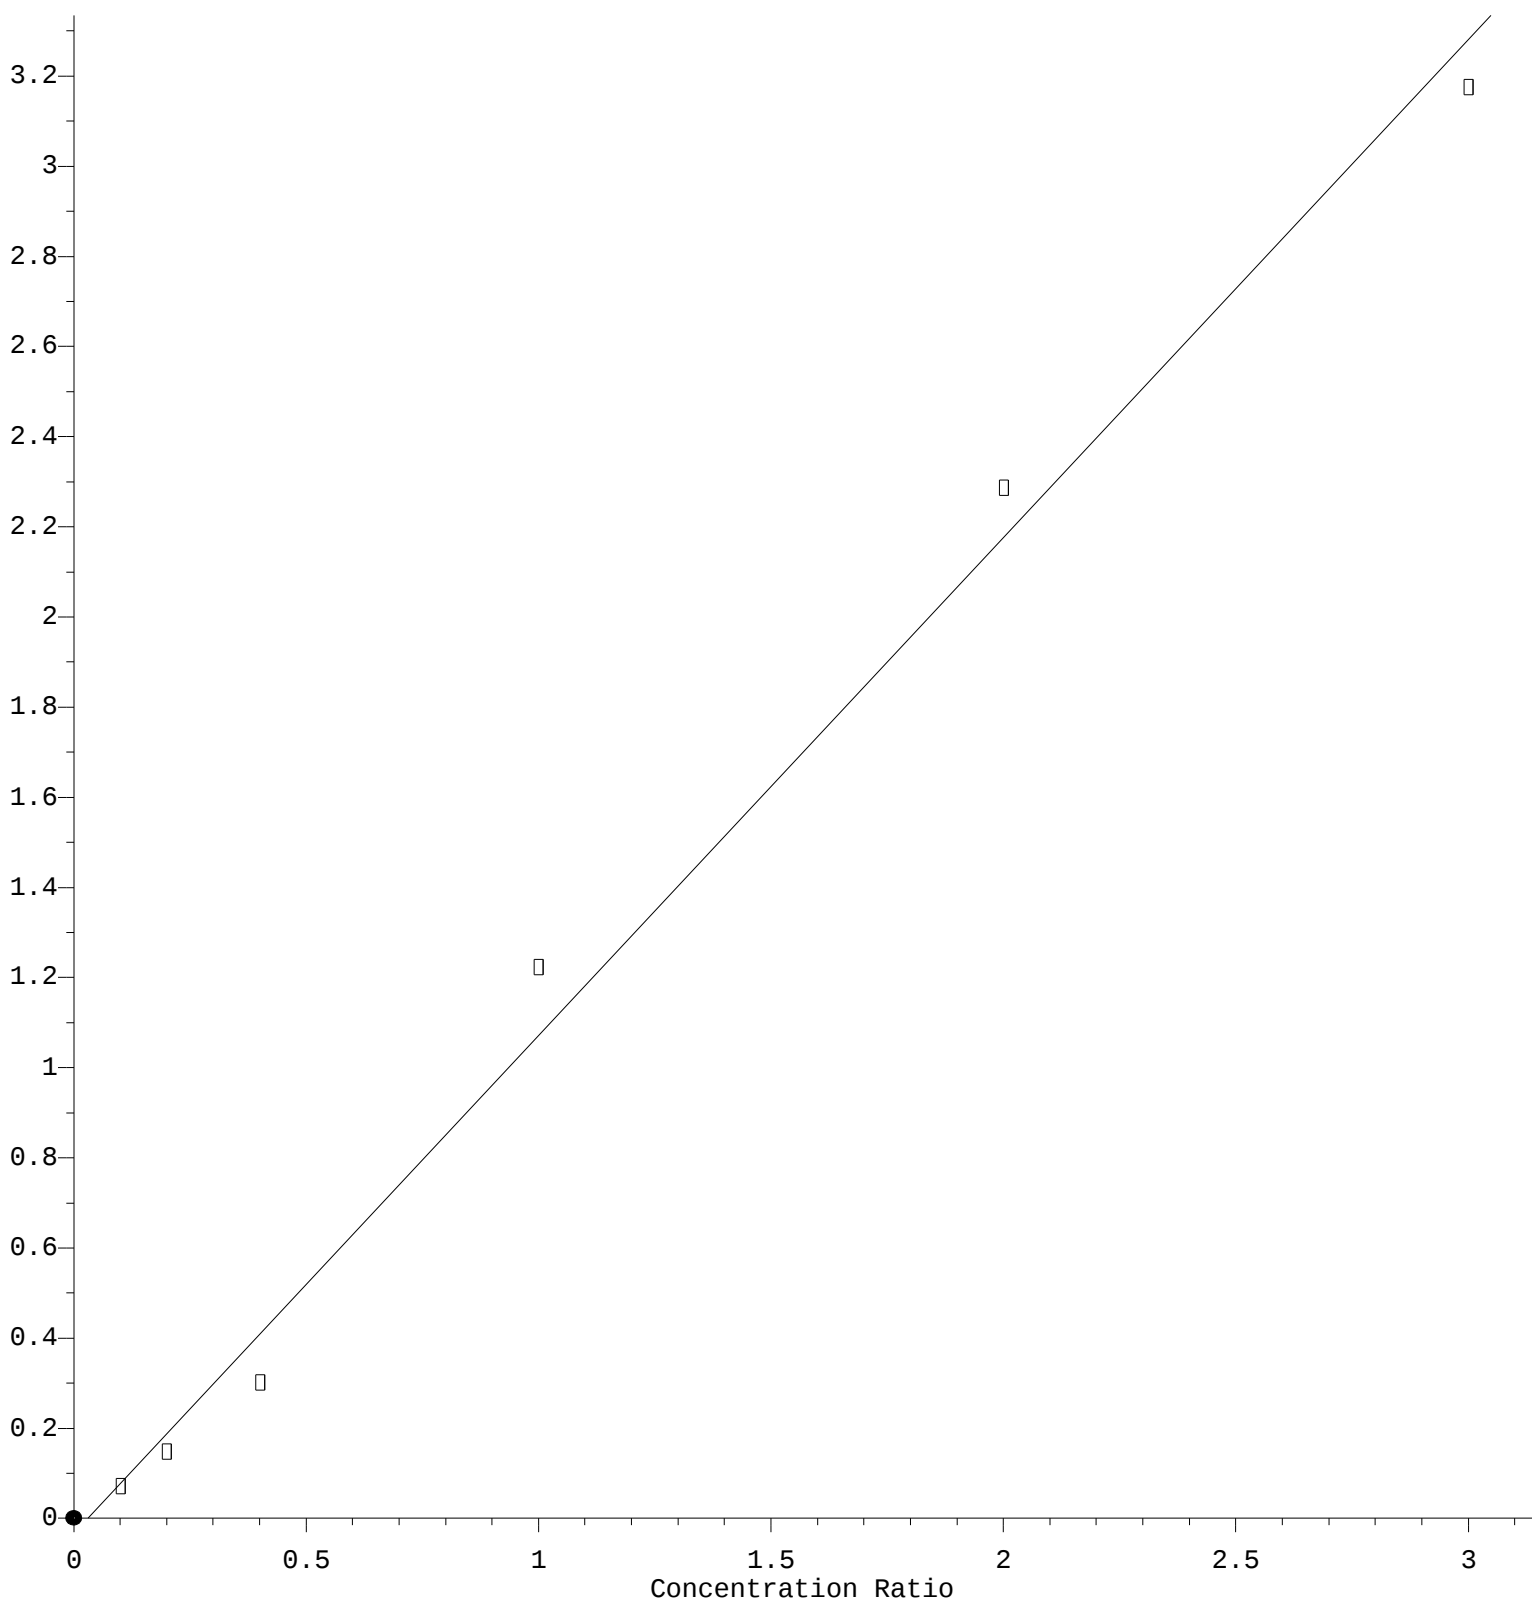

$$\text{Response} = 1.105\text{e}+000 * \text{Amt} - 3.316\text{e}-002$$


Coef of Det (r^2) = 0.992835 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M

Calibration Table Last Updated: Mon Mar 14 05:18:06 2022

Methylene Chloride

Response Ratio

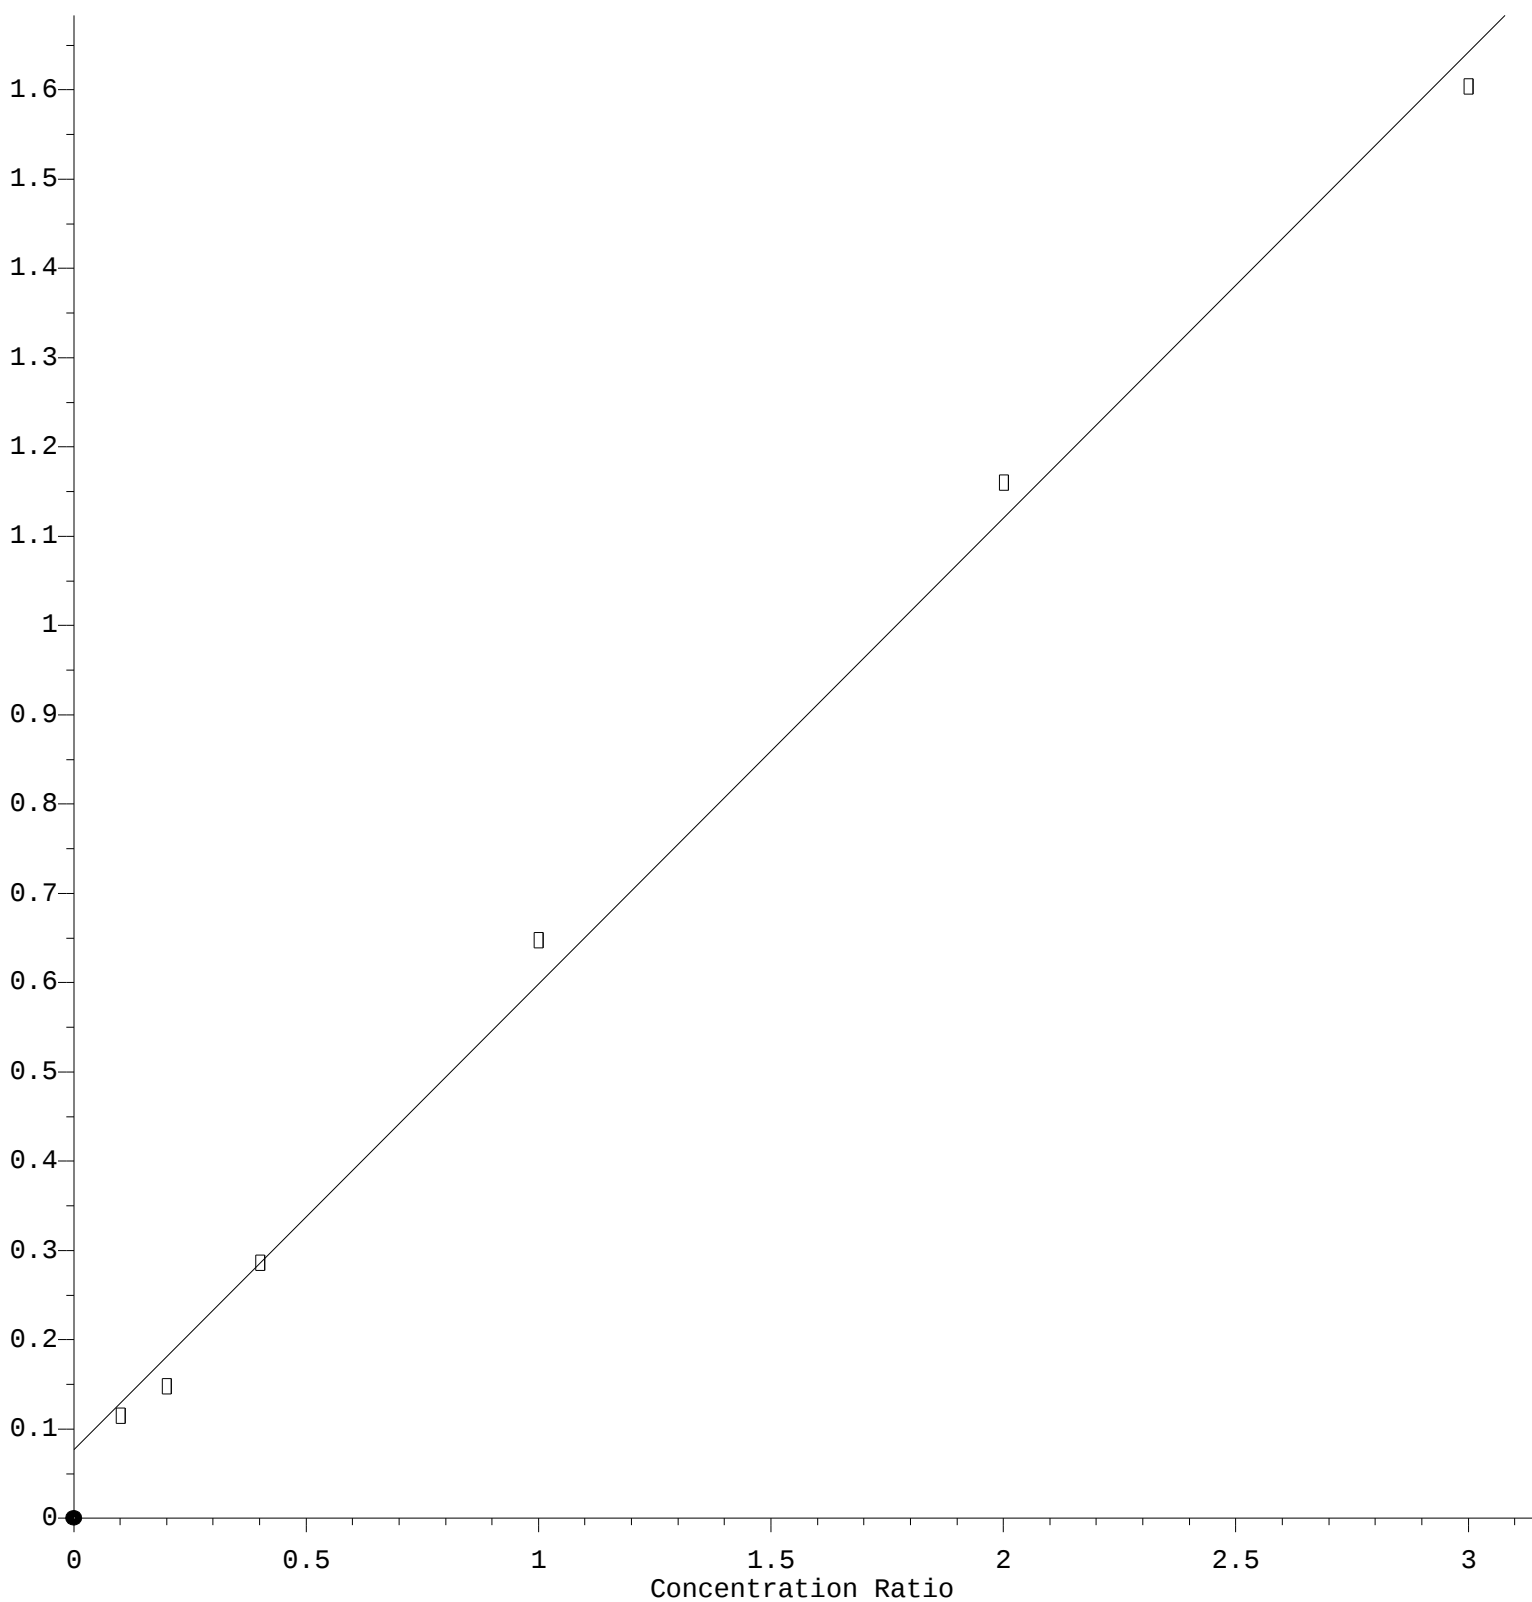

$$\text{Response} = 5.219\text{e-}001 * \text{Amt} + 7.694\text{e-}002$$

Coef of Det (r^2) = 0.996361 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M

Calibration Table Last Updated: Mon Mar 14 05:18:06 2022