


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031219\
Data File : VD061017.D
Acq On : 12 Mar 2019 10:07
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
Title : SW846 8260
Last Update : Fri Mar 08 02:35:39 2019

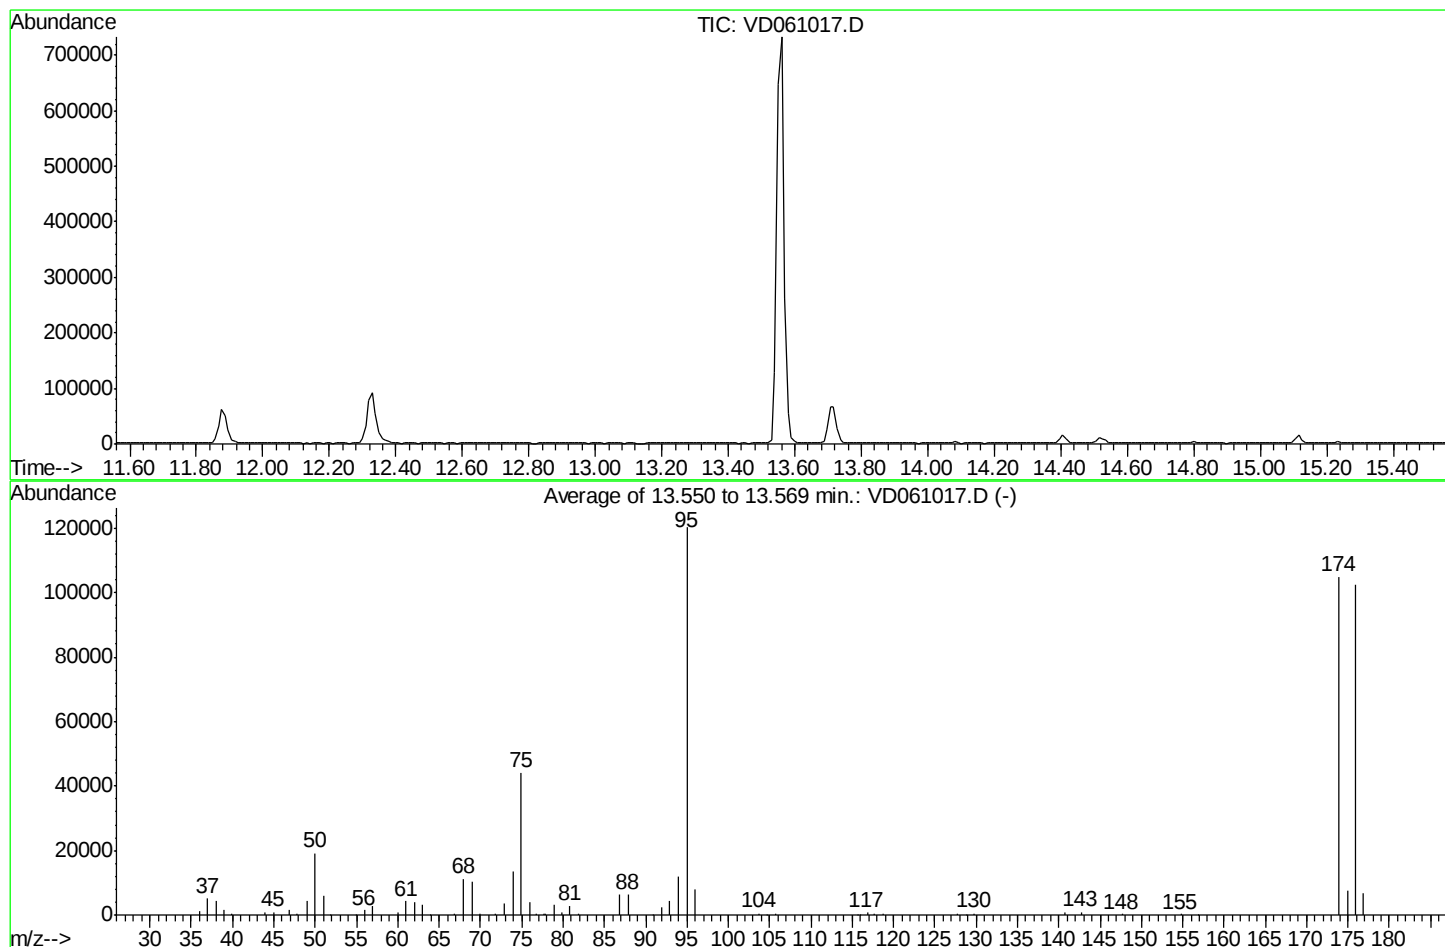

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	19244	PASS
75	95	30	60	36.7	44160	PASS
95	95	100	100	100.0	120242	PASS
96	95	5	9	6.5	7813	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.2	104821	PASS
175	174	5	9	7.1	7453	PASS
176	174	95	101	97.9	102610	PASS
177	176	5	9	6.5	6634	PASS