


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD031220\
 Data File : VD065482.D
 Acq On : 12 Mar 2020 09:42
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030420S.M
 Title : SW846 8260
 Last Update : Thu Mar 05 01:22:07 2020

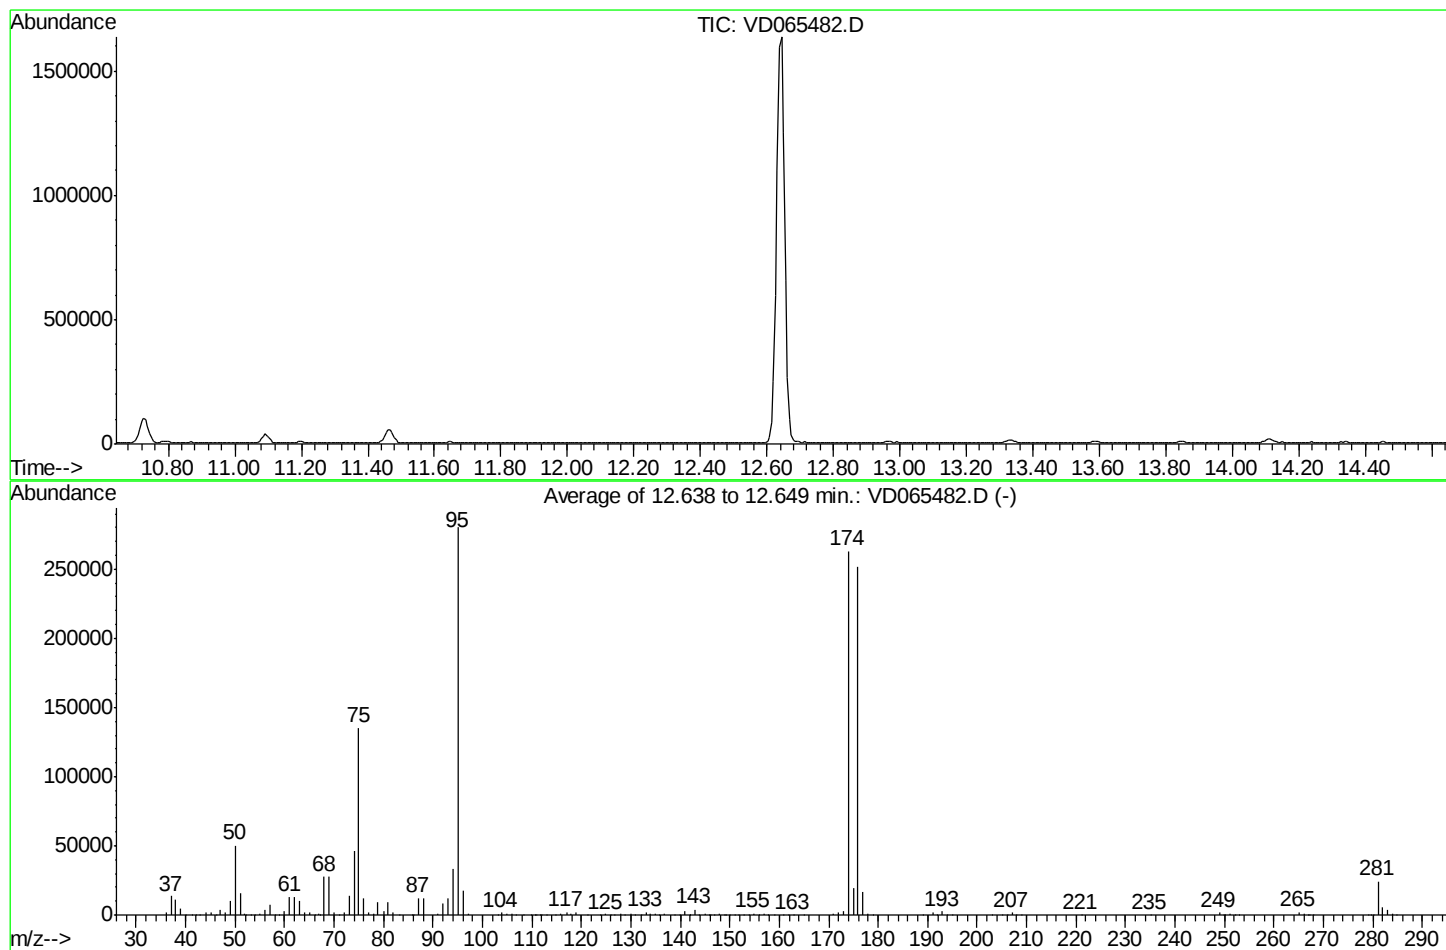

AutoFind: Scans 1822, 1823, 1824; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	50109	PASS
75	95	30	60	48.3	135368	PASS
95	95	100	100	100.0	280213	PASS
96	95	5	9	6.4	18059	PASS
173	174	0.00	2	1.2	3257	PASS
174	95	50	100	93.9	263189	PASS
175	174	5	9	7.4	19533	PASS
176	174	95	101	95.6	251605	PASS
177	176	5	9	6.6	16605	PASS