

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031221\
 Data File : VD068598.D
 Acq On : 12 Mar 2021 11:04
 Operator : VA/SY
 Sample : VD0312SBL02
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0312SBL02

Quant Time: Mar 12 23:33:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 26 14:04:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.985	168	387846	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	675439	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.643	117	662596	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	364848	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	190830	49.24	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	98.48%
35) Dibromofluoromethane	7.914	113	208723	51.30	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.60%
50) Toluene-d8	10.344	98	846092	52.21	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.42%
62) 4-Bromofluorobenzene	12.632	95	296528	56.77	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	113.54%
Target Compounds						
					Qvalue	
10) Methyl Iodide	4.309	142	407	2.70	ug/l #	38
11) Tert butyl alcohol	5.179	59	578	2.79	ug/l #	74
16) Acetone	4.167	43	1109	1.80	ug/l #	71
31) Cyclohexane	7.985	56	8916	1.27	ug/l #	48
36) 1,1-Dichloropropene	7.979	75	29337	4.57	ug/l #	47
38) Carbon Tetrachloride	7.985	117	36916	6.12	ug/l #	17
76) 1,2,3-Trichloropropane	12.632	75	151634	46.82	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.632	75	151634	109.25	ug/l #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031221\
Data File : VD068598.D
Acq On : 12 Mar 2021 11:04
Operator : VA/SY
Sample : VD0312SBL02
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL02

Quant Time: Mar 12 23:33:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
Quant Title : SW846 8260
QLast Update : Fri Feb 26 14:04:14 2021
Response via : Initial Calibration




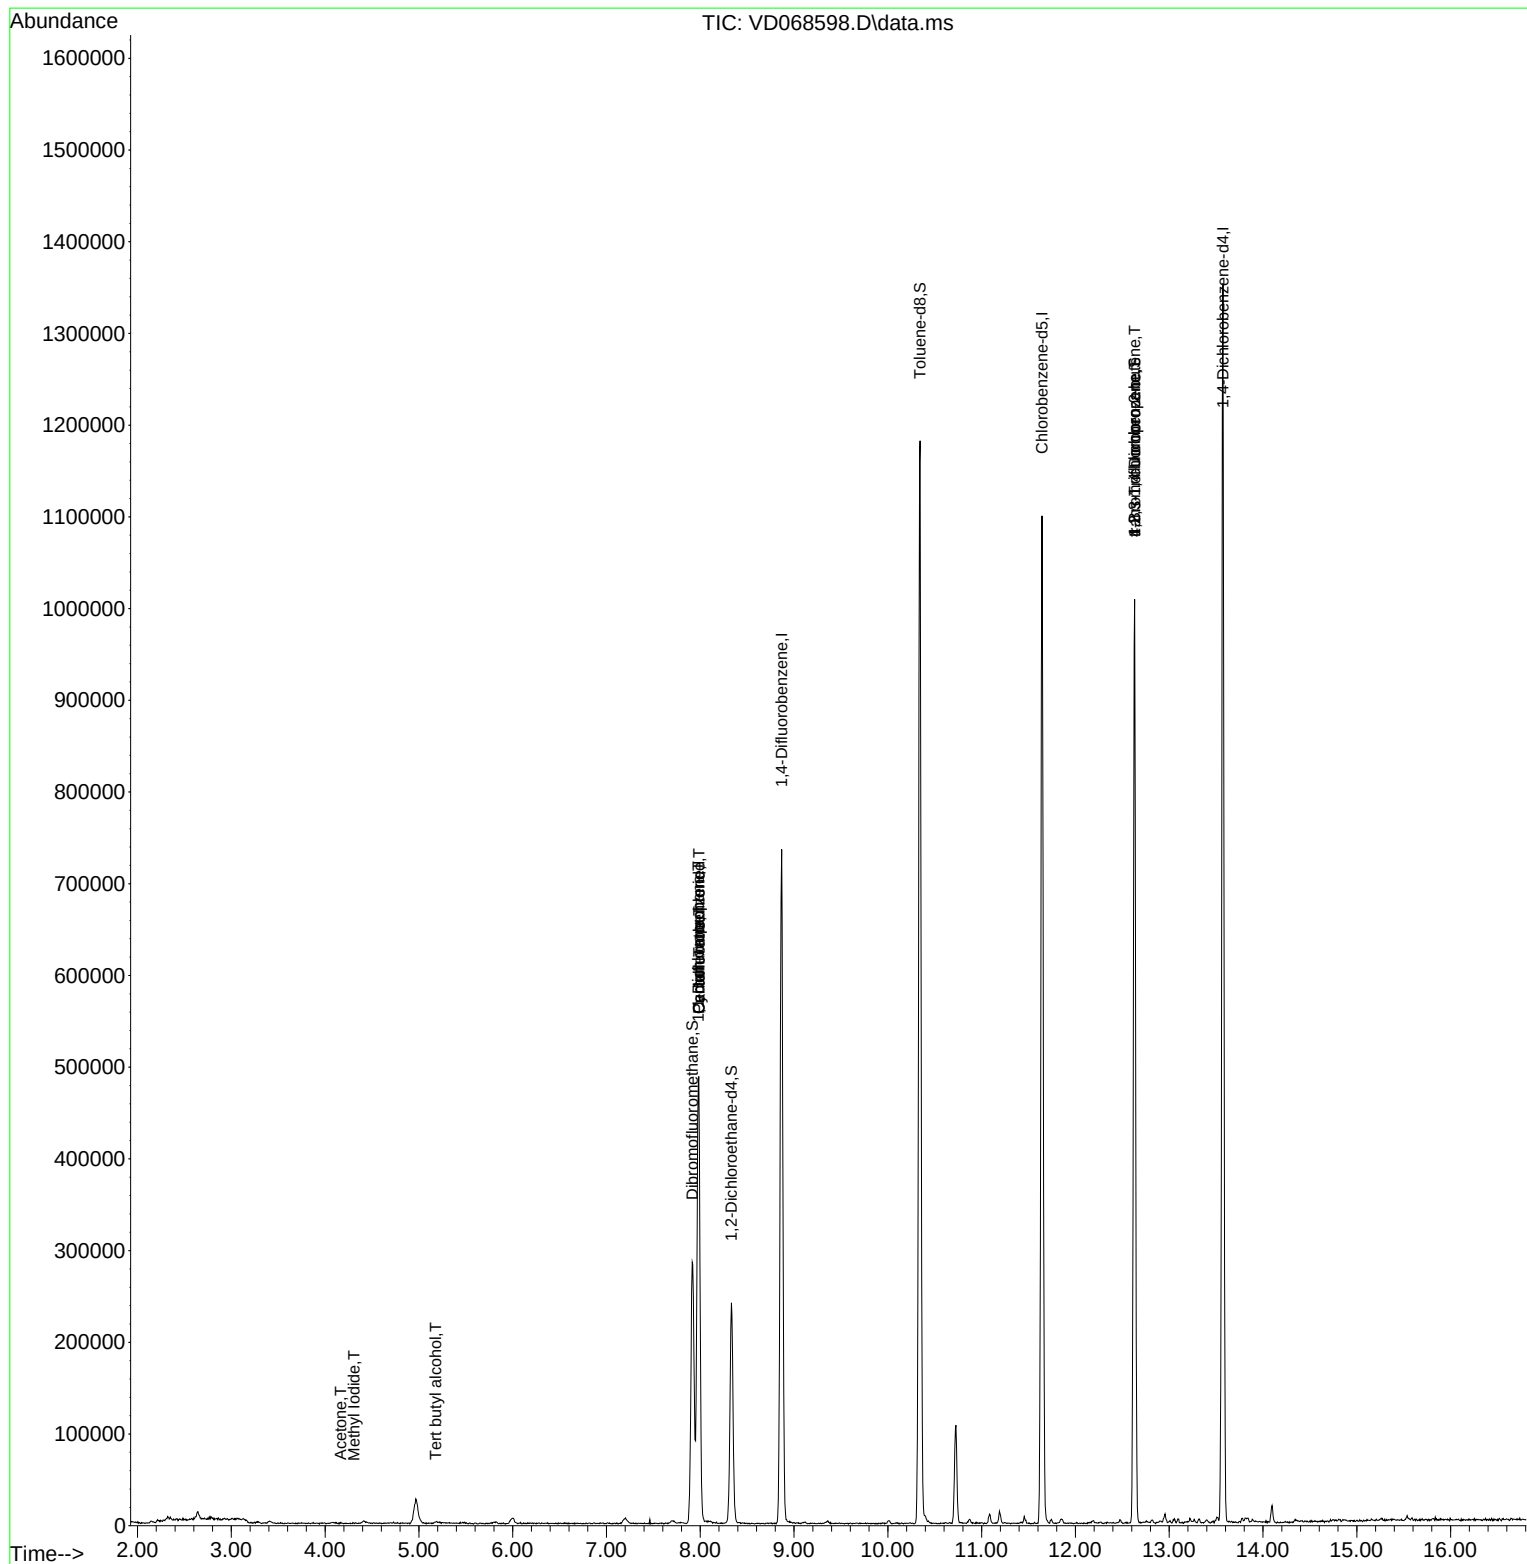


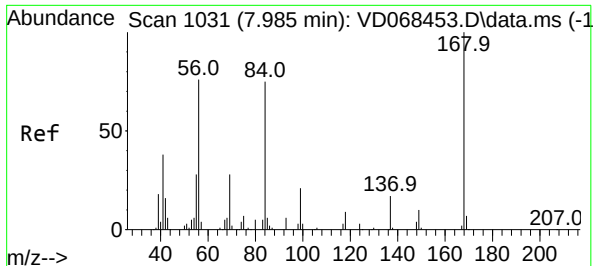

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.985 min Scan# 1031
Delta R.T. -0.000 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04




Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL02


Tgt Ion:168 Resp: 387846
Ion Ratio Lower Upper
168 100
99 52.1 43.5 65.3

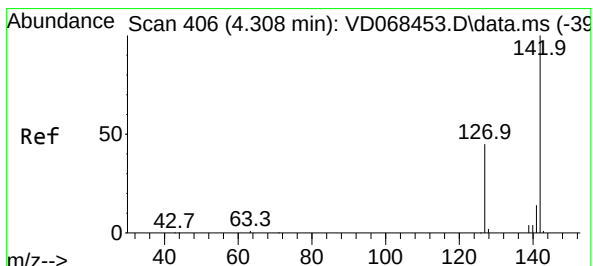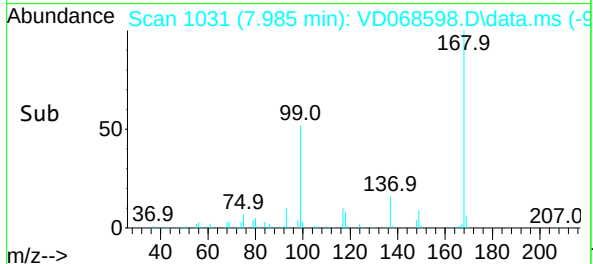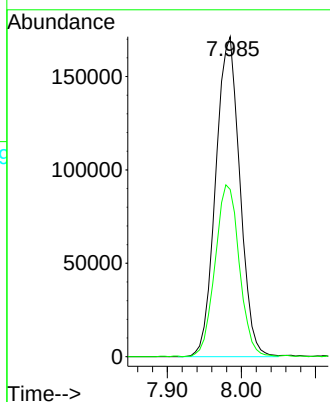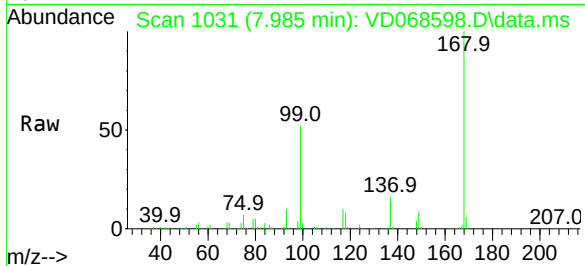

#10
Methyl Iodide
Concen: 2.70 ug/l
RT: 4.309 min Scan# 406
Delta R.T. 0.001 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04

Tgt Ion:142 Resp: 407
Ion Ratio Lower Upper
142 100
127 0.0 37.9 56.9#
141 0.0 11.5 17.3#


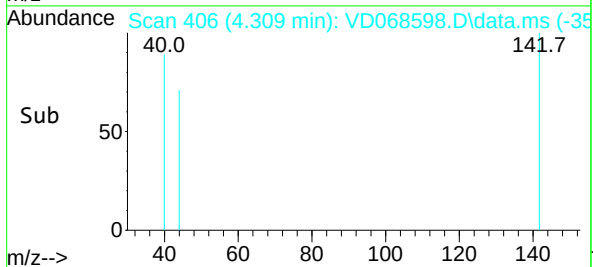
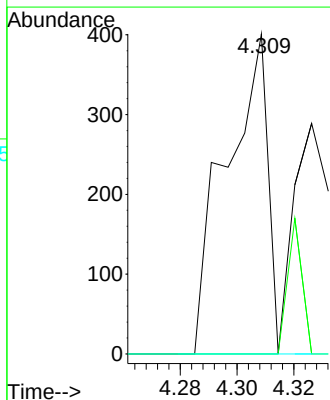
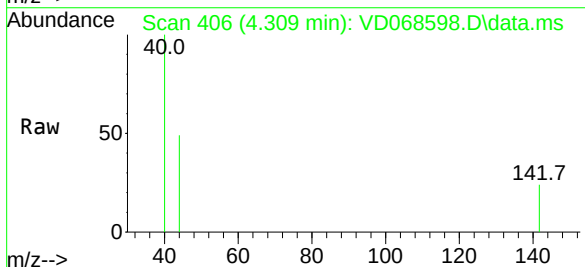


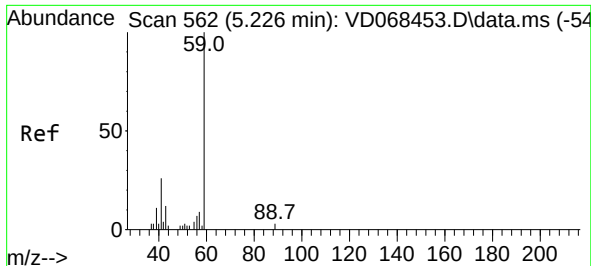

#11
Tert butyl alcohol
Concen: 2.79 ug/l
RT: 5.179 min Scan# 554
Delta R.T. -0.047 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04




Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL02


Tgt Ion: 59 Resp: 578
Ion Ratio Lower Upper
59 100
57 0.0 7.4 11.2#

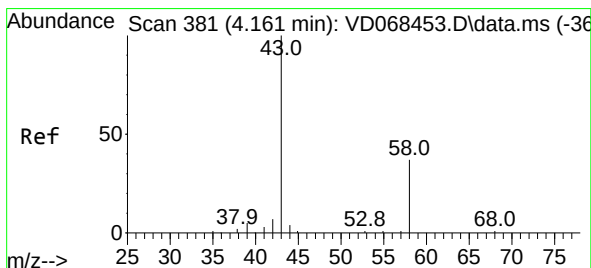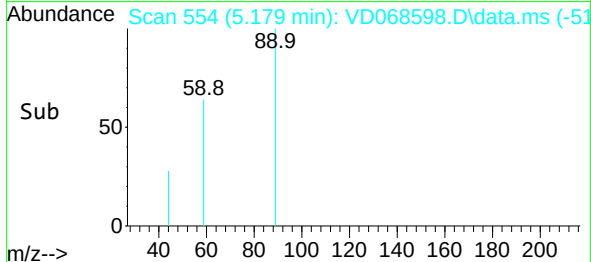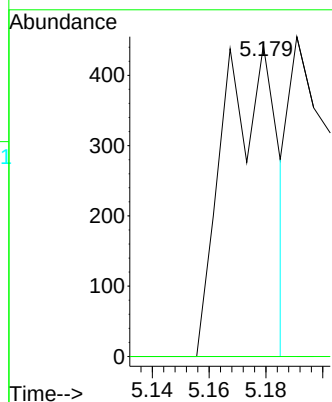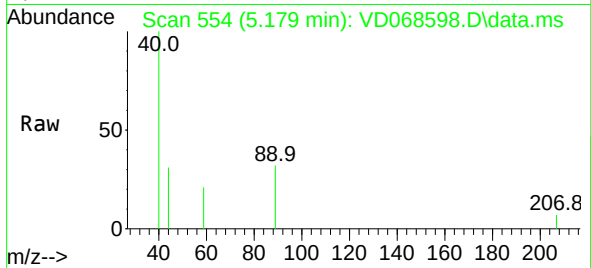

#16
Acetone
Concen: 1.80 ug/l
RT: 4.167 min Scan# 382
Delta R.T. 0.006 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04

Tgt Ion: 43 Resp: 1109
Ion Ratio Lower Upper
43 100
58 46.0 24.2 36.4#


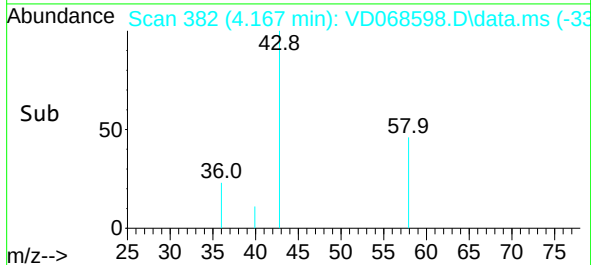
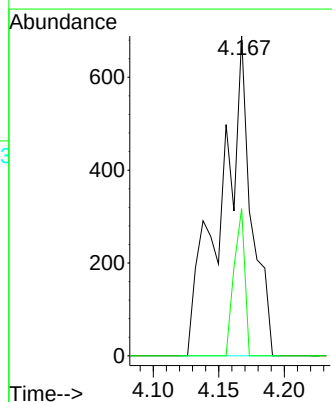
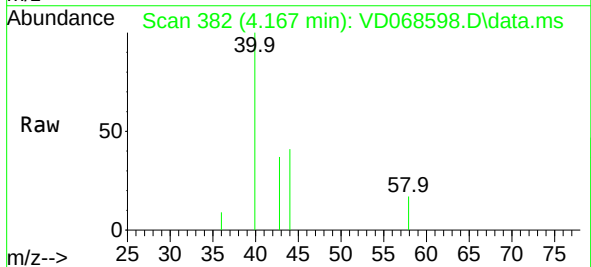


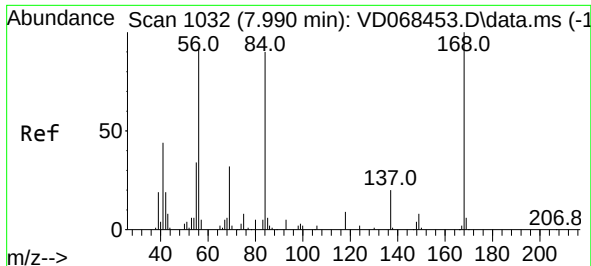

#31
Cyclohexane
Concen: 1.27 ug/l
RT: 7.985 min Scan# 1031
Delta R.T. -0.006 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04




Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL02


Tgt Ion: 56 Resp: 8916
Ion Ratio Lower Upper
56 100
69 131.5 30.1 45.1#
84 116.7 82.1 123.1

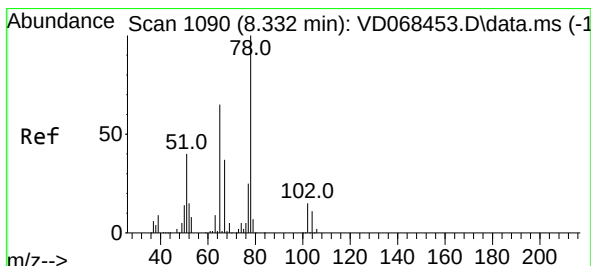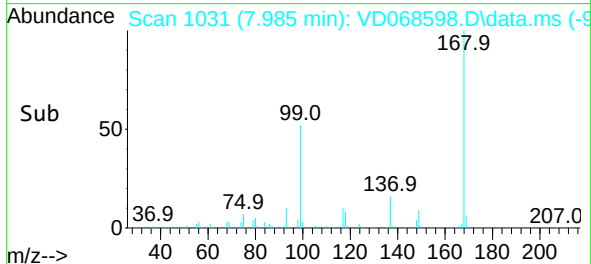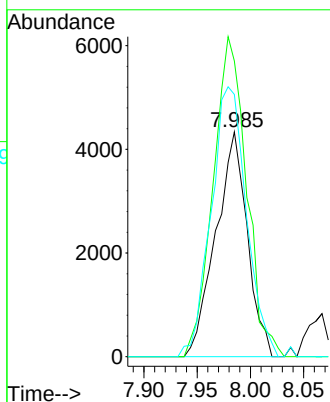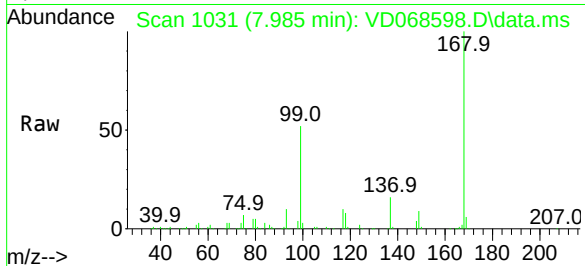

#33
1,2-Dichloroethane-d4
Concen: 49.24 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. 0.000 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04

Tgt Ion: 65 Resp: 190830
Ion Ratio Lower Upper
65 100
67 52.5 0.0 105.0


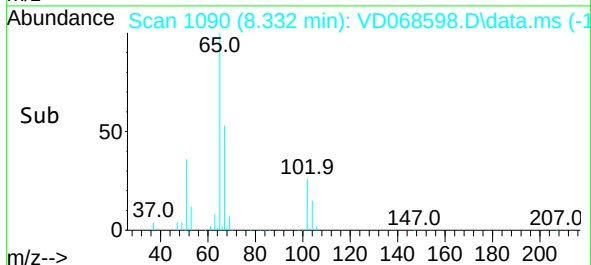
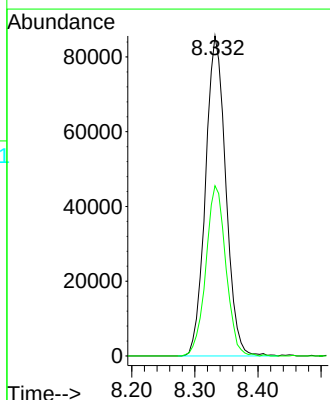
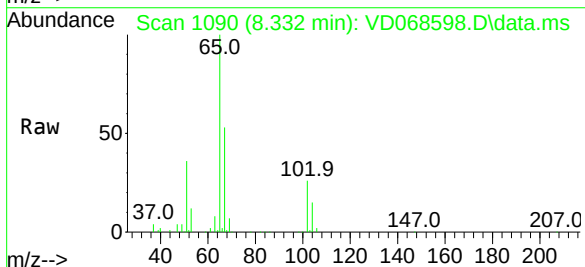


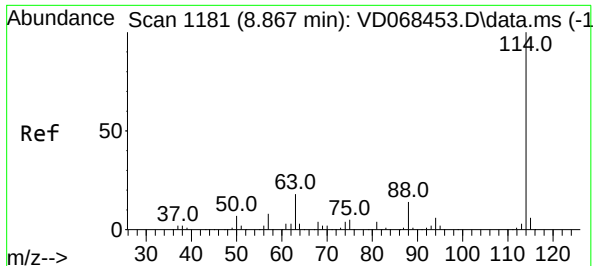

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04




Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL02


Tgt Ion:114 Resp: 675439
Ion Ratio Lower Upper
114 100
63 18.3 0.0 34.8
88 14.5 0.0 31.6

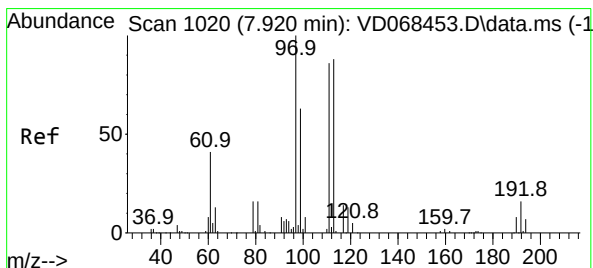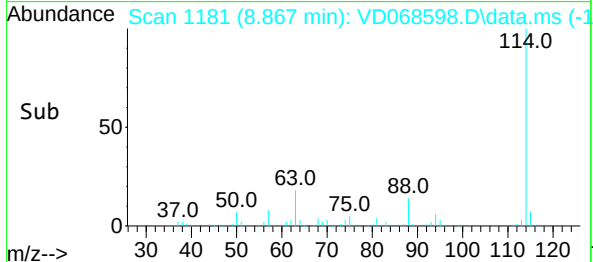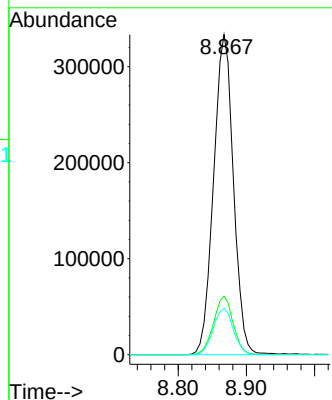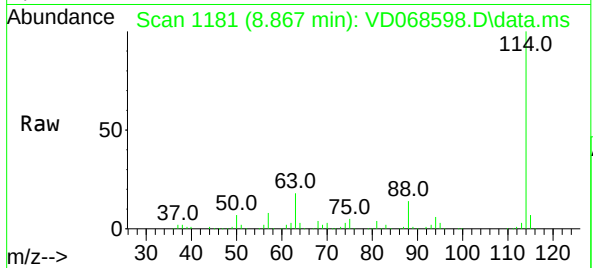

#35
Dibromofluoromethane
Concen: 51.30 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.006 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04

Tgt Ion:113 Resp: 208723
Ion Ratio Lower Upper
113 100
111 102.3 81.4 122.0
192 20.1 16.1 24.1


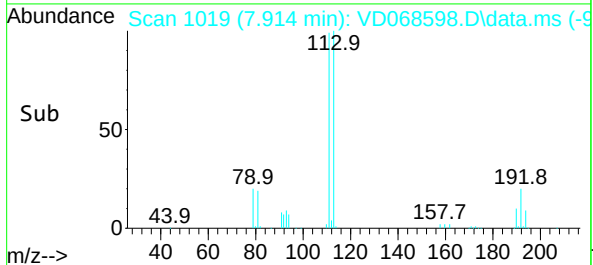
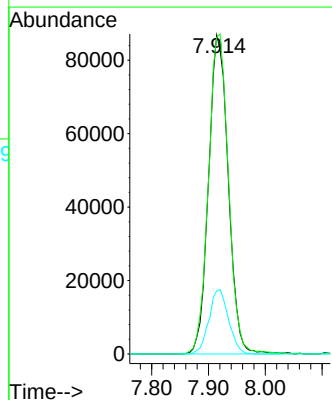
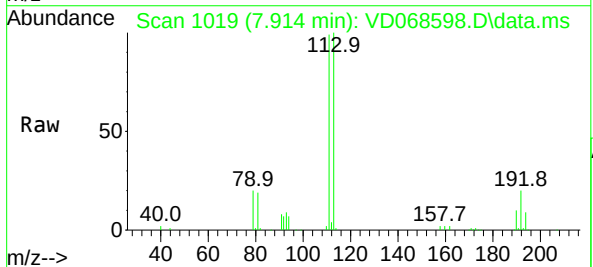


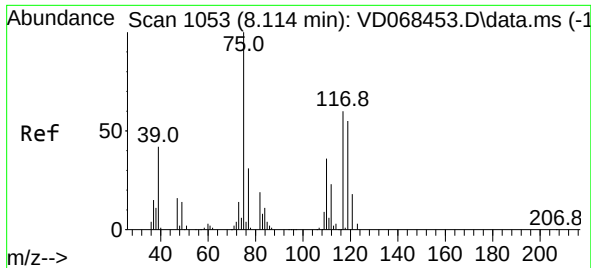

#36
1,1-Dichloropropene
Concen: 4.57 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.135 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04




Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL02


Tgt Ion: 75 Resp: 29337
Ion Ratio Lower Upper
75 100
110 8.4 19.4 58.2#
77 0.0 25.3 37.9#

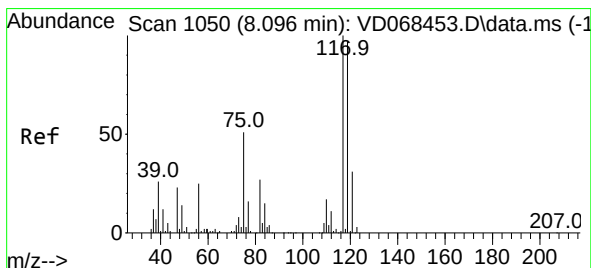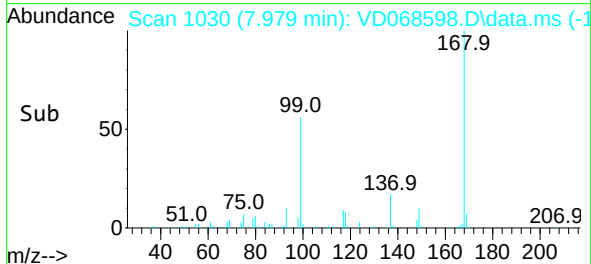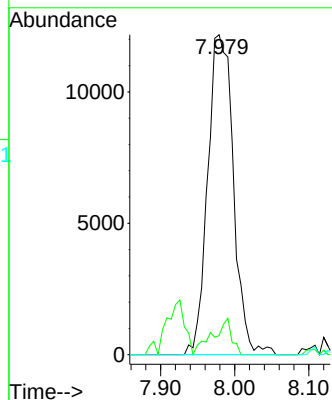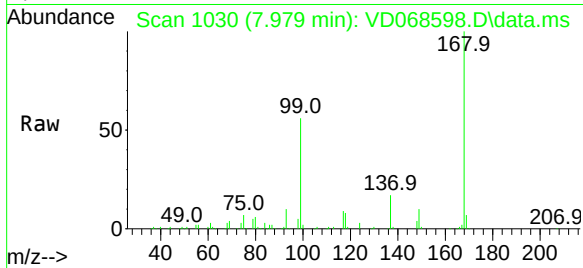

#38
Carbon Tetrachloride
Concen: 6.12 ug/l
RT: 7.985 min Scan# 1031
Delta R.T. -0.111 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04

Tgt Ion: 117 Resp: 36916
Ion Ratio Lower Upper
117 100
119 6.2 77.3 115.9#
121 0.0 24.7 37.1#


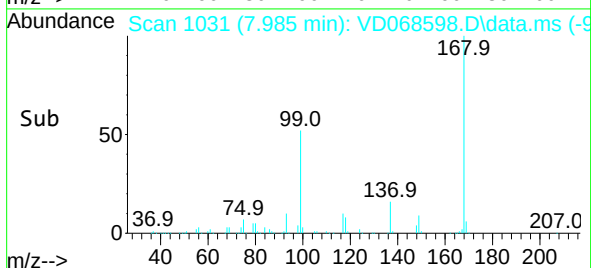
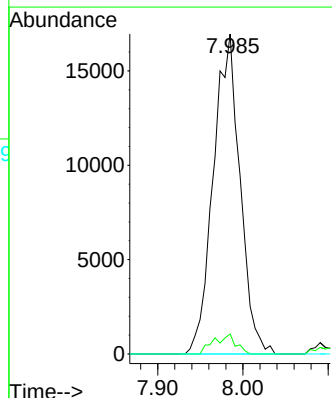
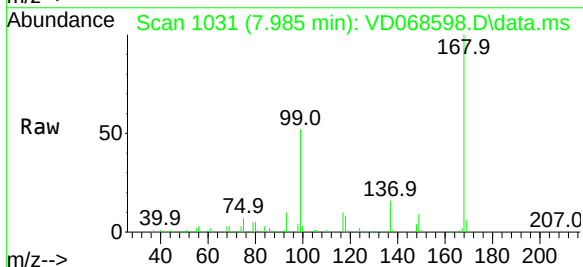


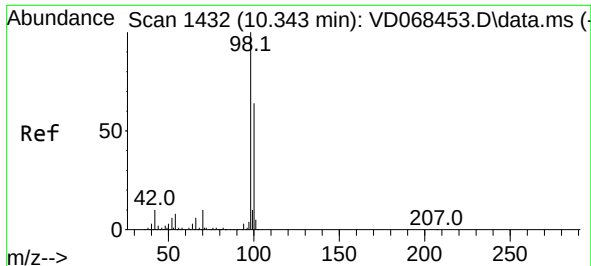

#50
Toluene-d8
Concen: 52.21 ug/l
RT: 10.344 min Scan# 1432
Delta R.T. 0.000 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04




Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL02


Tgt Ion: 98 Resp: 846092
Ion Ratio Lower Upper
98 100
100 64.0 53.0 79.4

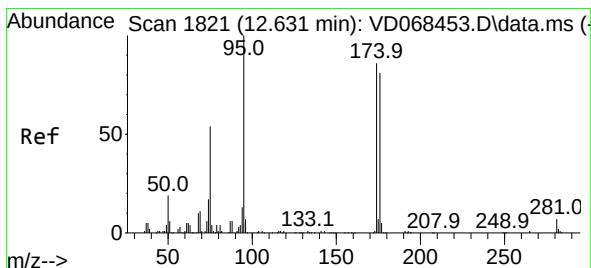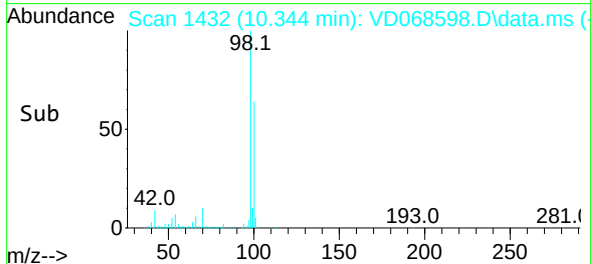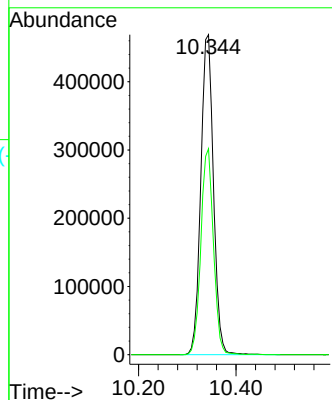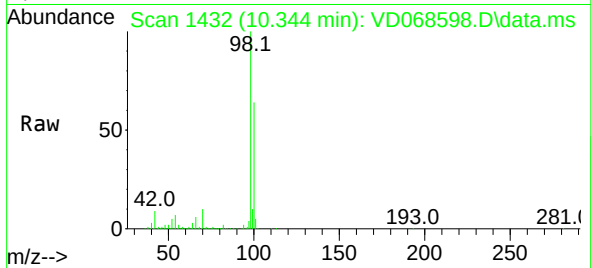

#62
4-Bromofluorobenzene
Concen: 56.77 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.000 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04

Tgt Ion: 95 Resp: 296528
Ion Ratio Lower Upper
95 100
174 87.1 0.0 172.4
176 83.4 0.0 168.4


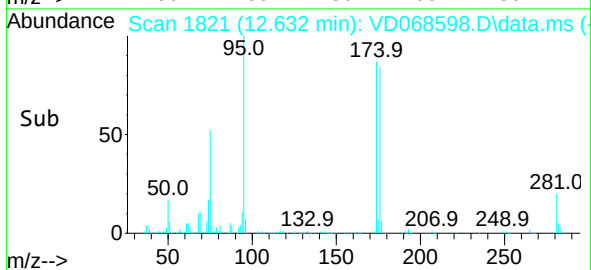
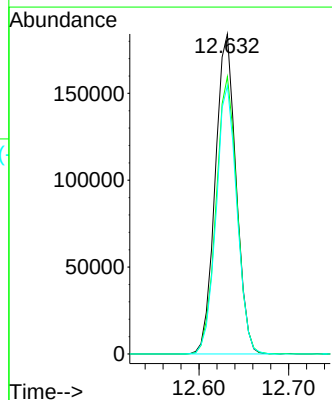
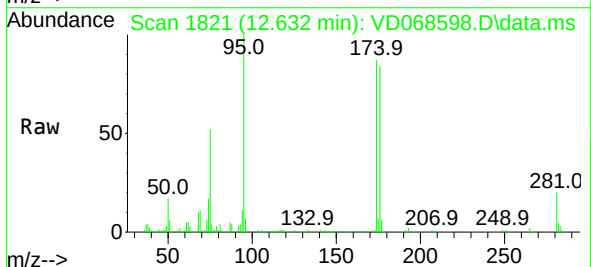


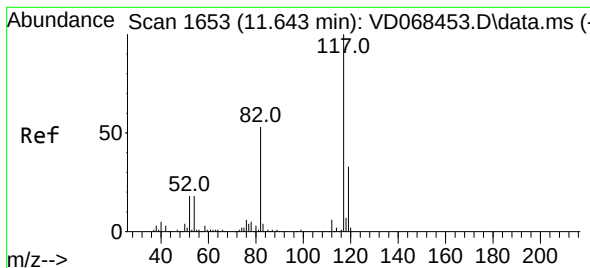

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.643 min Scan# 1653
Delta R.T. 0.000 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04




Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL02


Tgt Ion:117 Resp: 662596
Ion Ratio Lower Upper
117 100
82 51.8 41.4 62.0
119 31.0 26.1 39.1

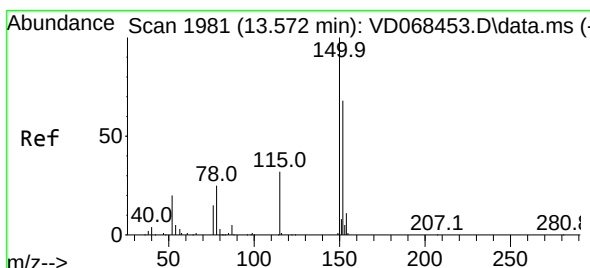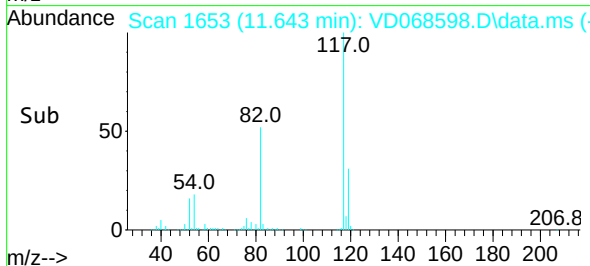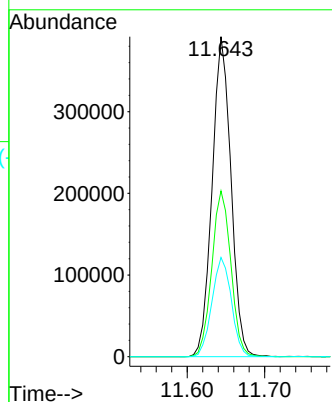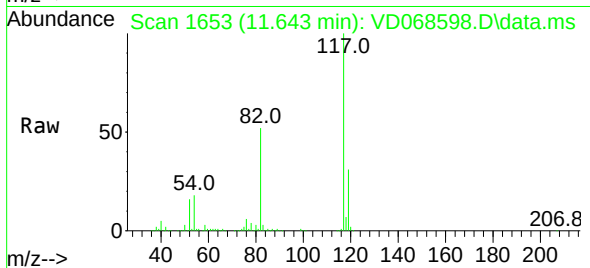

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. 0.001 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04

Tgt Ion:152 Resp: 364848
Ion Ratio Lower Upper
152 100
115 57.2 28.9 86.8
150 158.3 0.0 344.4


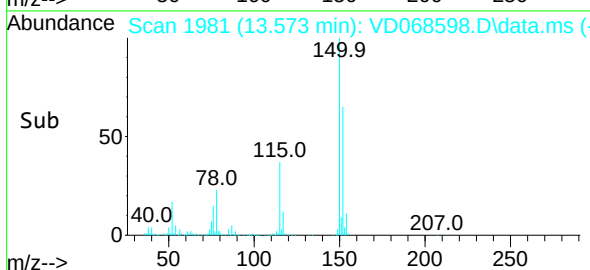
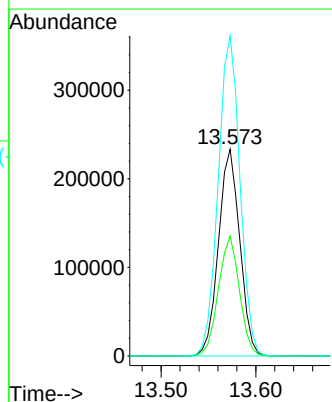
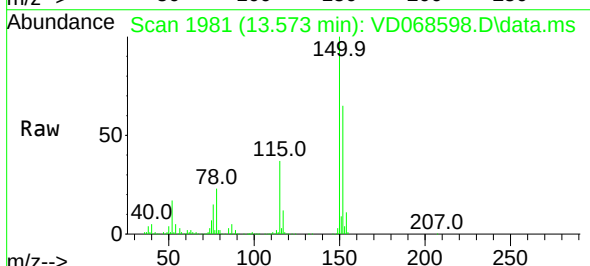


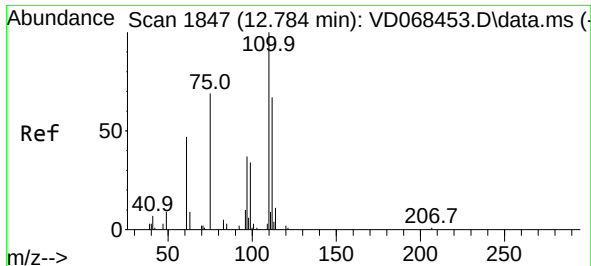

#76
1,2,3-Trichloropropane
Concen: 46.82 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. -0.152 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04

Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL02

Tgt Ion: 75 Resp: 151634
Ion Ratio Lower Upper
75 100
77 1.2 0.0 0.0#

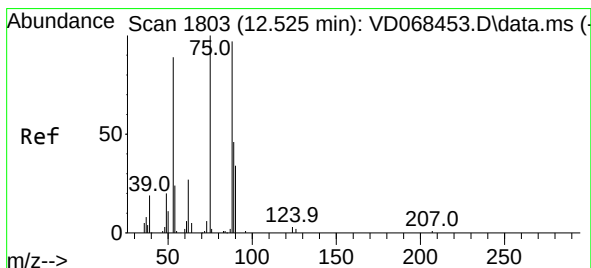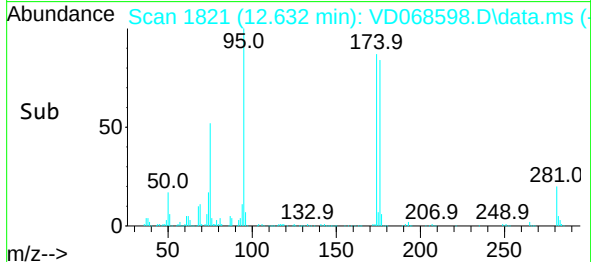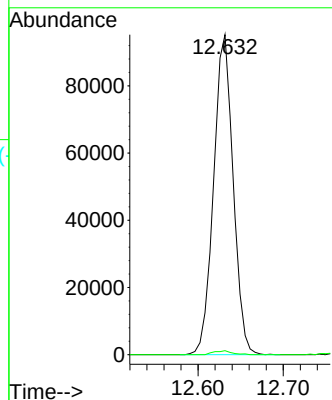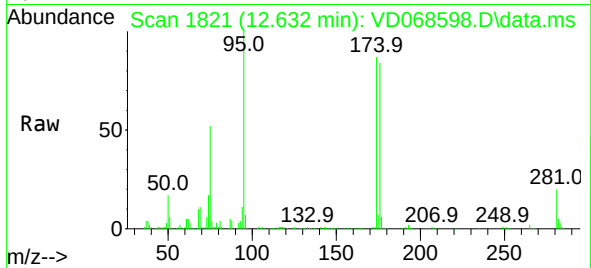

#81
trans-1,4-Dichloro-2-butene
Concen: 109.25 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.106 min
Lab File: VD068598.D
Acq: 12 Mar 2021 11:04

Tgt Ion: 75 Resp: 151634
Ion Ratio Lower Upper
75 100
53 0.0 70.2 105.2#
89 0.0 40.3 60.5#

