

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031221\
 Data File : VD068597.D
 Acq On : 12 Mar 2021 10:36
 Operator : VA/SY
 Sample : VD0312SBL01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0312SBL01

Quant Time: Mar 12 23:33:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 26 14:04:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	421527	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	735456	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.643	117	717326	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	386063	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	208824	49.58	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	99.16%
35) Dibromofluoromethane	7.914	113	224051	50.57	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.14%
50) Toluene-d8	10.338	98	916423	51.93	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	103.86%
62) 4-Bromofluorobenzene	12.632	95	320328	56.32	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	112.64%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031221\
Data File : VD068597.D
Acq On : 12 Mar 2021 10:36
Operator : VA/SY
Sample : VD0312SBL01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL01

Quant Time: Mar 12 23:33:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
Quant Title : SW846 8260
QLast Update : Fri Feb 26 14:04:14 2021
Response via : Initial Calibration




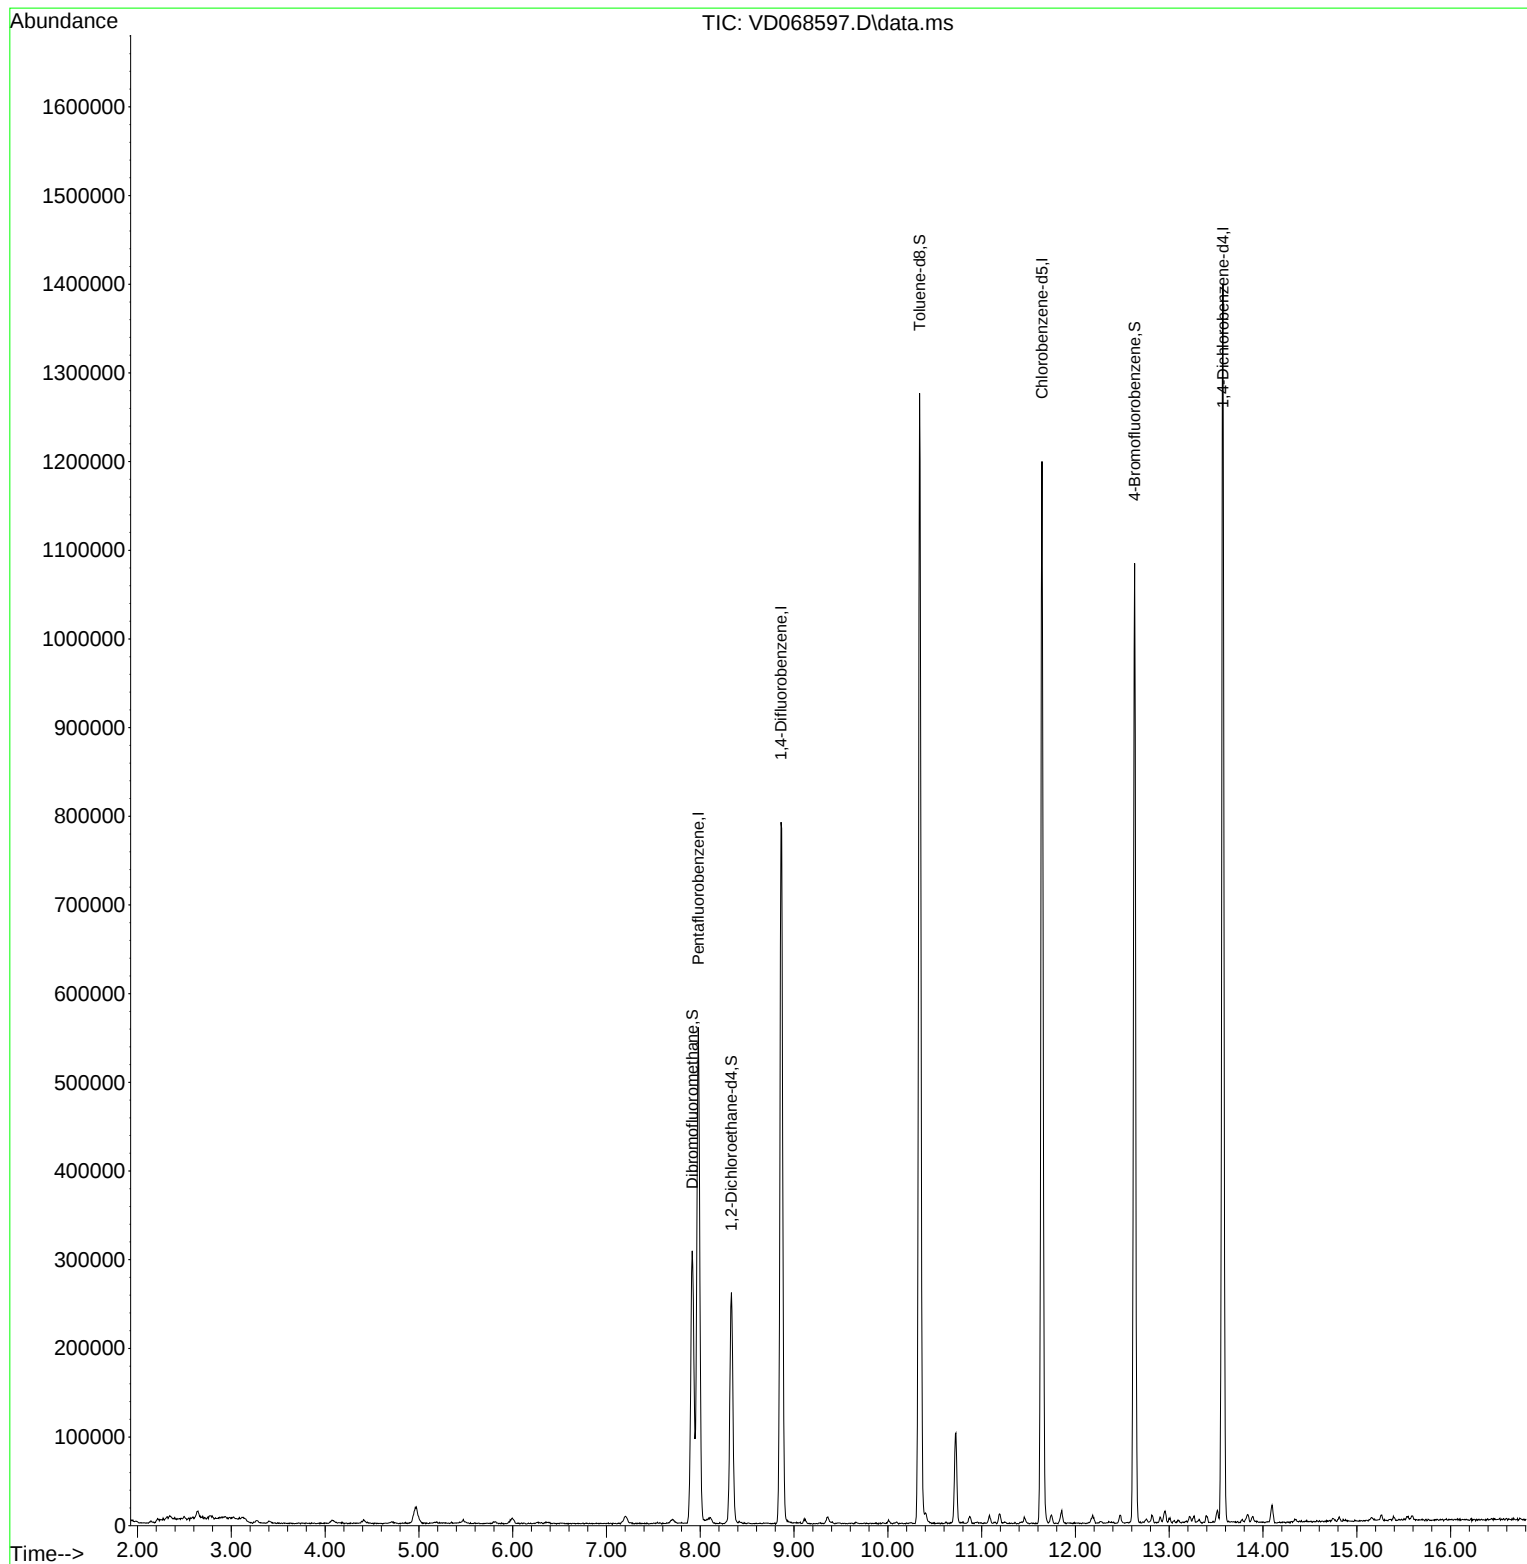


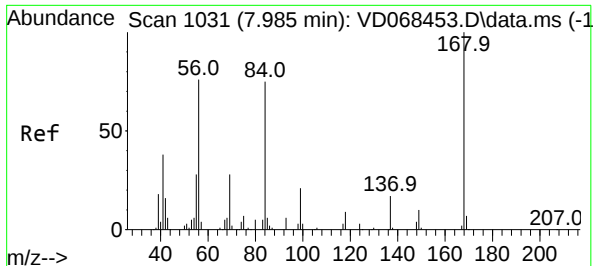

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD068597.D
Acq: 12 Mar 2021 10:36




Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL01


Tgt Ion:168 Resp: 421527
Ion Ratio Lower Upper
168 100
99 58.2 43.5 65.3

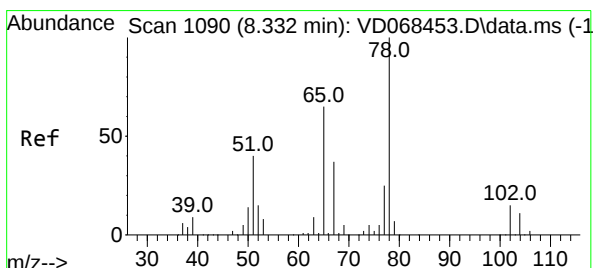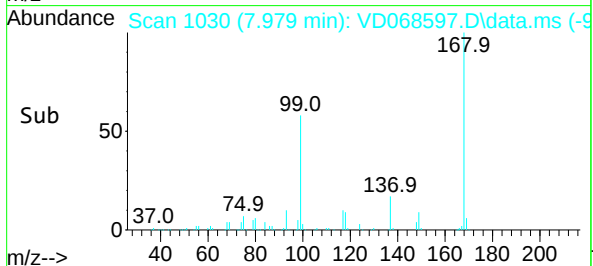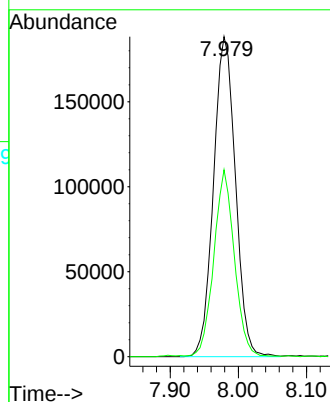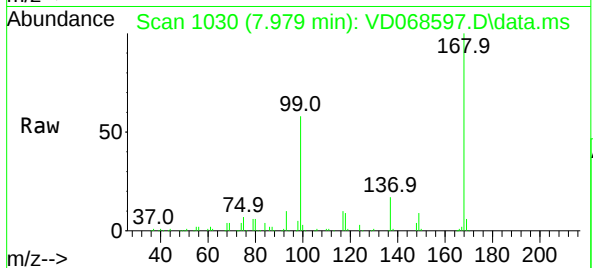

#33
1,2-Dichloroethane-d4
Concen: 49.58 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. 0.000 min
Lab File: VD068597.D
Acq: 12 Mar 2021 10:36

Tgt Ion: 65 Resp: 208824
Ion Ratio Lower Upper
65 100
67 53.0 0.0 105.0


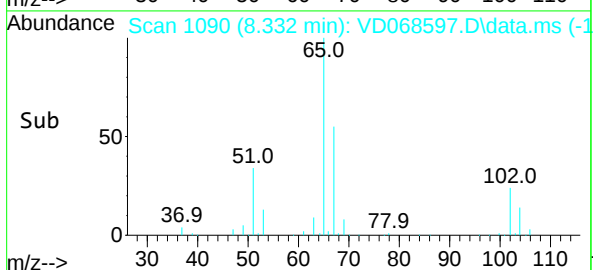
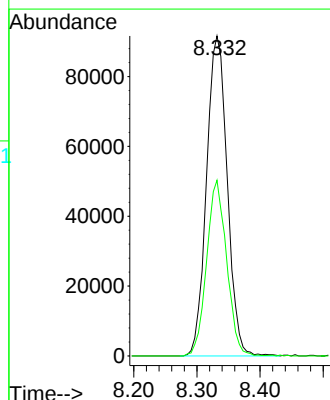
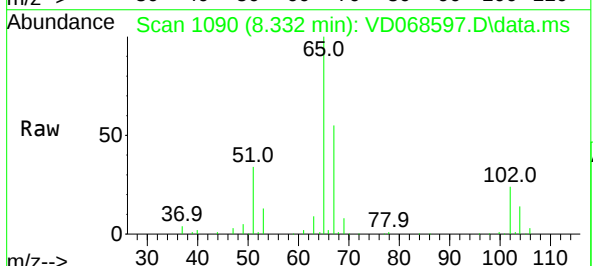


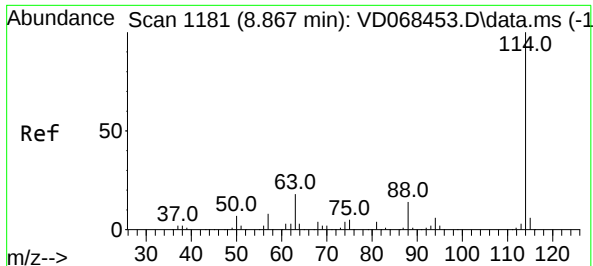

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.006 min
Lab File: VD068597.D
Acq: 12 Mar 2021 10:36




Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL01


Tgt Ion:114 Resp: 735456
Ion Ratio Lower Upper
114 100
63 17.1 0.0 34.8
88 14.5 0.0 31.6

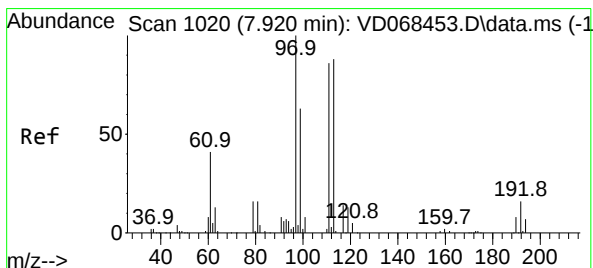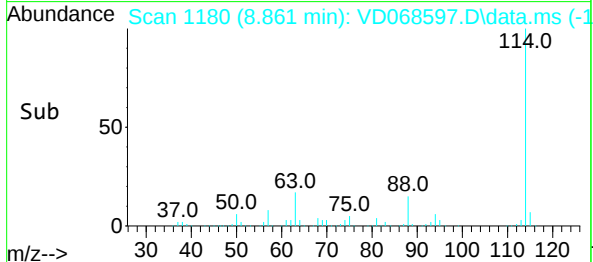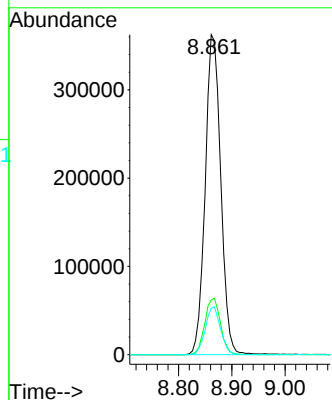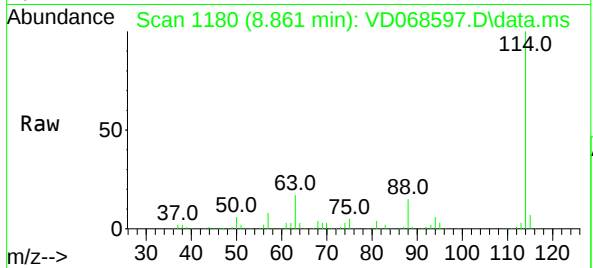

#35
Dibromofluoromethane
Concen: 50.57 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.006 min
Lab File: VD068597.D
Acq: 12 Mar 2021 10:36

Tgt Ion:113 Resp: 224051
Ion Ratio Lower Upper
113 100
111 103.7 81.4 122.0
192 20.6 16.1 24.1


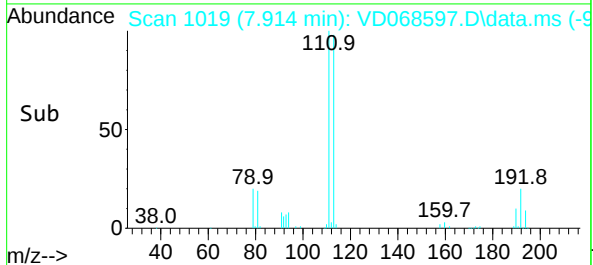
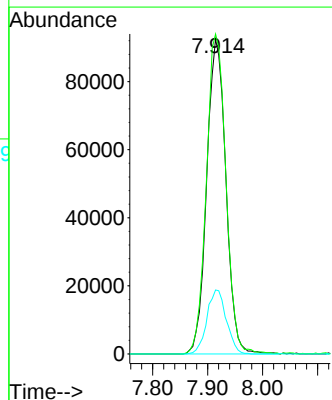
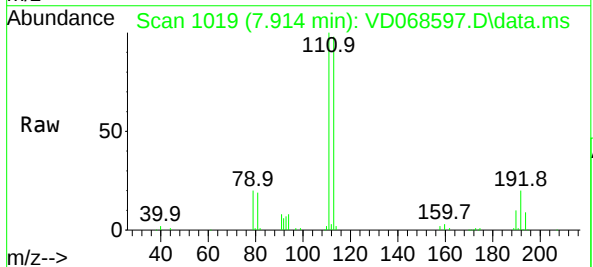


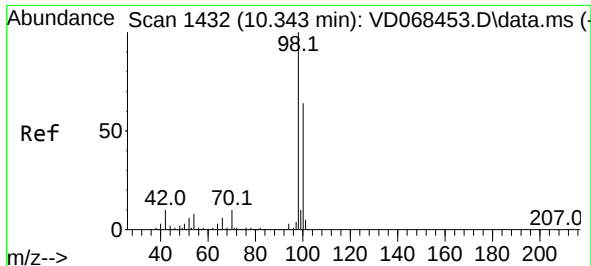

#50
Toluene-d8
Concen: 51.93 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.006 min
Lab File: VD068597.D
Acq: 12 Mar 2021 10:36




Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL01


Tgt Ion: 98 Resp: 916423
Ion Ratio Lower Upper
98 100
100 63.9 53.0 79.4

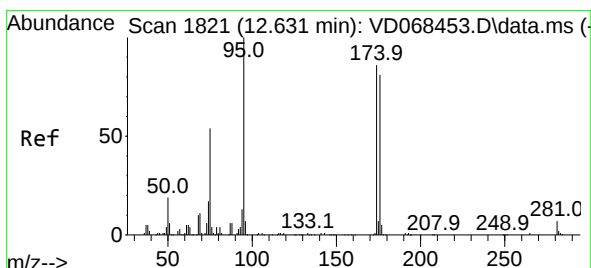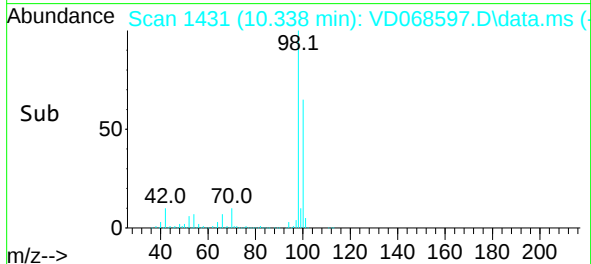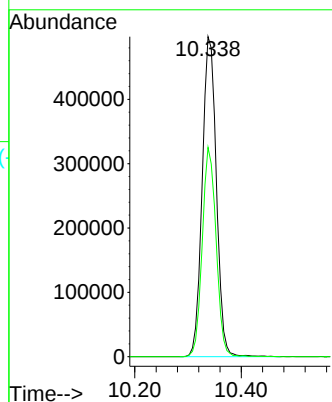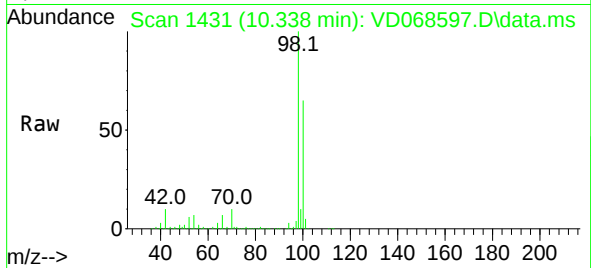

#62
4-Bromofluorobenzene
Concen: 56.32 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.000 min
Lab File: VD068597.D
Acq: 12 Mar 2021 10:36

Tgt Ion: 95 Resp: 320328
Ion Ratio Lower Upper
95 100
174 86.9 0.0 172.4
176 84.7 0.0 168.4


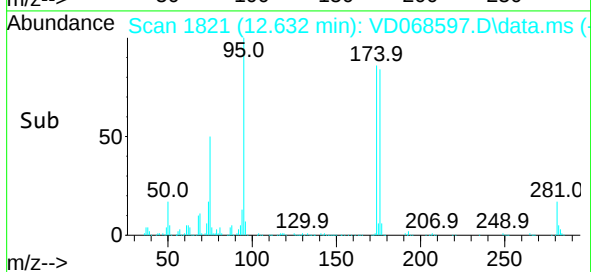
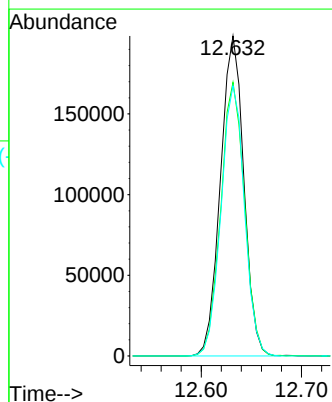
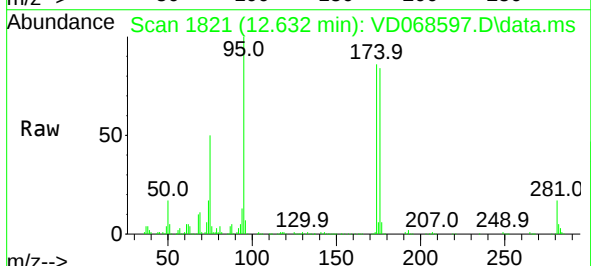


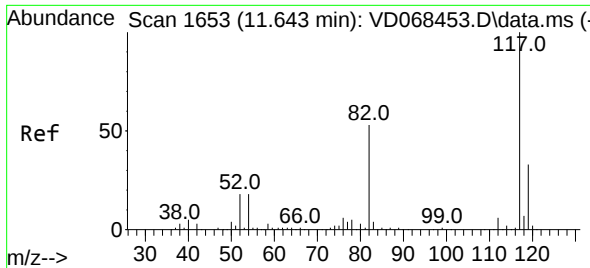

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.643 min Scan# 1653
Delta R.T. 0.000 min
Lab File: VD068597.D
Acq: 12 Mar 2021 10:36

Instrument :
MSVOA_D
ClientSampleId :
VD0312SBL01

Tgt Ion:117 Resp: 717326
Ion Ratio Lower Upper
117 100
82 50.7 41.4 62.0
119 31.1 26.1 39.1

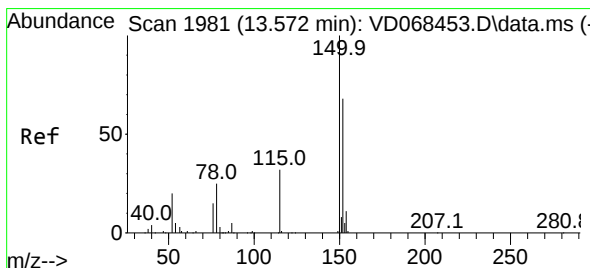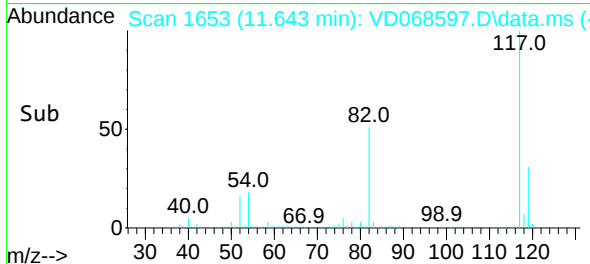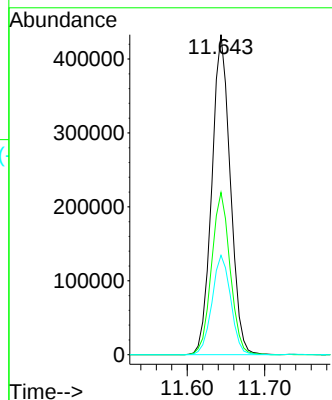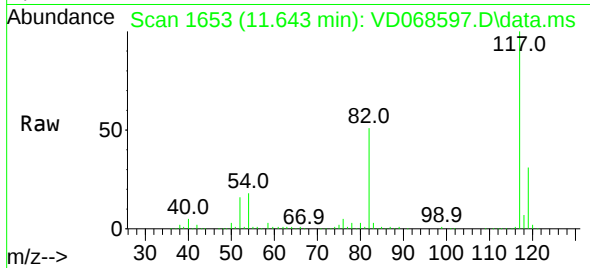

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. 0.001 min
Lab File: VD068597.D
Acq: 12 Mar 2021 10:36

Tgt Ion:152 Resp: 386063
Ion Ratio Lower Upper
152 100
115 57.3 28.9 86.8
150 158.5 0.0 344.4

