

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD031319\
 Data File : VD061054.D
 Acq On : 13 Mar 2019 20:44
 Operator : VA/AP
 Sample : K1824-15
 Misc : 5.04g/5ml/MSVOA D/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 14 03:32:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 08 02:35:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.04	168	559604	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.21	114	940509	50.00	ug/l	0.00
63) Chlorobenzene-d5	12.37	117	744393	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	14.51	152	246790	50.00	ug/l	0.00


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.45	65	238675	51.24	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	102.48%	
35) Dibromofluoromethane	6.92	113	366640	52.53	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	105.06%	
50) Toluene-d8	10.41	98	804050	45.87	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	91.74%	
62) 4-Bromofluorobenzene	13.55	95	279608	41.11	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	82.22%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD031319\
Data File : VD061054.D
Acq On : 13 Mar 2019 20:44
Operator : VA/AP
Sample : K1824-15
Misc : 5.04g/5ml/MSVOA D/SOIL
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 14 03:32:52 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 08 02:35:39 2019
Response via : Initial Calibration

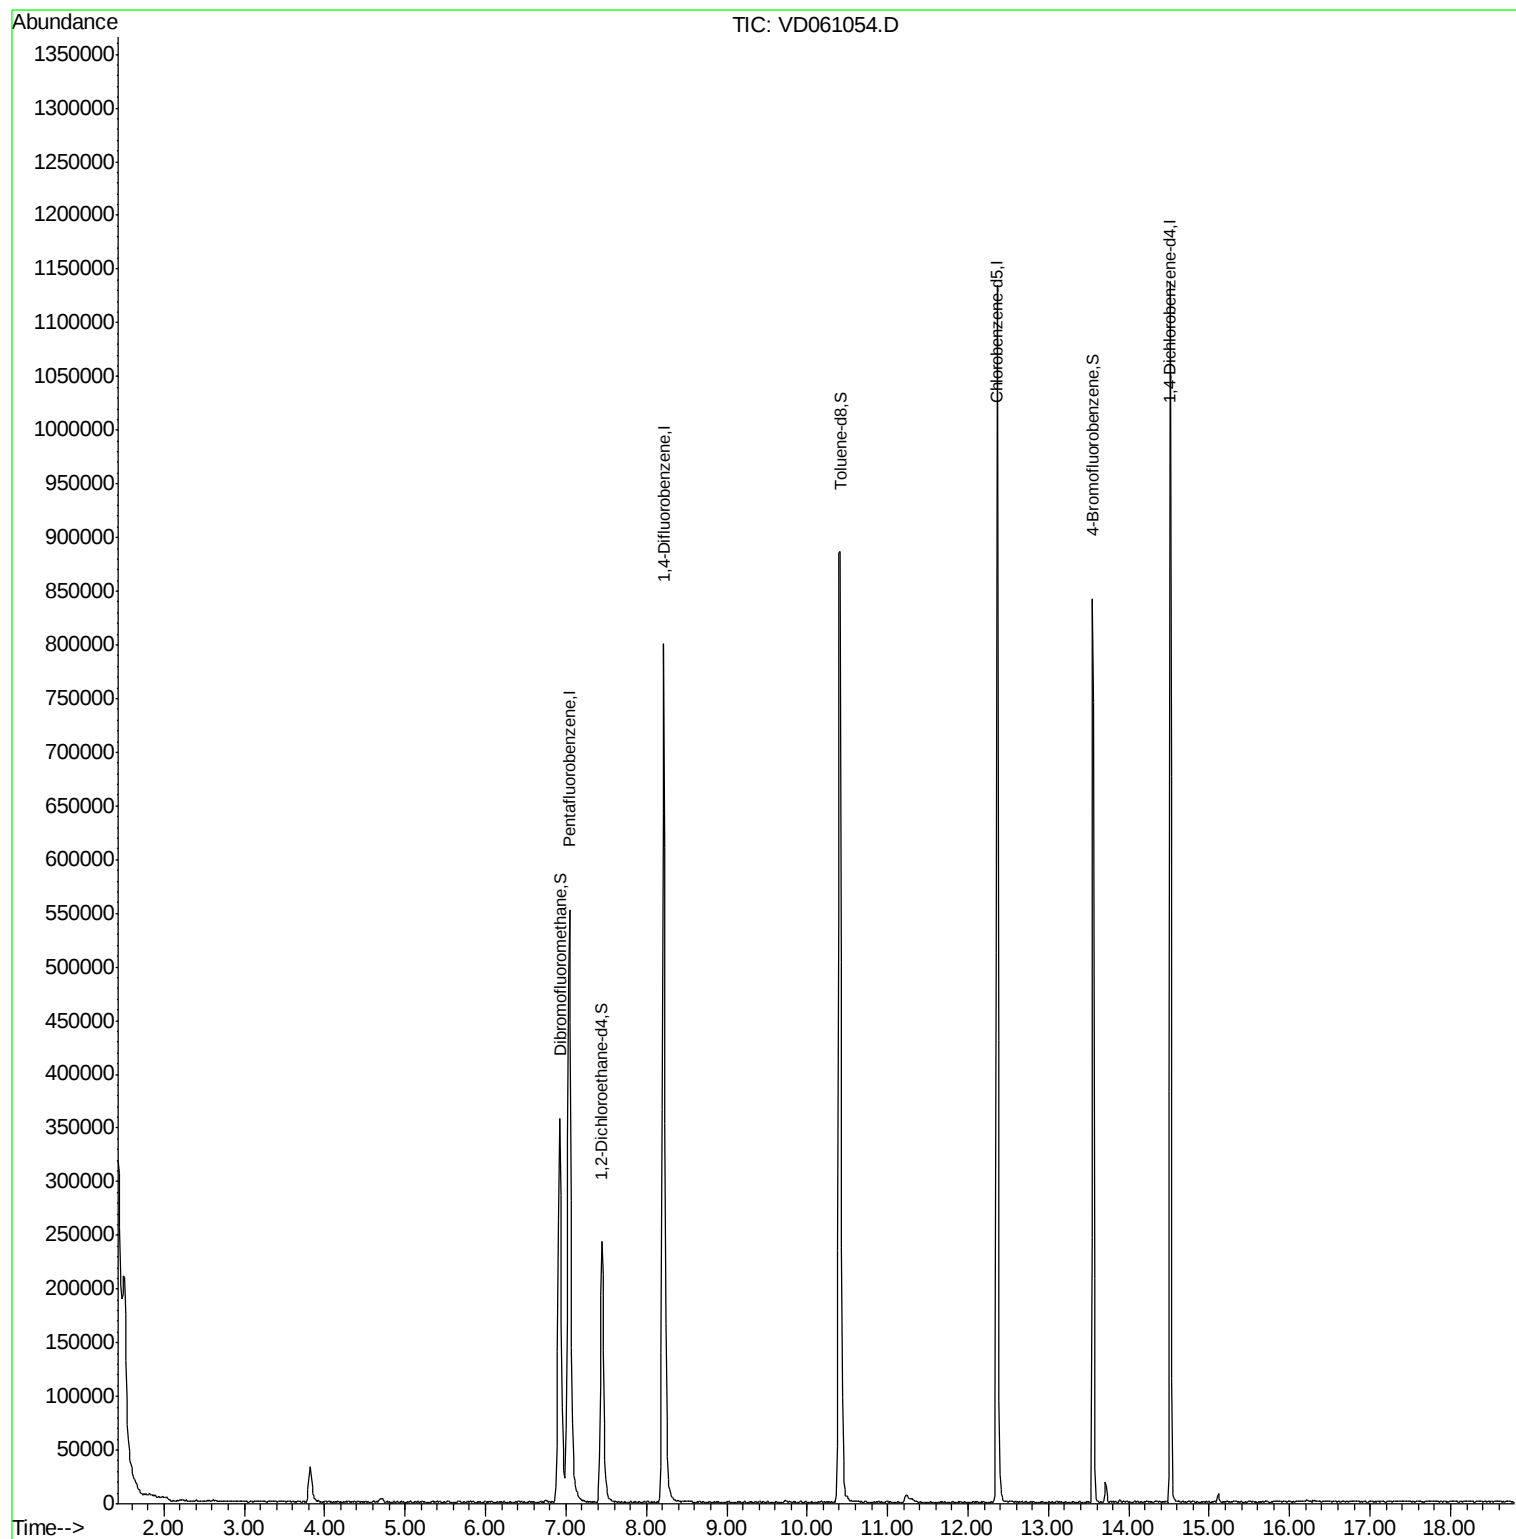

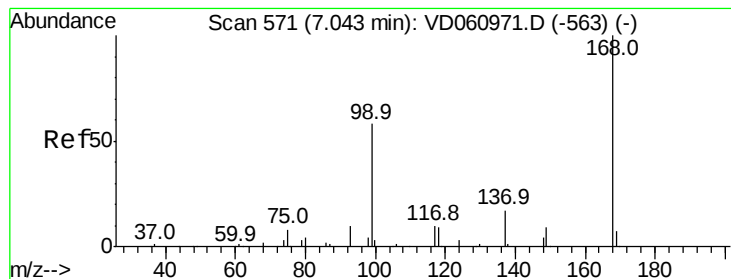

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.04 min Scan# 571

Delta R.T. -0.00 min

Lab File: VD061054.D


Acq: 13 Mar 2019 20:44

Tot Ion:168 Resp: 559604

Ion Ratio Lower Upper




168 100

99 57.7 47.3 70.9

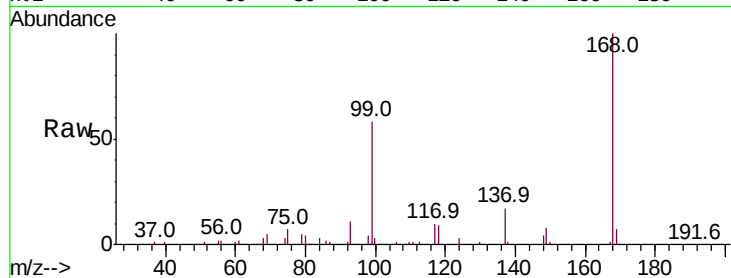

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

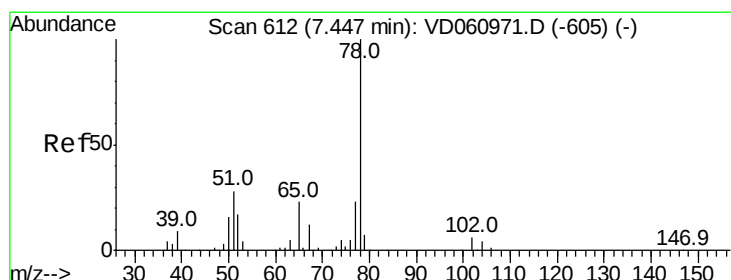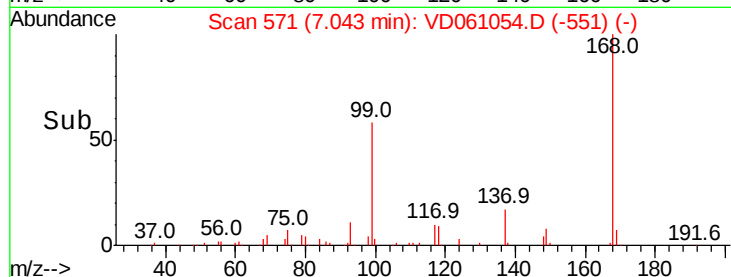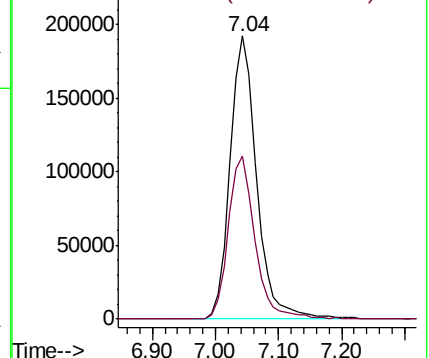

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 7.45 min Scan# 612

Delta R.T. -0.00 min

Lab File: VD061054.D


Acq: 13 Mar 2019 20:44

Tgt Ion: 65 Resp: 238675

Ion Ratio Lower Upper



65 100


67 49.4 0.0 105.2

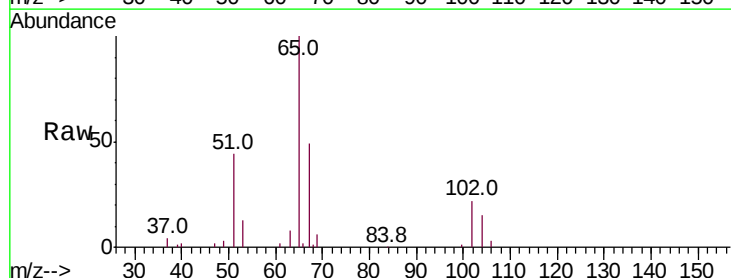

Abundance Ion 64.95 (64.65 to 65.65): VDC


Ion 66.90 (66.60 to 67.60): VDC

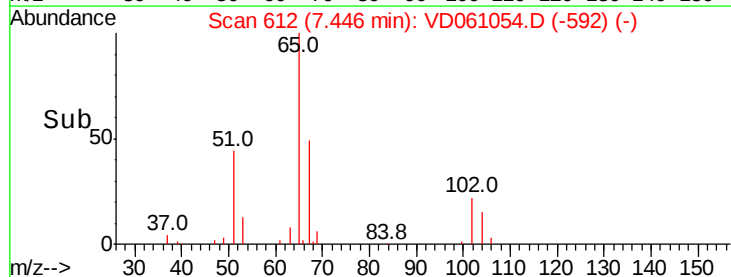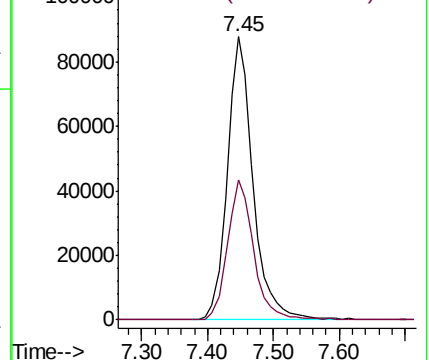



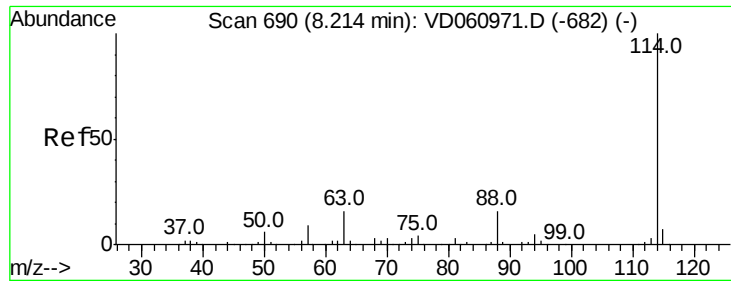


#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.21 min Scan# 690
 Delta R.T. -0.00 min
 Lab File: VD061054.D
 Acq: 13 Mar 2019 20:44

Tot Ion:114 Resp: 940509
 Ion Ratio Lower Upper
 114 100
 63 16.8 0.0 31.4
 88 16.8 0.0 33.0

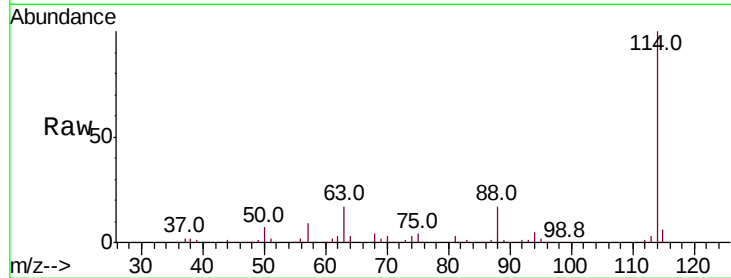


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 62.95 (62.65 to 63.65): V
 Ion 87.90 (87.60 to 88.60): V

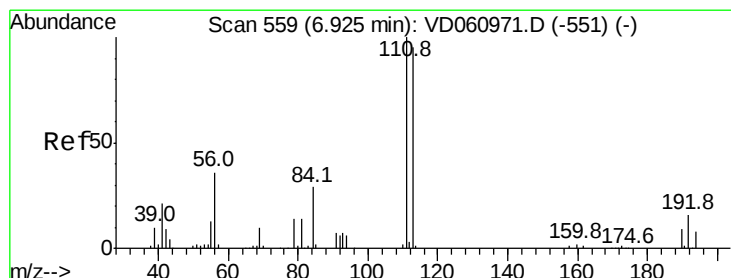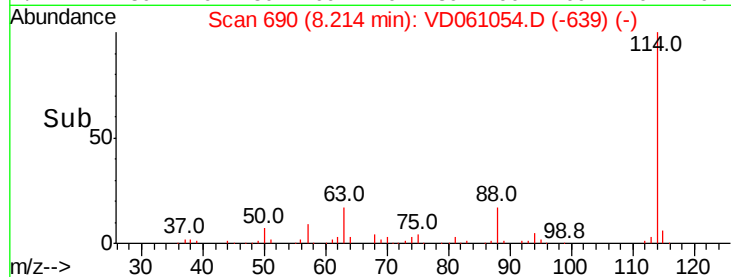
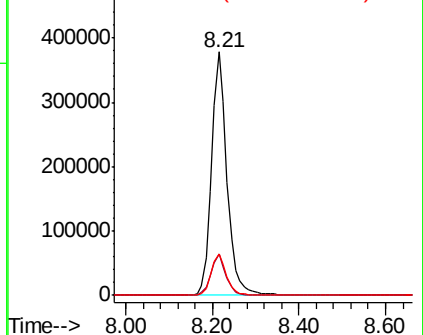



#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 6.92 min Scan# 559
 Delta R.T. -0.00 min
 Lab File: VD061054.D
 Acq: 13 Mar 2019 20:44

Tgt Ion:113 Resp: 366640
 Ion Ratio Lower Upper
 113 100
 111 98.6 84.2 126.4
 192 16.4 13.1 19.7

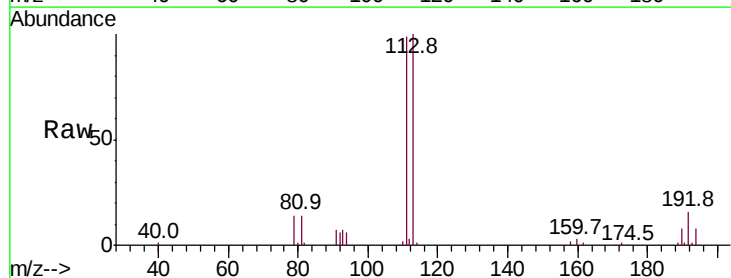

Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V

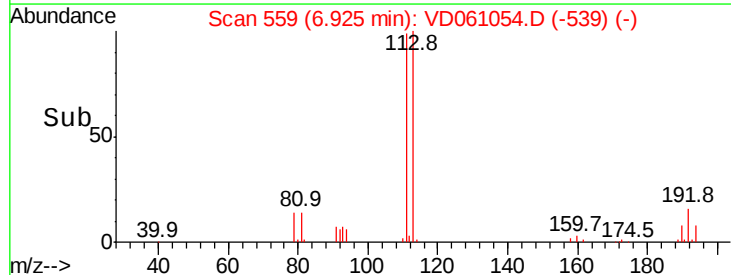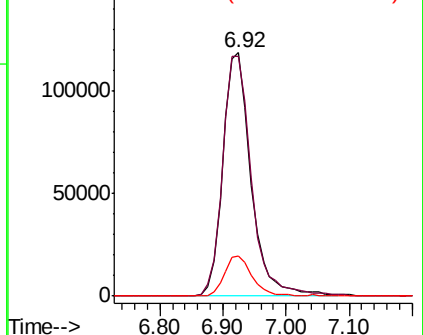

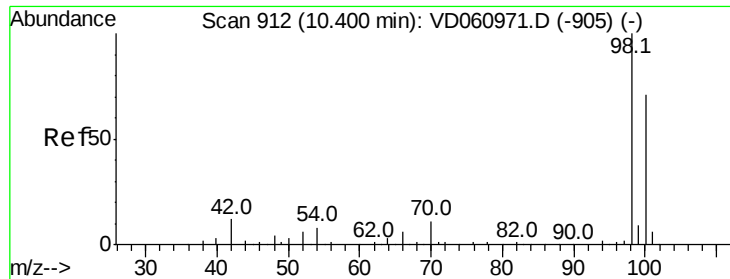

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.41 min Scan# 913

Delta R.T. 0.01 min

Lab File: VD061054.D


Acq: 13 Mar 2019 20:44

Tot Ion: 98 Resp: 804050

Ion Ratio Lower Upper

98 100

100 69.5 57.4 86.2

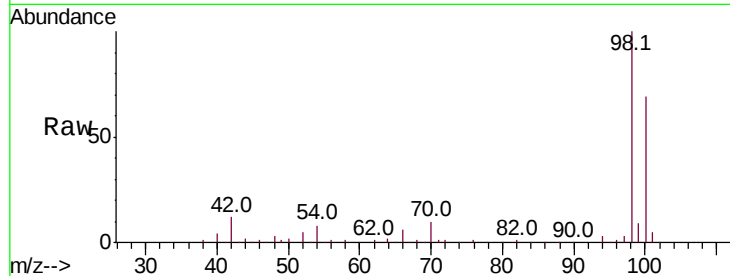

Abundance Ion 98.05 (97.75 to 98.75): VDC

Ion 100.05 (99.75 to 100.75): VDC

10.41



300000

200000

100000

0

Time-->

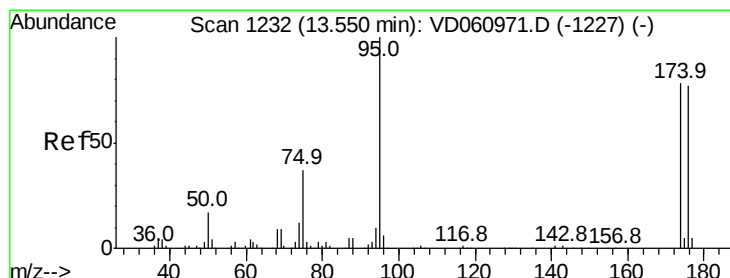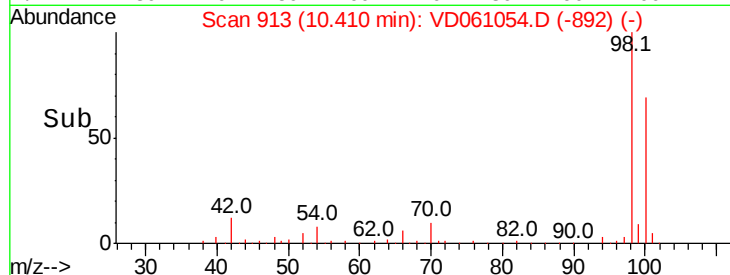

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 13.55 min Scan# 1232

Delta R.T. -0.00 min

Lab File: VD061054.D

Acq: 13 Mar 2019 20:44


Tgt Ion: 95 Resp: 279608

Ion Ratio Lower Upper

95 100

174 71.2 0.0 155.6

176 66.7 0.0 153.8

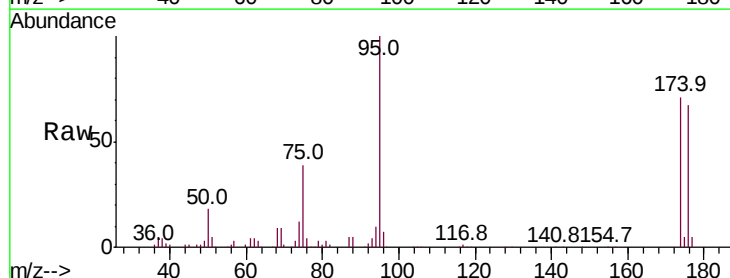

Abundance Ion 95.00 (94.70 to 95.70): VDC

Ion 173.90 (173.60 to 174.60): VDC

Ion 175.90 (175.60 to 176.60): VDC

250000

200000


150000


100000

50000

0





Time-->

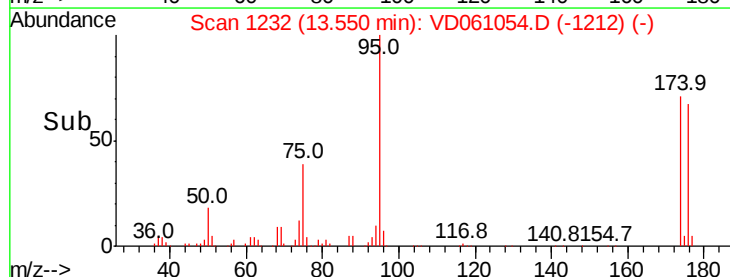

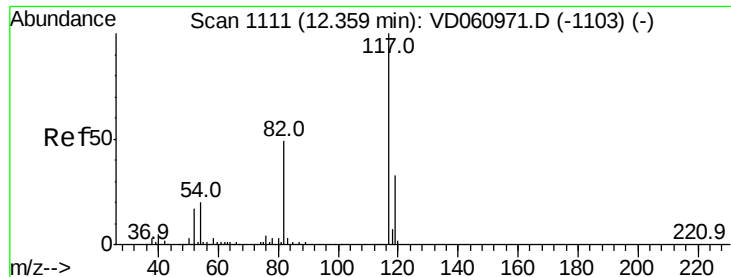

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.37 min Scan# 1112
Delta R.T. 0.01 min
Lab File: VD061054.D
Acq: 13 Mar 2019 20:44

Tot Ion:117 Resp: 744393
Ion Ratio Lower Upper
117 100
82 45.0 38.9 58.3
119 32.8 26.6 39.8

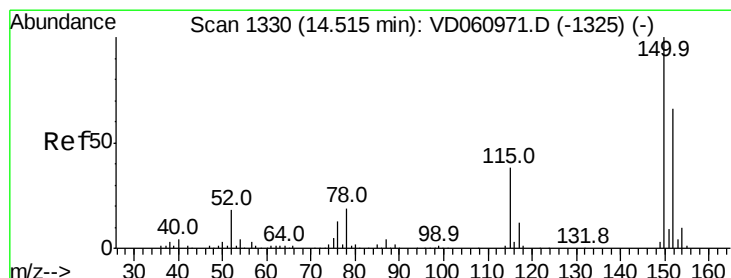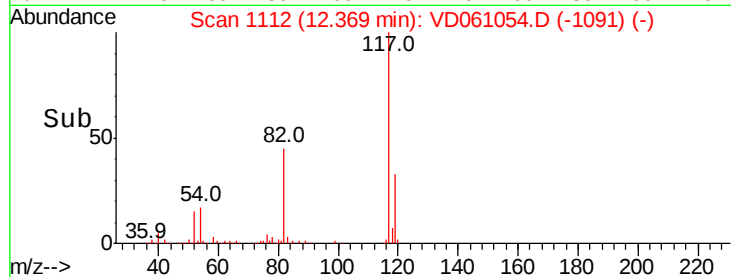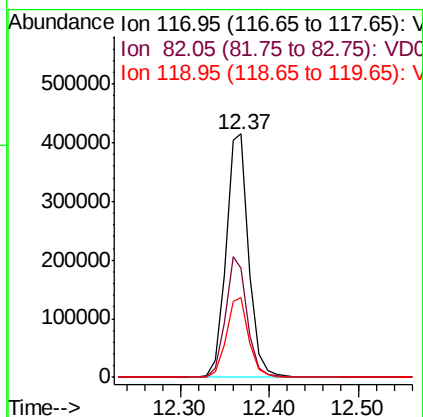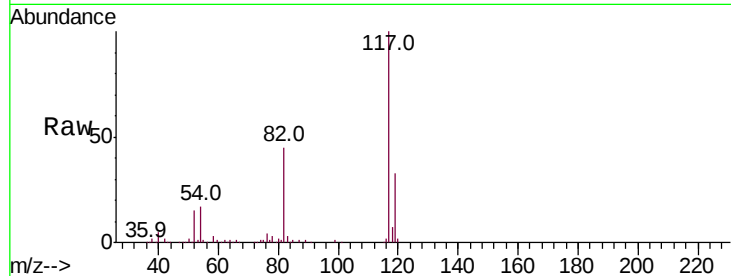

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 14.51 min Scan# 1330
Delta R.T. -0.00 min
Lab File: VD061054.D
Acq: 13 Mar 2019 20:44

Tgt Ion:152 Resp: 246790
Ion Ratio Lower Upper
152 100
115 61.3 28.6 85.9
150 159.7 0.0 310.6

