

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD031319\
 Data File : VD061056.D
 Acq On : 13 Mar 2019 21:39
 Operator : VA/AP
 Sample : K1897-06
 Misc : 8.76g/5ml/MSVOA D/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 14 03:35:44 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 08 02:35:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.04	168	28578	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.21	114	55873	50.00	ug/l	0.00
63) Chlorobenzene-d5	12.36	117	47171	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	14.51	152	19067	50.00	ug/l	0.00


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.44	65	23162	97.37	ug/l	0.00
Spiked Amount 50.000			Recovery	=	194.74%	
35) Dibromofluoromethane	6.92	113	26553	64.04	ug/l	0.00
Spiked Amount 50.000			Recovery	=	128.08%	
50) Toluene-d8	10.40	98	47268	45.39	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.78%	
62) 4-Bromofluorobenzene	13.55	95	21436	53.06	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.12%	


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD031319\
Data File : VD061056.D
Acq On : 13 Mar 2019 21:39
Operator : VA/AP
Sample : K1897-06
Misc : 8.76g/5ml/MSVOA D/SOIL
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 14 03:35:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 08 02:35:39 2019
Response via : Initial Calibration

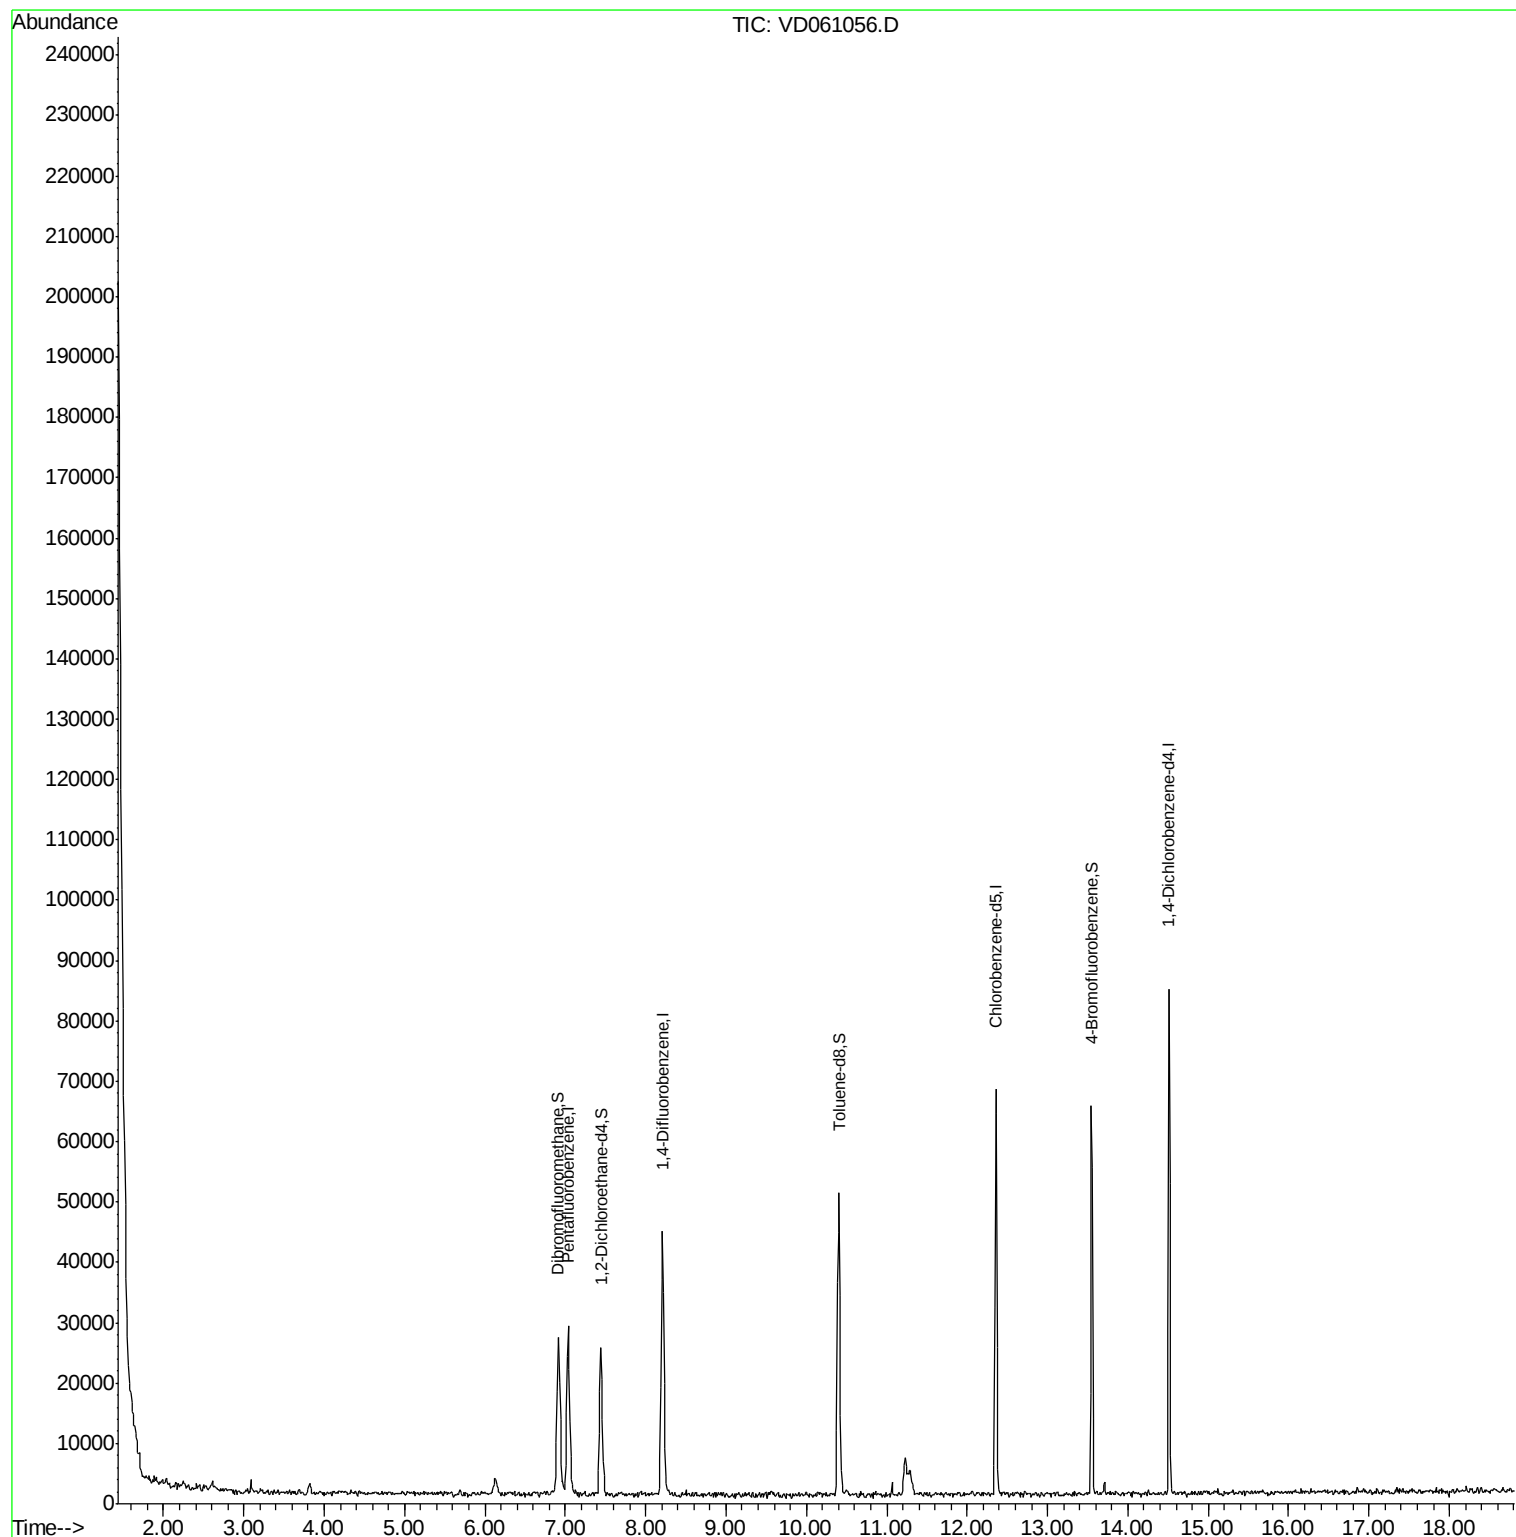

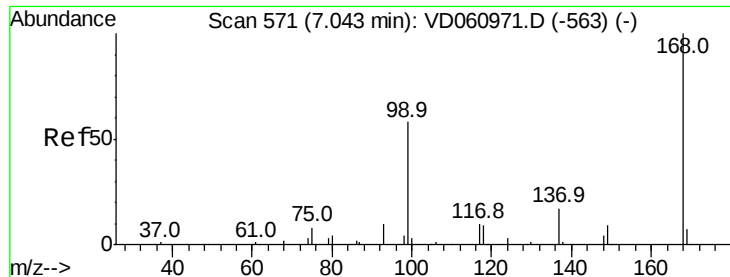

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.04 min Scan# 570

Delta R.T. -0.00 min

Lab File: VD061056.D


Acq: 13 Mar 2019 21:39

Tot Ion:168 Resp: 28578

Ion Ratio Lower Upper

168 100

99 66.2 47.3 70.9


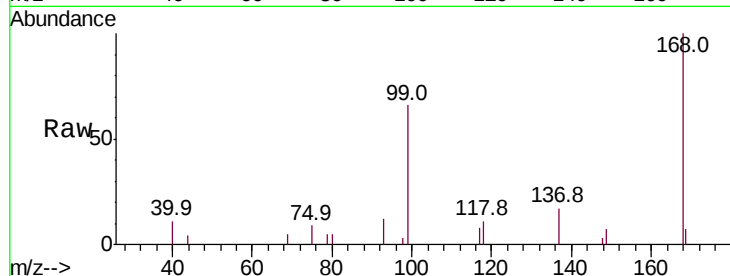


Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

7.04

Time-->

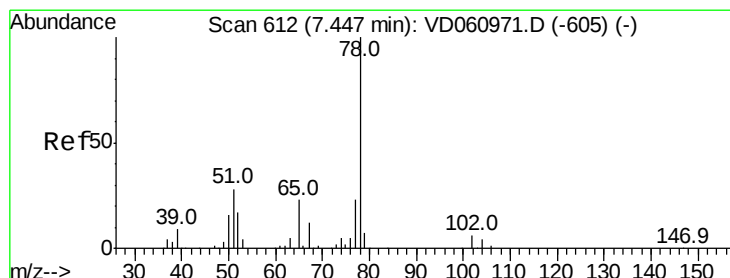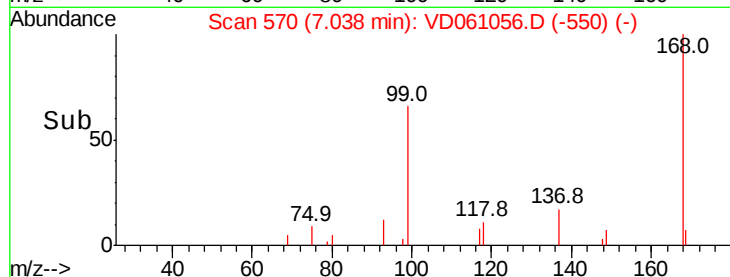

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 7.44 min Scan# 611

Delta R.T. -0.00 min

Lab File: VD061056.D


Acq: 13 Mar 2019 21:39

Tgt Ion: 65 Resp: 23162

Ion Ratio Lower Upper

65 100

67 50.7 0.0 105.2

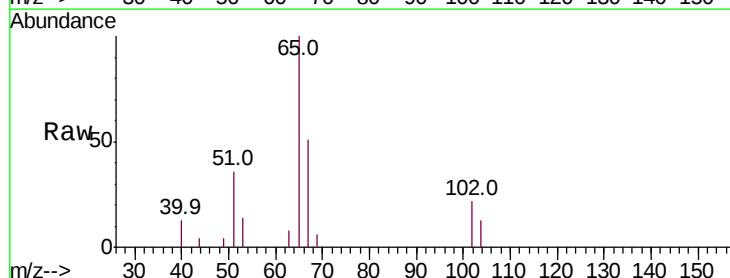



Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

7.44


Time-->

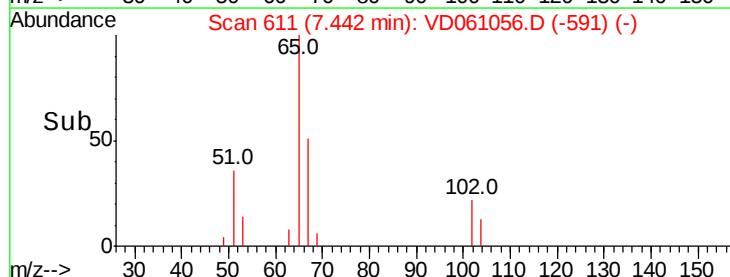



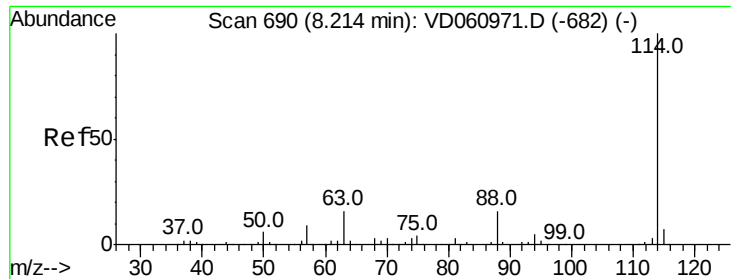


#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.21 min Scan# 689
 Delta R.T. -0.00 min
 Lab File: VD061056.D
 Acq: 13 Mar 2019 21:39

Tot Ion:114 Resp: 55873
 Ion Ratio Lower Upper
 114 100
 63 14.5 0.0 31.4
 88 16.6 0.0 33.0

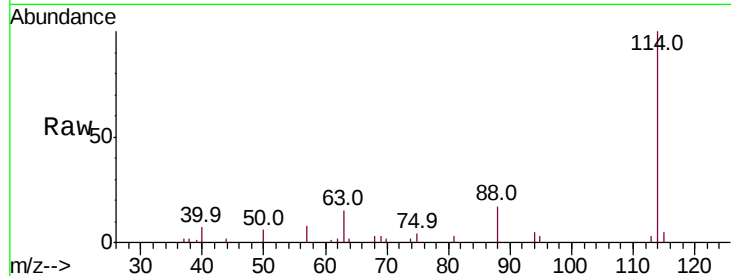


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 62.95 (62.65 to 63.65): V
 Ion 87.90 (87.60 to 88.60): V

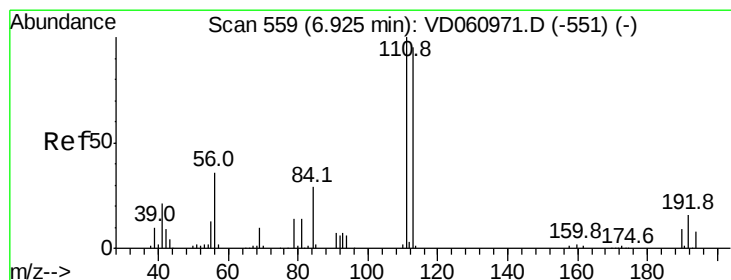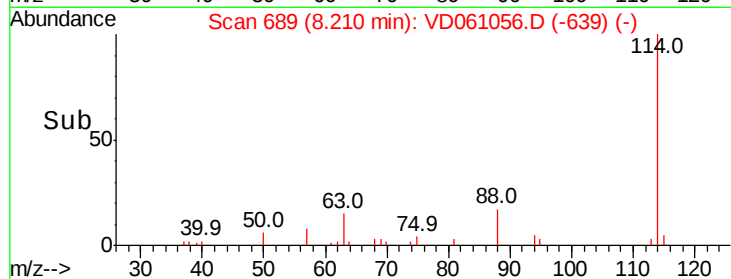
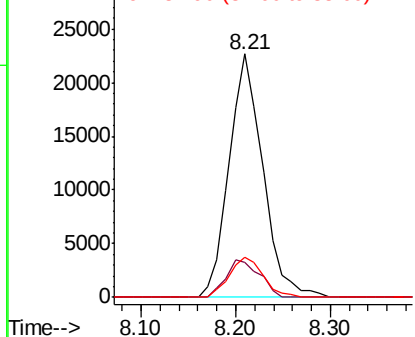



#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 6.92 min Scan# 558
 Delta R.T. -0.00 min
 Lab File: VD061056.D
 Acq: 13 Mar 2019 21:39

Tgt Ion:113 Resp: 26553
 Ion Ratio Lower Upper
 113 100
 111 90.7 84.2 126.4
 192 16.6 13.1 19.7

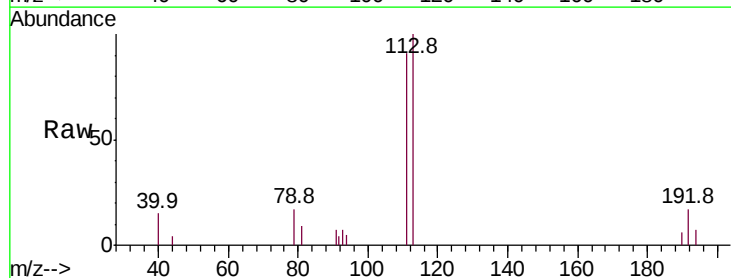

Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V

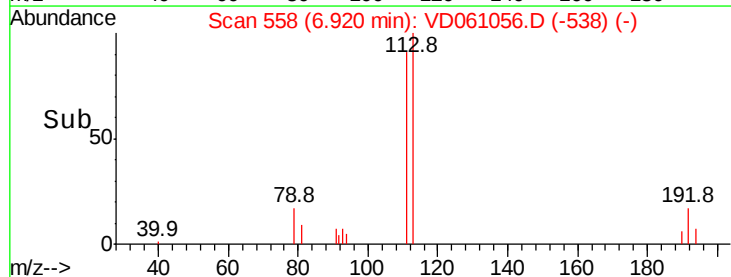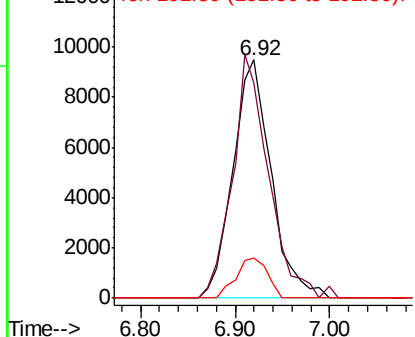

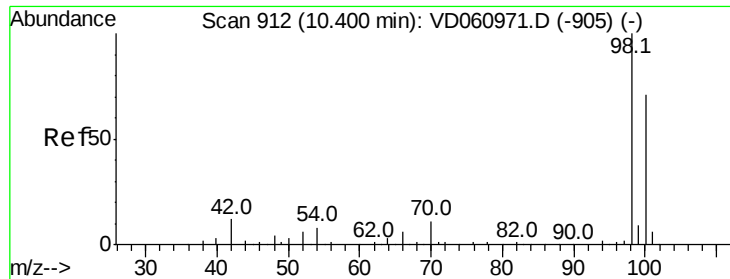

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.40 min Scan# 912

Delta R.T. 0.01 min

Lab File: VD061056.D


Acq: 13 Mar 2019 21:39

Tot Ion: 98 Resp: 47268

Ion Ratio Lower Upper

98 100

100 78.8 57.4 86.2

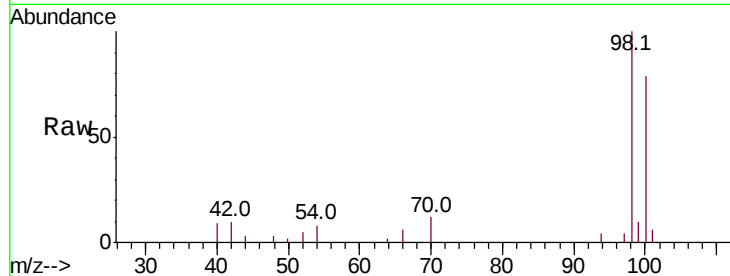

Abundance Ion 98.05 (97.75 to 98.75): VD060971.D (-905) (-)

Ion 100.05 (99.75 to 100.75): VD060971.D (-905) (-)

10.40

20000

15000

10000

5000



0

Time-->

10.30

10.40

10.50

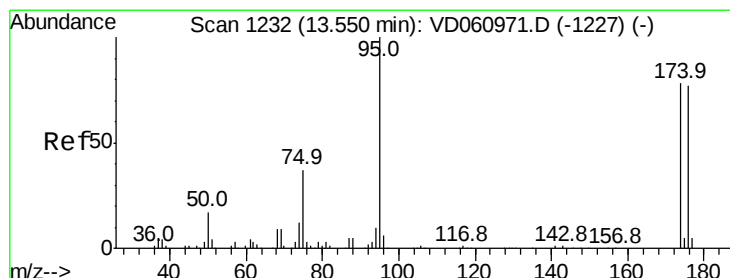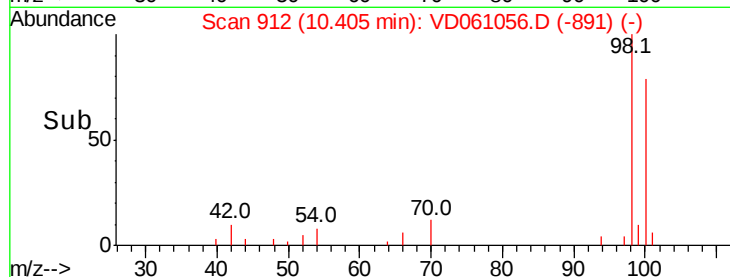

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 13.55 min Scan# 1231

Delta R.T. -0.00 min

Lab File: VD061056.D

Acq: 13 Mar 2019 21:39


Tgt Ion: 95 Resp: 21436

Ion Ratio Lower Upper

95 100

174 73.2 0.0 155.6

176 73.4 0.0 153.8

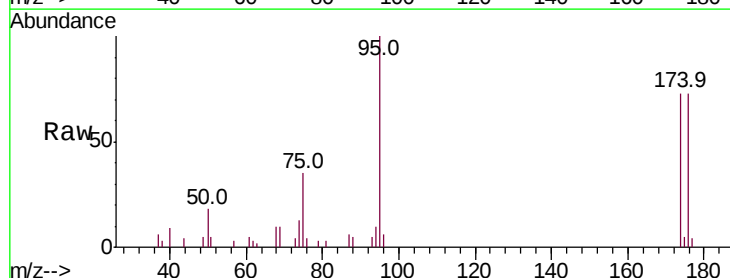

Abundance Ion 95.00 (94.70 to 95.70): VD060971.D (-1227) (-)

Ion 173.90 (173.60 to 174.60): VD060971.D (-1227) (-)

Ion 175.90 (175.60 to 176.60): VD060971.D (-1227) (-)

20000

15000

10000

5000


0


Time-->

13.50

13.55





13.60

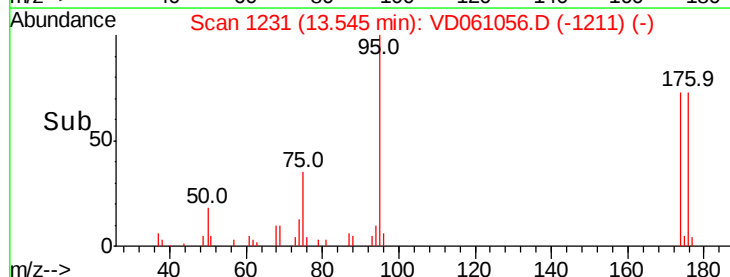

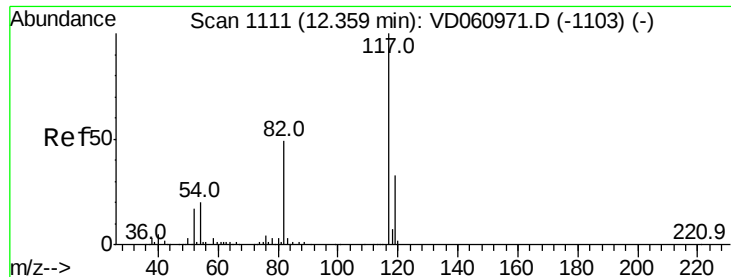

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.36 min Scan# 1111
Delta R.T. 0.01 min
Lab File: VD061056.D
Acq: 13 Mar 2019 21:39

Tot Ion:117 Resp: 47171
Ion Ratio Lower Upper
117 100
82 41.6 38.9 58.3
119 29.9 26.6 39.8

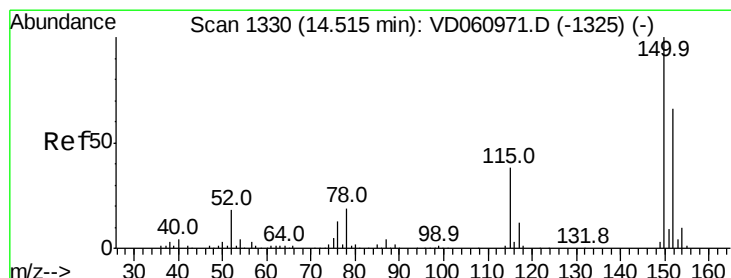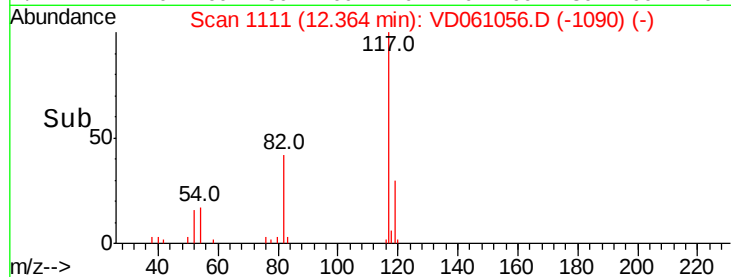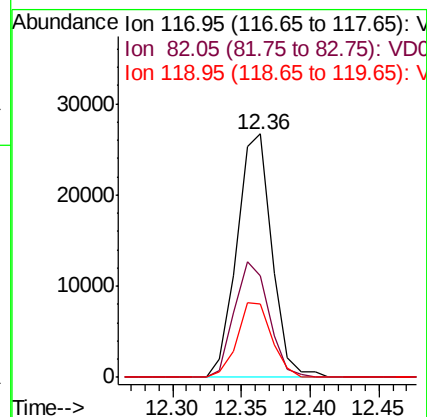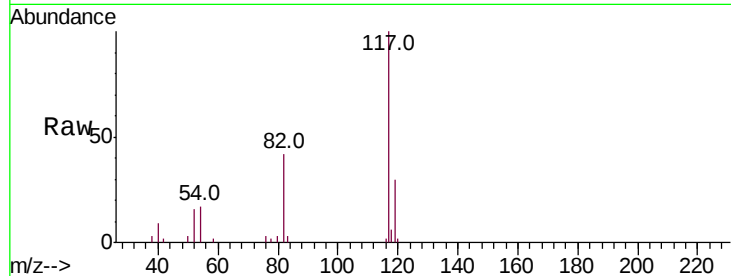

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 14.51 min Scan# 1329
Delta R.T. -0.00 min
Lab File: VD061056.D
Acq: 13 Mar 2019 21:39

Tgt Ion:152 Resp: 19067
Ion Ratio Lower Upper
152 100
115 55.4 28.6 85.9
150 162.5 0.0 310.6

