


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD031419\
Data File : VD061057.D
Acq On : 14 Mar 2019 9:48
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
Title : SW846 8260
Last Update : Fri Mar 08 02:35:39 2019

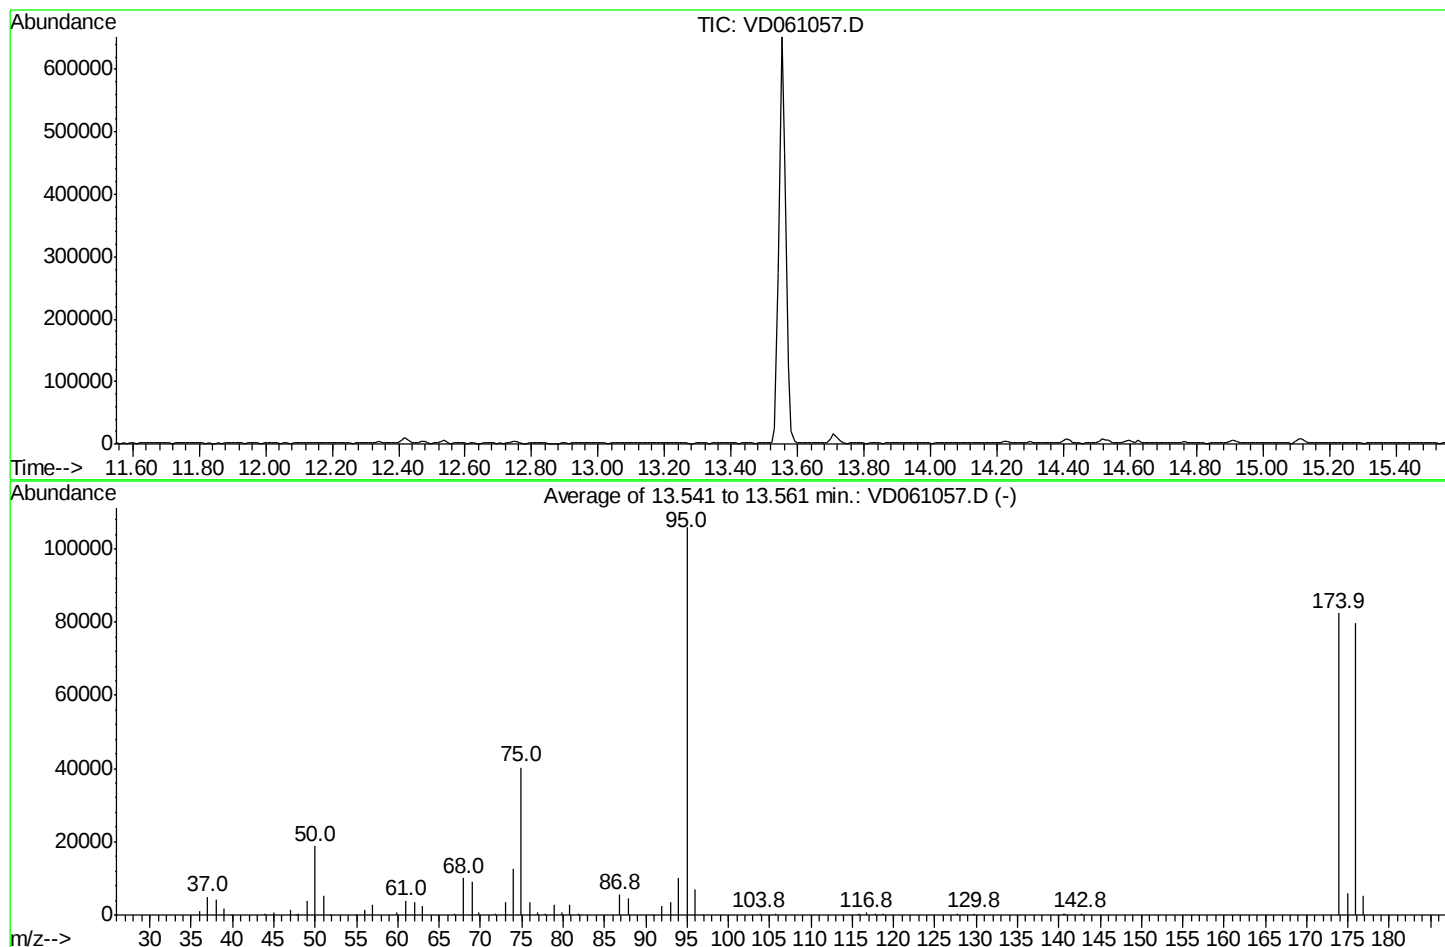

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	18861	PASS
75	95	30	60	38.0	40245	PASS
95	95	100	100	100.0	105874	PASS
96	95	5	9	6.6	6957	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.8	82405	PASS
175	174	5	9	7.1	5843	PASS
176	174	95	101	96.7	79685	PASS
177	176	5	9	6.7	5303	PASS