


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031422\
 Data File : VD072159.D
 Acq On : 14 Mar 2022 09:56
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M
 Title : SW846 8260
 Last Update : Mon Mar 14 05:18:06 2022

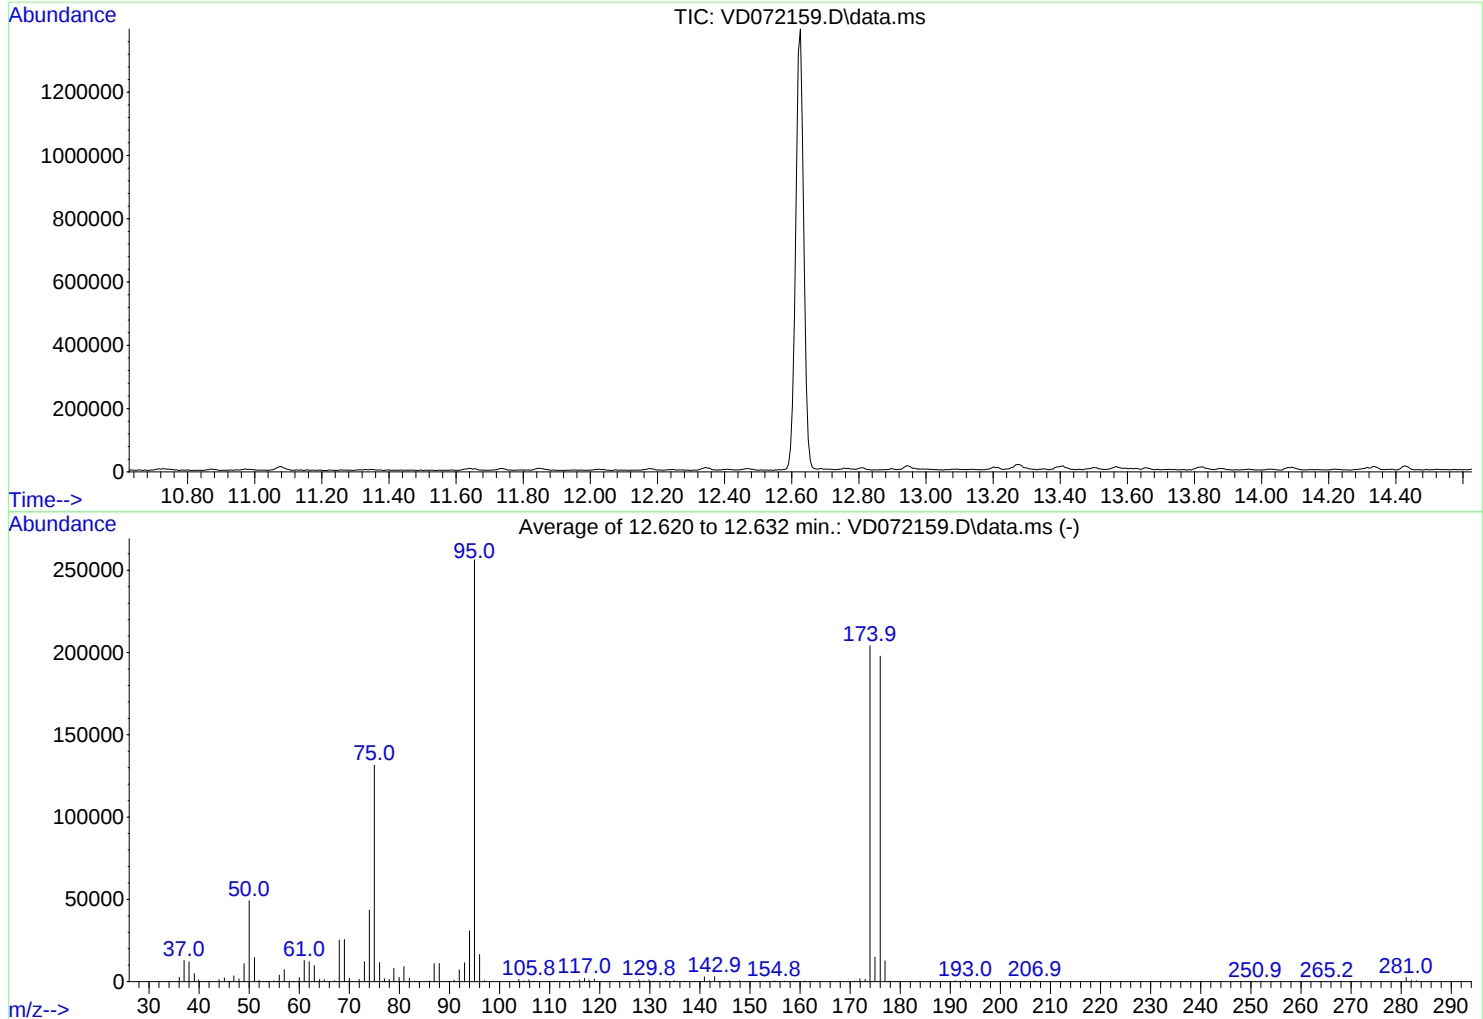

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	49216	PASS
75	95	30	60	51.3	131525	PASS
95	95	100	100	100.0	256341	PASS
96	95	5	9	6.4	16429	PASS
173	174	0.00	2	0.7	1506	PASS
174	95	50	100	79.7	204181	PASS
175	174	5	9	7.3	14872	PASS
176	174	95	101	96.9	197760	PASS
177	176	5	9	6.4	12614	PASS