


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031519\
Data File : VD061078.D
Acq On : 15 Mar 2019 9:50
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
Title : SW846 8260
Last Update : Fri Mar 08 02:35:39 2019

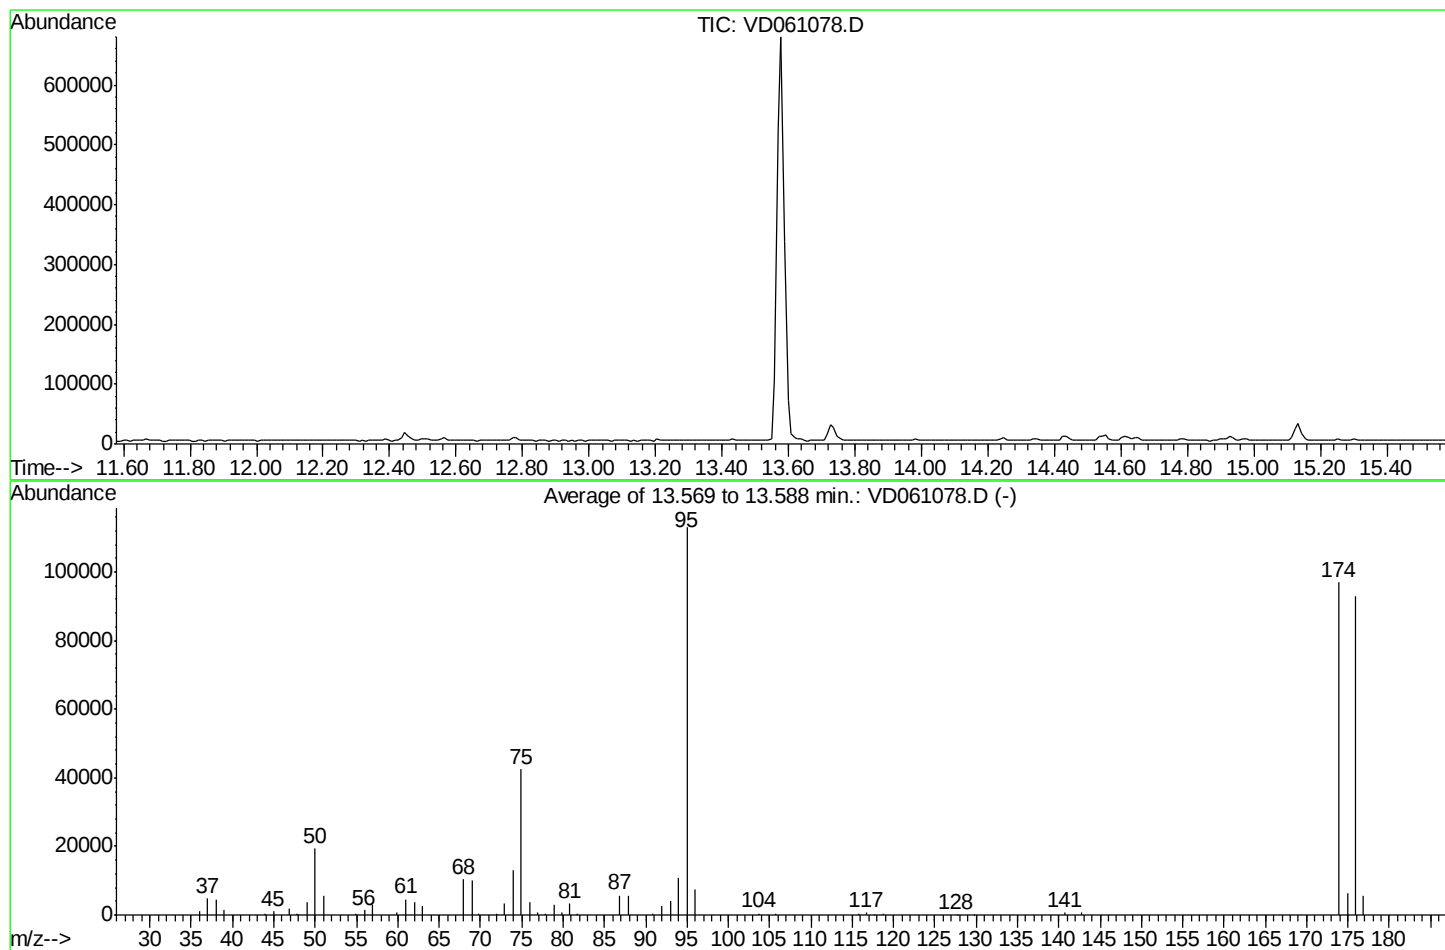

AutoFind: Scans 1234, 1235, 1236; Background Corrected with Scan 1229

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	19269	PASS
75	95	30	60	37.5	42410	PASS
95	95	100	100	100.0	113005	PASS
96	95	5	9	6.7	7552	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.8	96970	PASS
175	174	5	9	6.7	6460	PASS
176	174	95	101	95.8	92872	PASS
177	176	5	9	6.0	5539	PASS