


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD031521\  
Data File : VD068613.D  
Acq On : 15 Mar 2021 09:46  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D022621S.M  
Title : SW846 8260  
Last Update : Fri Feb 26 14:04:14 2021

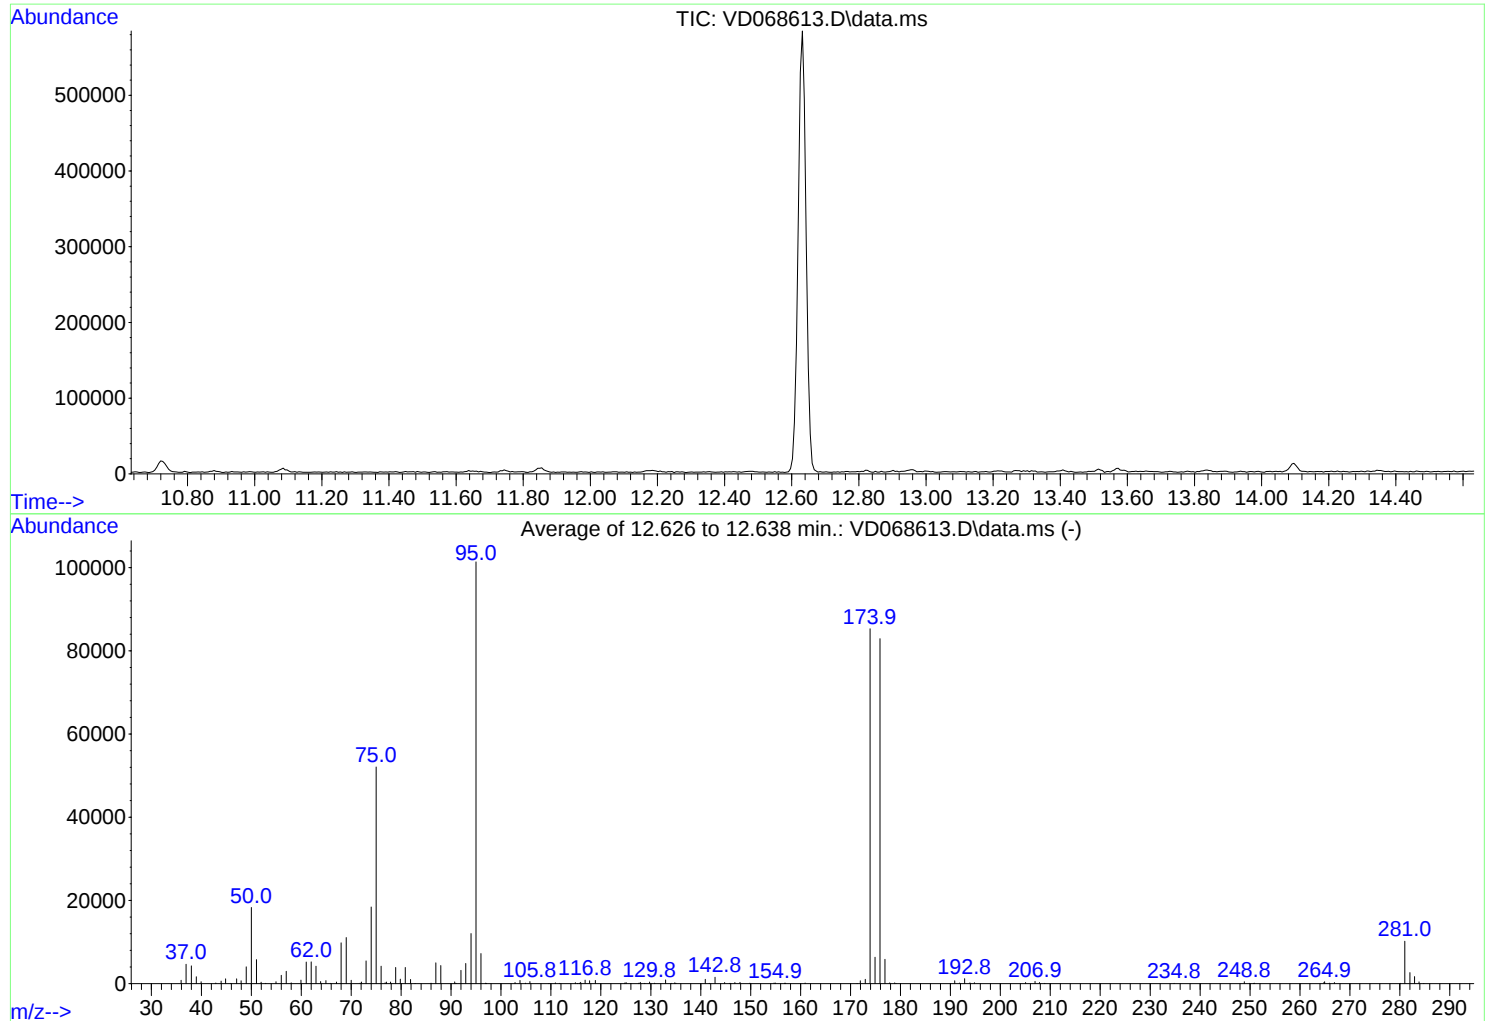

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.1         | 18329      | PASS                |
| 75             | 95              | 30              | 60              | 51.4         | 52085      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 101408     | PASS                |
| 96             | 95              | 5               | 9               | 7.1          | 7250       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.2          | 1027       | PASS                |
| 174            | 95              | 50              | 100             | 84.1         | 85312      | PASS                |
| 175            | 174             | 5               | 9               | 7.5          | 6363       | PASS                |
| 176            | 174             | 95              | 101             | 97.2         | 82944      | PASS                |
| 177            | 176             | 5               | 9               | 7.0          | 5842       | PASS                |