
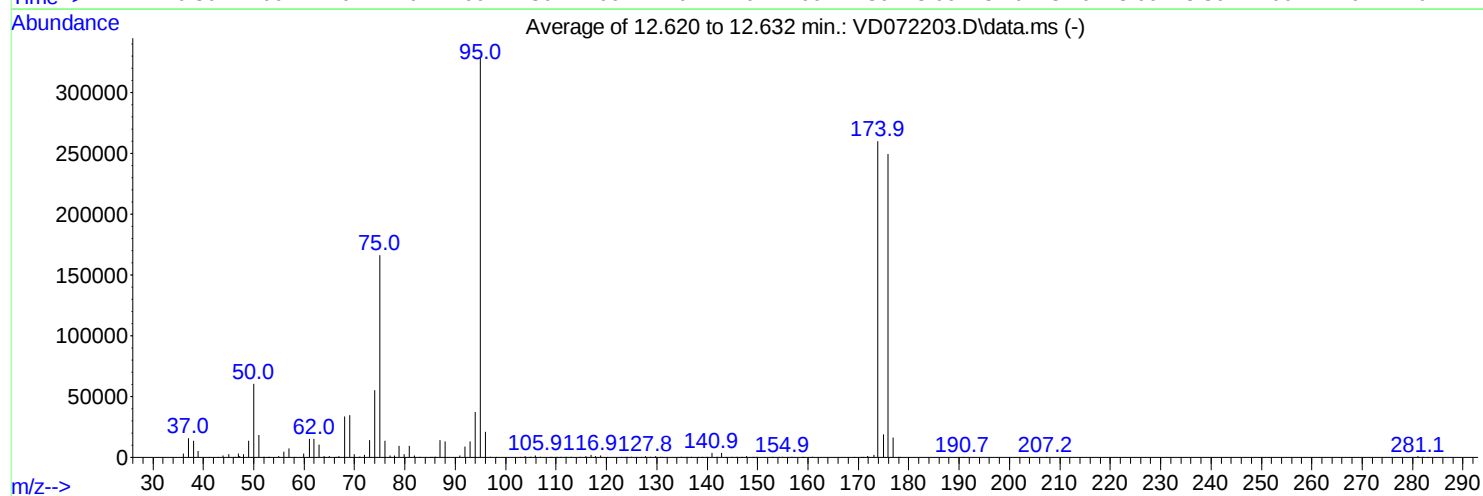


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031522\
 Data File : VD072203.D
 Acq On : 15 Mar 2022 22:26
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M
 Title : SW846 8260
 Last Update : Mon Mar 14 05:18:06 2022

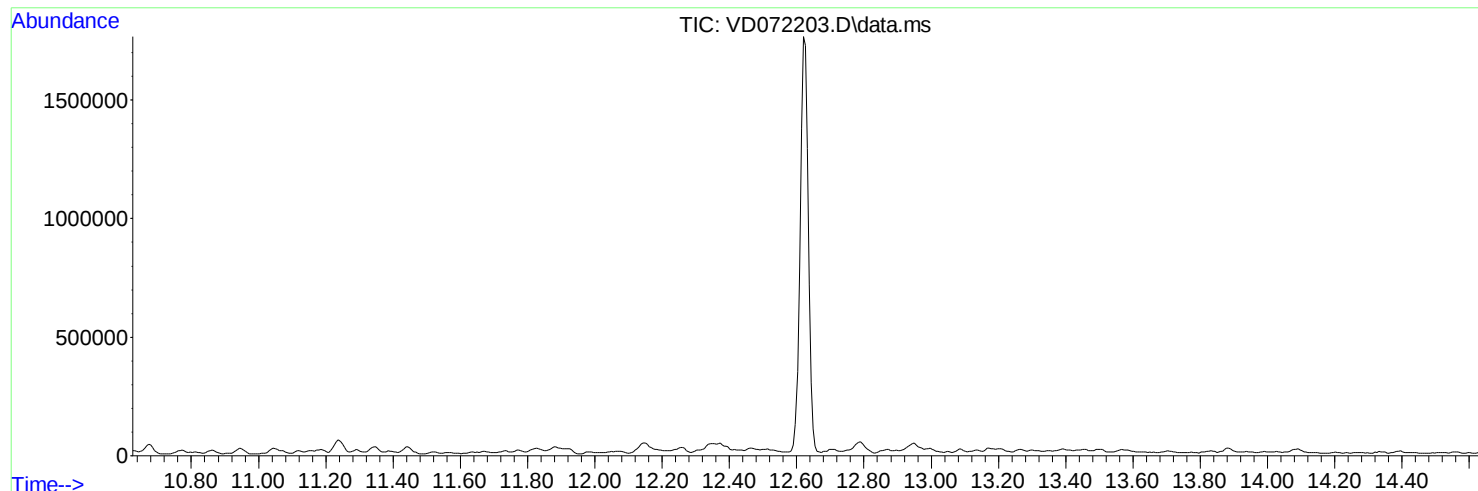

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1807

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	60515	PASS
75	95	30	60	50.7	166315	PASS
95	95	100	100	100.0	328141	PASS
96	95	5	9	6.4	21051	PASS
173	174	0.00	2	0.8	1980	PASS
174	95	50	100	79.3	260075	PASS
175	174	5	9	7.2	18824	PASS
176	174	95	101	95.9	249301	PASS
177	176	5	9	6.5	16081	PASS