
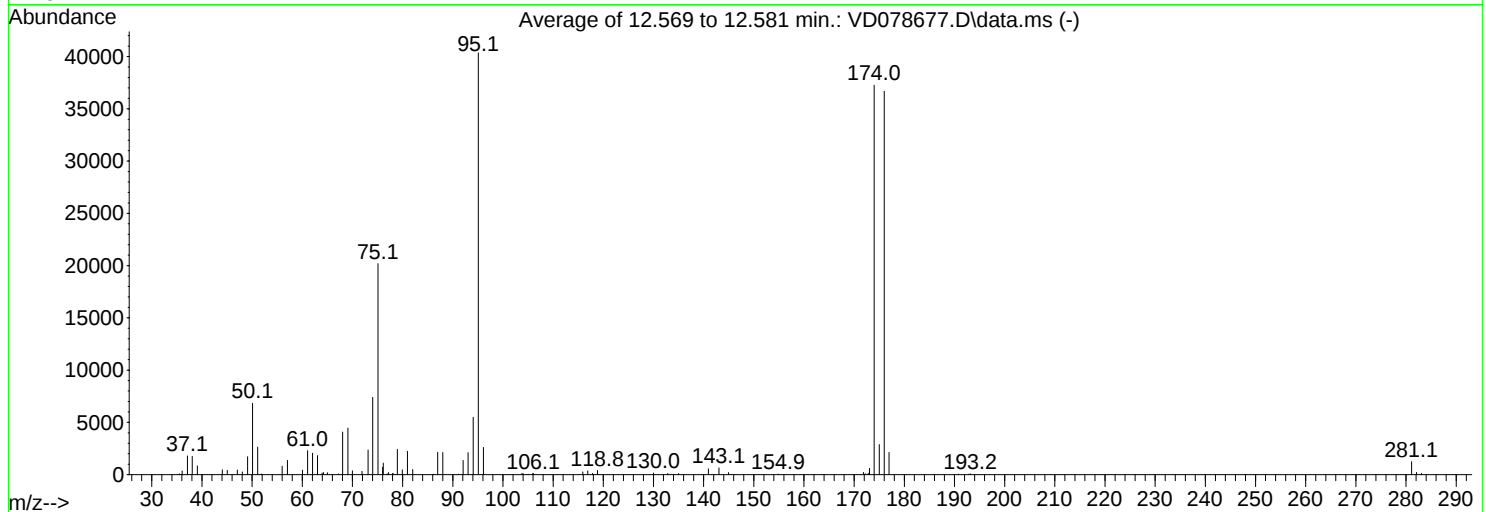


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031524\
Data File : VD078677.D
Acq On : 15 Mar 2024 08:40
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y022324S.M
Title : SW846 8260
Last Update : Sat Feb 24 04:41:20 2024

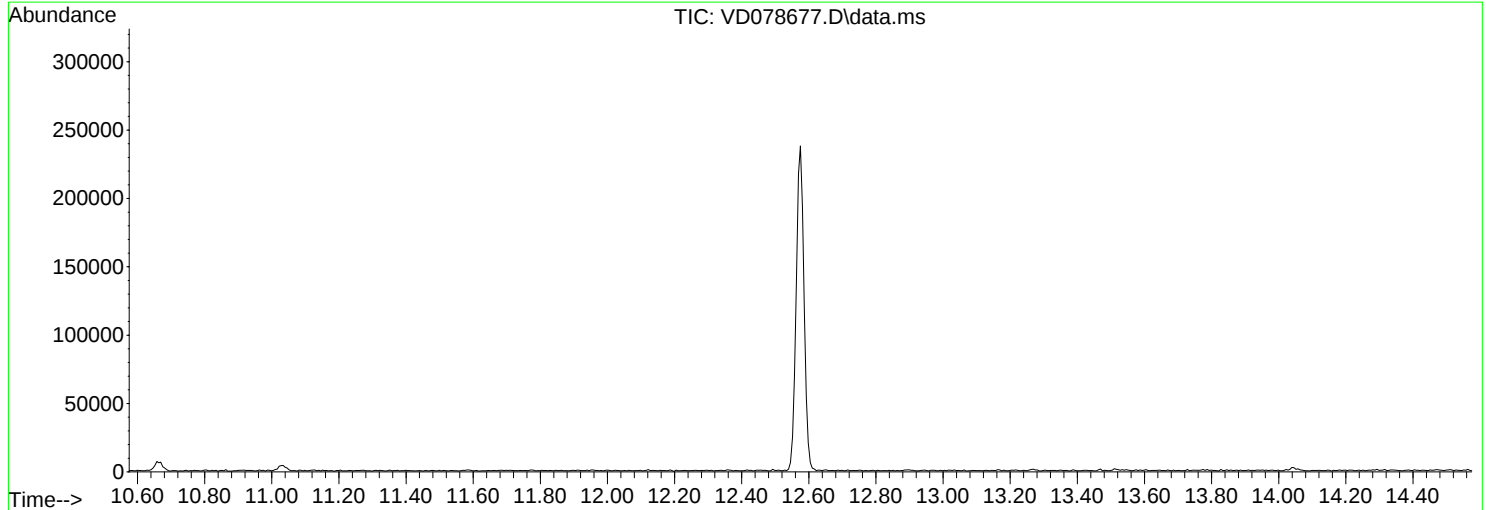

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	6827	PASS
75	95	30	60	50.0	20192	PASS
95	95	100	100	100.0	40355	PASS
96	95	5	9	6.4	2602	PASS
173	174	0.00	2	1.6	599	PASS
174	95	50	100	92.3	37256	PASS
175	174	5	9	7.7	2879	PASS
176	174	95	101	98.4	36672	PASS
177	176	5	9	5.8	2122	PASS