


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031621\
Data File : VD068622.D
Acq On : 16 Mar 2021 08:45
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
Title : SW846 8260
Last Update : Fri Feb 26 14:04:14 2021

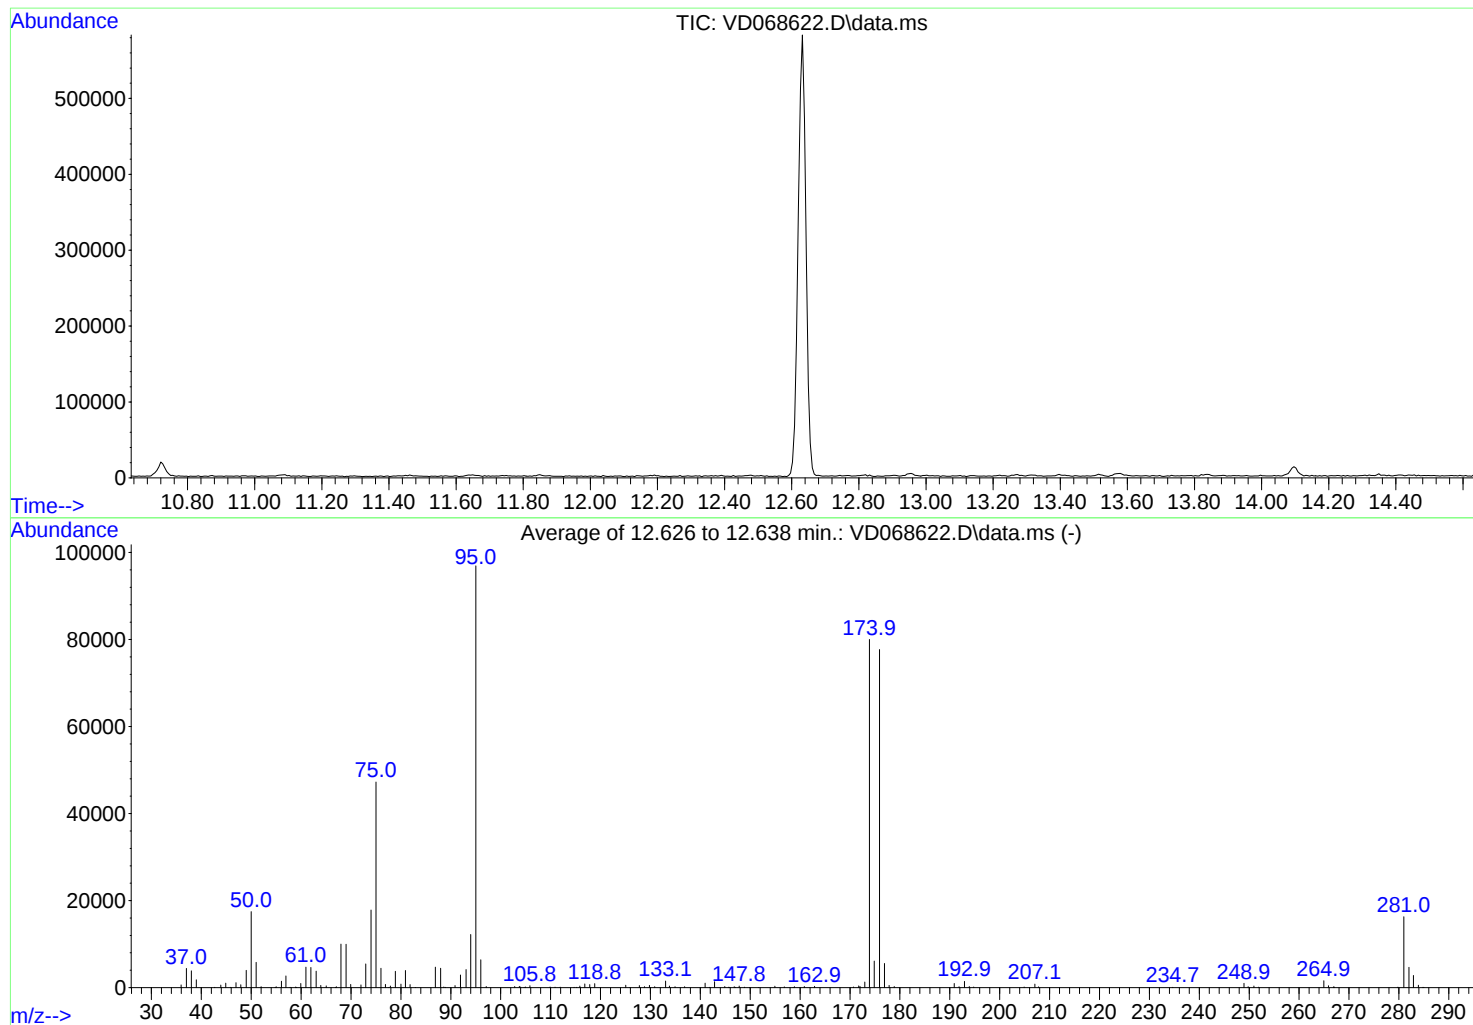

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	17481	PASS
75	95	30	60	48.8	47259	PASS
95	95	100	100	100.0	96936	PASS
96	95	5	9	6.6	6391	PASS
173	174	0.00	2	1.6	1276	PASS
174	95	50	100	82.5	80019	PASS
175	174	5	9	7.6	6120	PASS
176	174	95	101	97.1	77704	PASS
177	176	5	9	7.2	5566	PASS