

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031721\
 Data File : VD068640.D
 Acq On : 17 Mar 2021 16:21
 Operator : VA/SY
 Sample : M1689-01
 Misc : 5.80G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 R-LA-4-4-WC

Quant Time: Mar 18 00:56:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 26 14:04:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	271452	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	493040	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	491724	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	253756	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	148771	54.85	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 109.70%	
35) Dibromofluoromethane	7.920	113	153368	51.64	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 103.28%	
50) Toluene-d8	10.338	98	612172	51.75	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 103.50%	
62) 4-Bromofluorobenzene	12.632	95	208842	54.78	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 109.56%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031721\
Data File : VD068640.D
Acq On : 17 Mar 2021 16:21
Operator : VA/SY
Sample : M1689-01
Misc : 5.80G/5.00ml/MSVOA_D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
R-LA-4-4-WC

Quant Time: Mar 18 00:56:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
Quant Title : SW846 8260
QLast Update : Fri Feb 26 14:04:14 2021
Response via : Initial Calibration




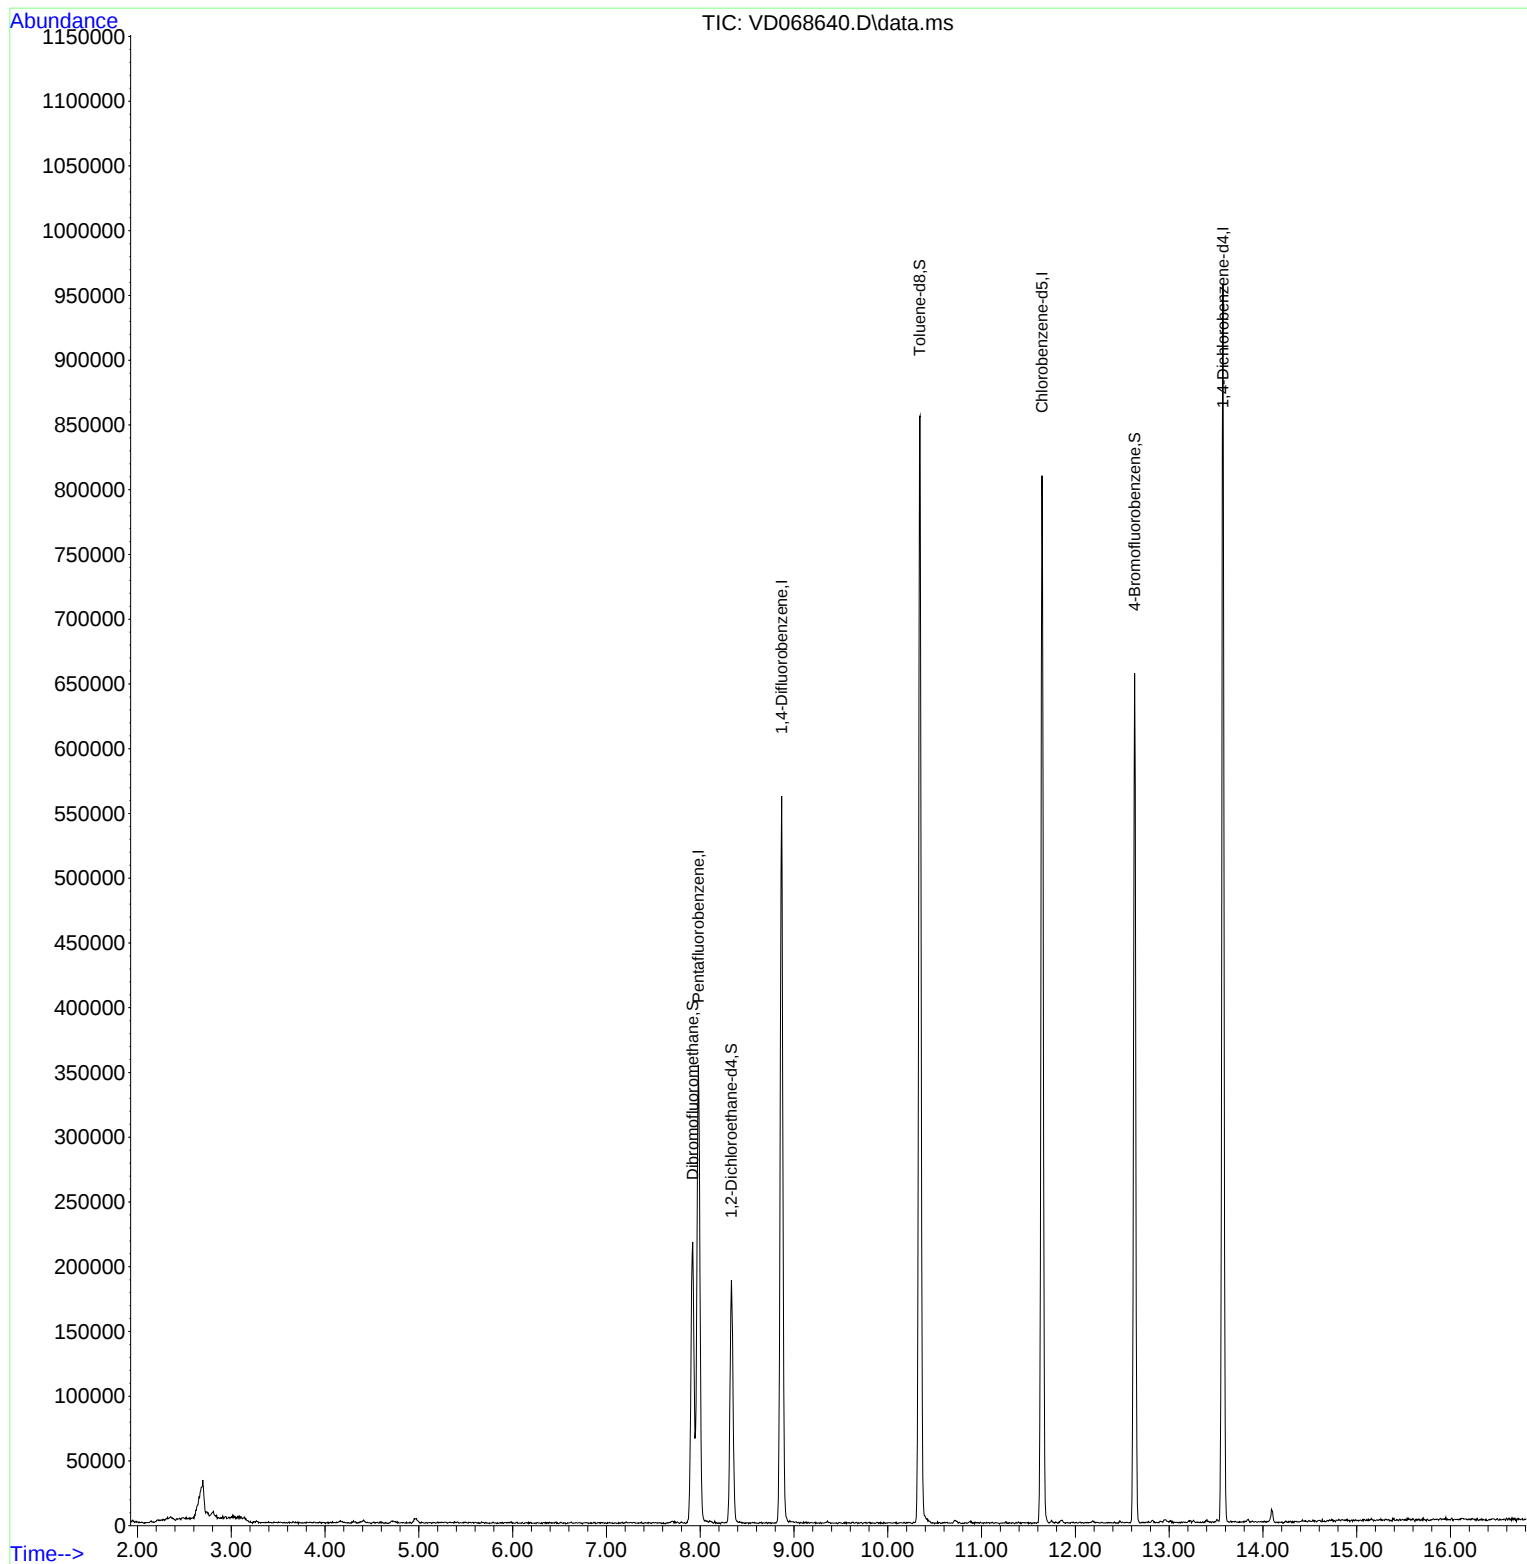


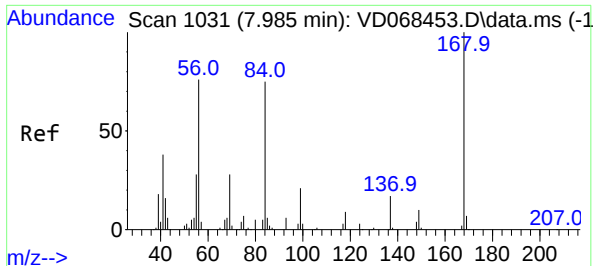

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD068640.D
Acq: 17 Mar 2021 16:21




Instrument :
MSVOA_D
ClientSampleId :
R-LA-4-4-WC


Tgt Ion:168 Resp: 271452
Ion Ratio Lower Upper
168 100
99 55.1 43.5 65.3

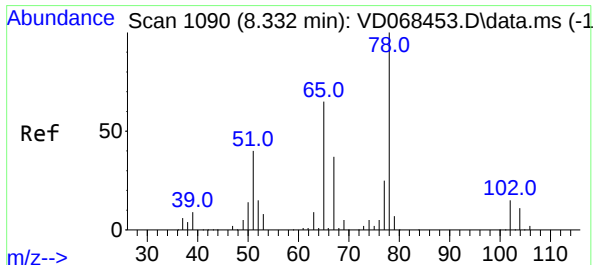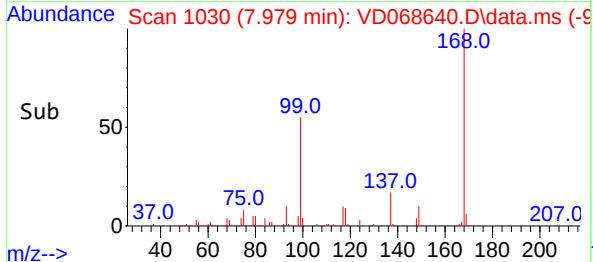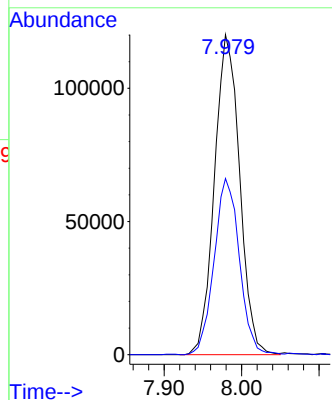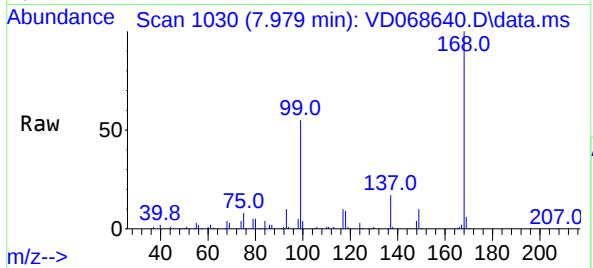

#33
1,2-Dichloroethane-d4
Concen: 54.85 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. 0.000 min
Lab File: VD068640.D
Acq: 17 Mar 2021 16:21

Tgt Ion: 65 Resp: 148771
Ion Ratio Lower Upper
65 100
67 52.4 0.0 105.0

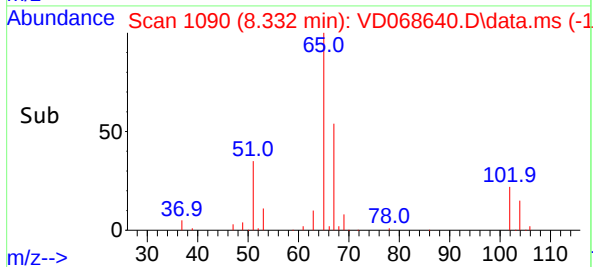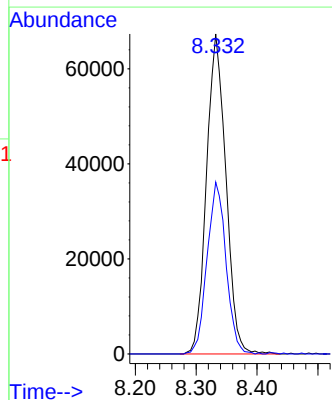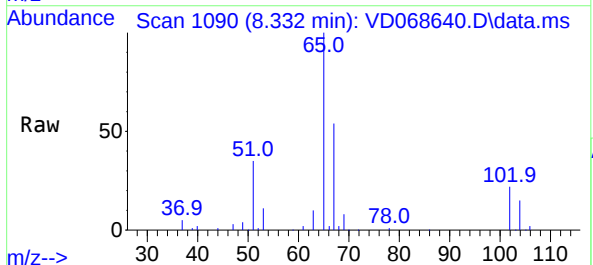




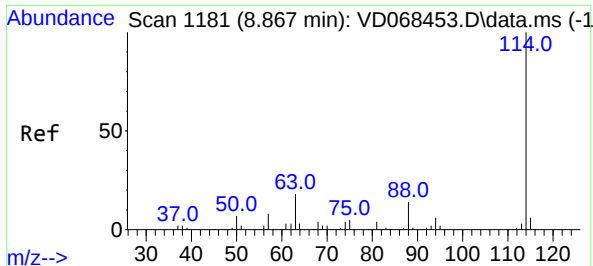


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068640.D
Acq: 17 Mar 2021 16:21

Instrument :
MSVOA_D
ClientSampleId :
R-LA-4-4-WC




Tgt Ion:114 Resp: 493040
Ion Ratio Lower Upper
114 100
63 18.7 0.0 34.8
88 14.2 0.0 31.6

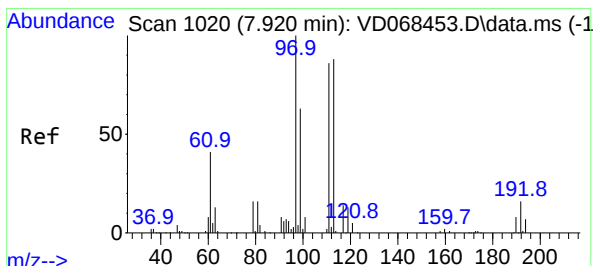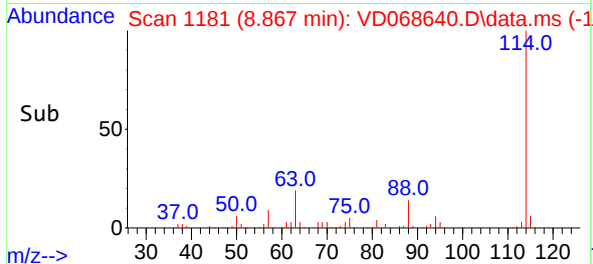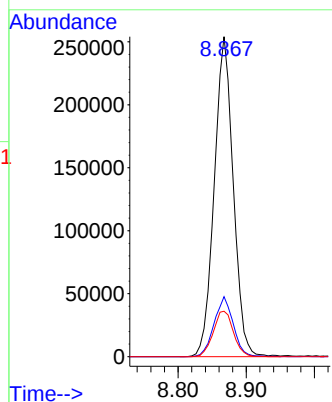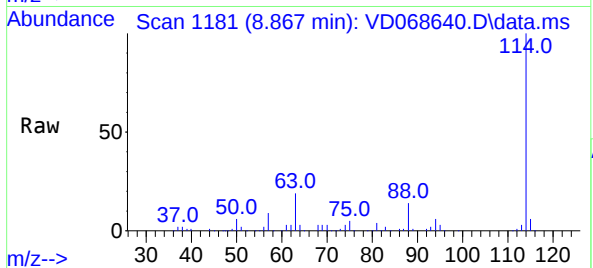


#35

Dibromofluoromethane
Concen: 51.64 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. 0.000 min
Lab File: VD068640.D
Acq: 17 Mar 2021 16:21

Tgt Ion:113 Resp: 153368
Ion Ratio Lower Upper
113 100
111 106.0 81.4 122.0
192 19.0 16.1 24.1


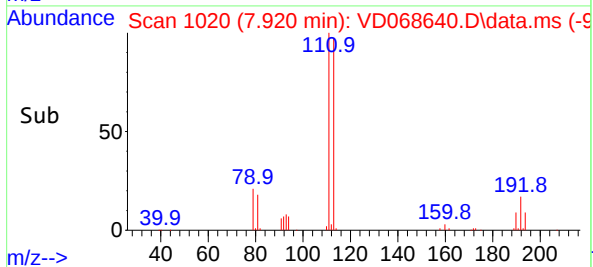
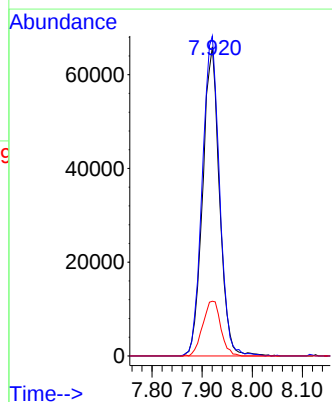
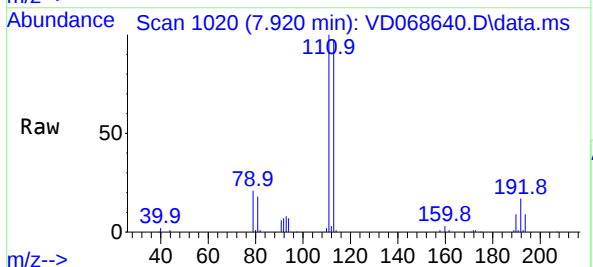


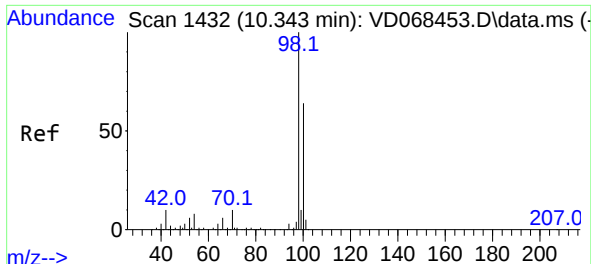

#50
Toluene-d8
Concen: 51.75 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.005 min
Lab File: VD068640.D
Acq: 17 Mar 2021 16:21




Instrument :
MSVOA_D
ClientSampleId :
R-LA-4-4-WC


Tgt Ion: 98 Resp: 612172
Ion Ratio Lower Upper
98 100
100 65.4 53.0 79.4

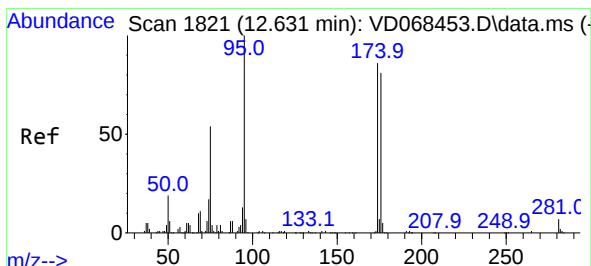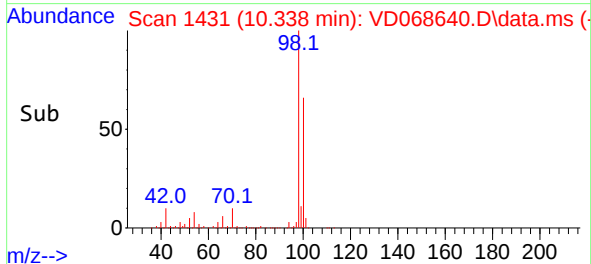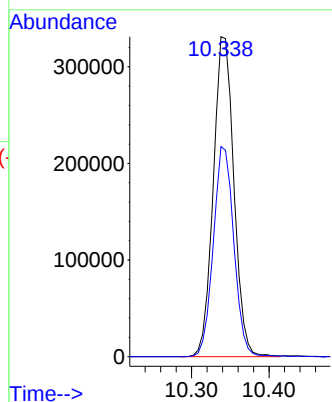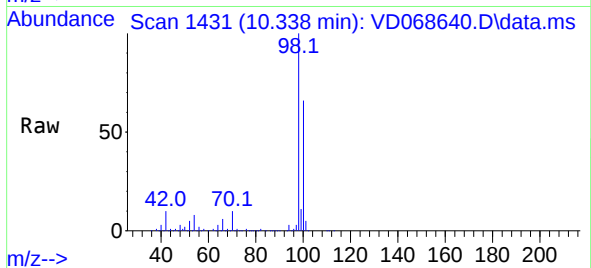

#62
4-Bromofluorobenzene
Concen: 54.78 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.000 min
Lab File: VD068640.D
Acq: 17 Mar 2021 16:21

Tgt Ion: 95 Resp: 208842
Ion Ratio Lower Upper
95 100
174 85.5 0.0 172.4
176 83.5 0.0 168.4


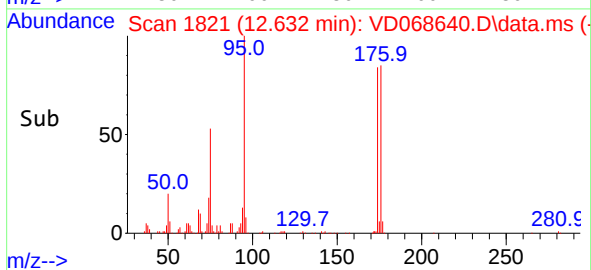
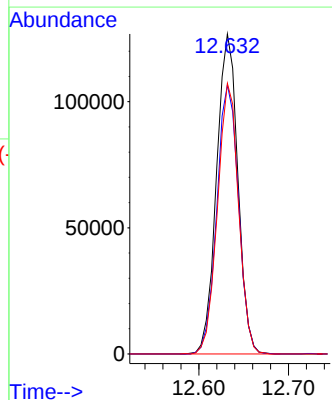
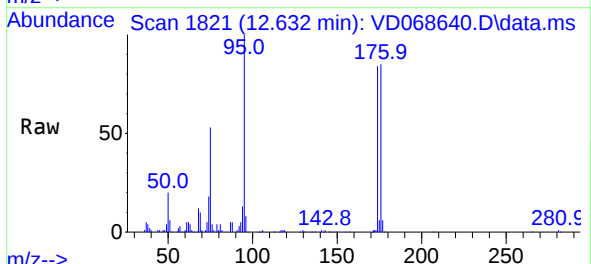


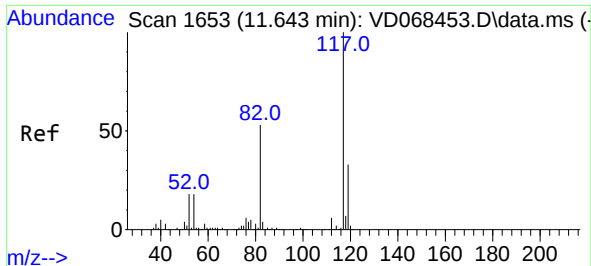

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. 0.000 min
Lab File: VD068640.D
Acq: 17 Mar 2021 16:21

Instrument :
MSVOA_D
ClientSampleId :
R-LA-4-4-WC

Tgt Ion:	117	Resp:	491724
Ion	Ratio	Lower	Upper
117	100		
82	50.6	41.4	62.0
119	30.8	26.1	39.1

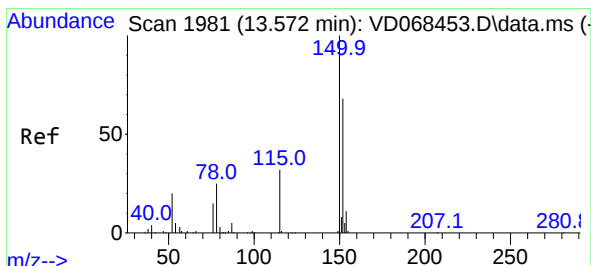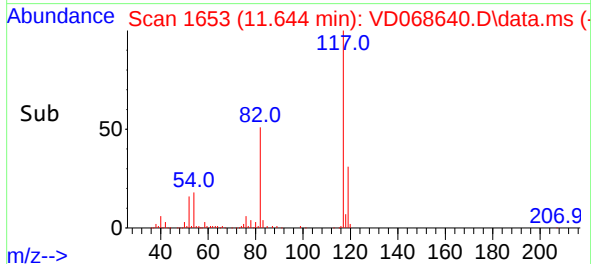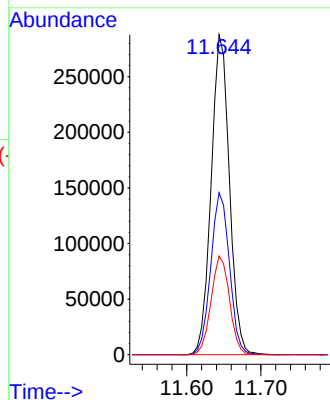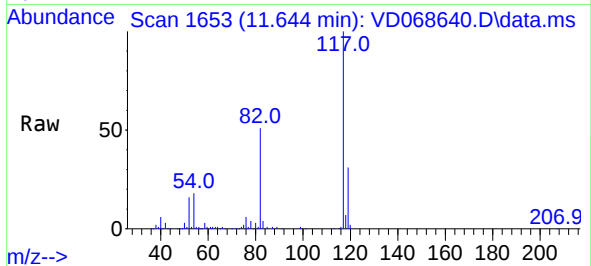

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. 0.001 min
Lab File: VD068640.D
Acq: 17 Mar 2021 16:21

Tgt Ion:	152	Resp:	253756
Ion	Ratio	Lower	Upper
152	100		
115	58.2	28.9	86.8
150	156.8	0.0	344.4

