


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031721\
Data File : VD068631.D
Acq On : 17 Mar 2021 09:20
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
Title : SW846 8260
Last Update : Fri Feb 26 14:04:14 2021

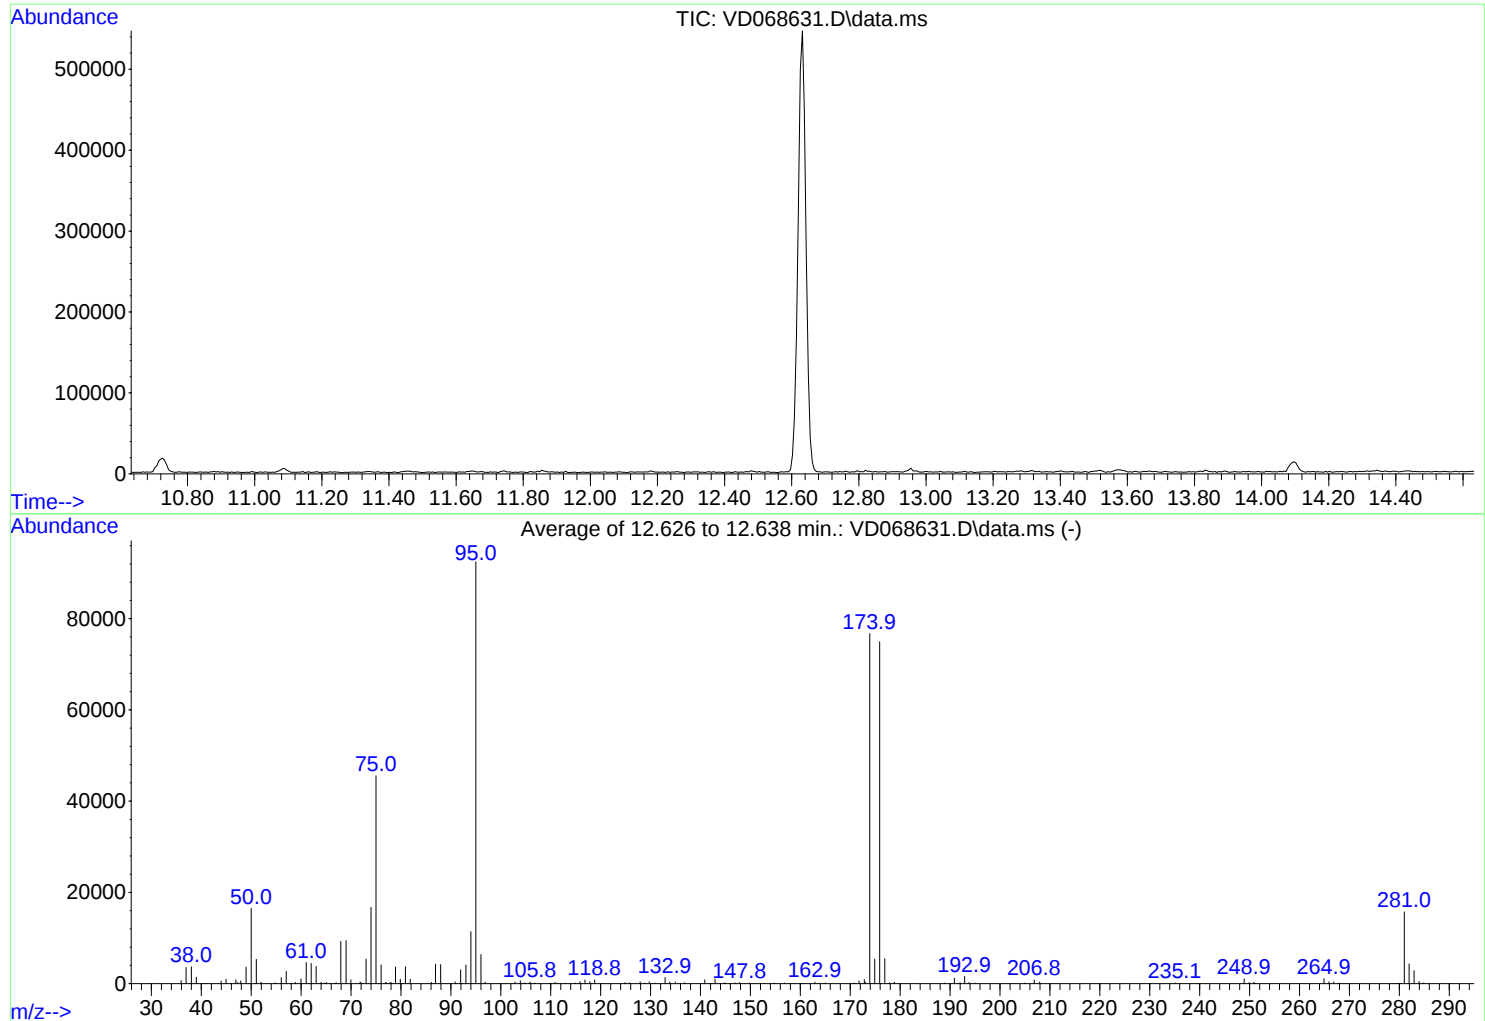

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	16477	PASS
75	95	30	60	49.3	45555	PASS
95	95	100	100	100.0	92453	PASS
96	95	5	9	6.9	6386	PASS
173	174	0.00	2	1.1	877	PASS
174	95	50	100	83.0	76723	PASS
175	174	5	9	7.0	5377	PASS
176	174	95	101	97.7	74965	PASS
177	176	5	9	7.3	5471	PASS