

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031822\
 Data File : VD072298.D
 Acq On : 18 Mar 2022 19:08
 Operator : VA/SY
 Sample : N1962-02
 Misc : 5.06G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C-17-16-17

Quant Time: Mar 19 05:27:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 14 05:18:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.973	168	340529	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	568490	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	624051	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	326735	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	167299	44.084	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	88.160%
35) Dibromofluoromethane	7.909	113	178192	44.542	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	89.080%
50) Toluene-d8	10.332	98	717589	49.056	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	98.120%
62) 4-Bromofluorobenzene	12.620	95	301352	53.020	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	106.040%
Target Compounds						
					Qvalue	
16) Acetone	4.144	43	18228	22.122	ug/l	100
17) Carbon Disulfide	4.409	76	29934	5.478	ug/l	97
40) Benzene	8.344	78	43608	2.724	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031822\
Data File : VD072298.D
Acq On : 18 Mar 2022 19:08
Operator : VA/SY
Sample : N1962-02
Misc : 5.06G/5.00ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C-17-16-17

Quant Time: Mar 19 05:27:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M
Quant Title : SW846 8260
QLast Update : Mon Mar 14 05:18:06 2022
Response via : Initial Calibration




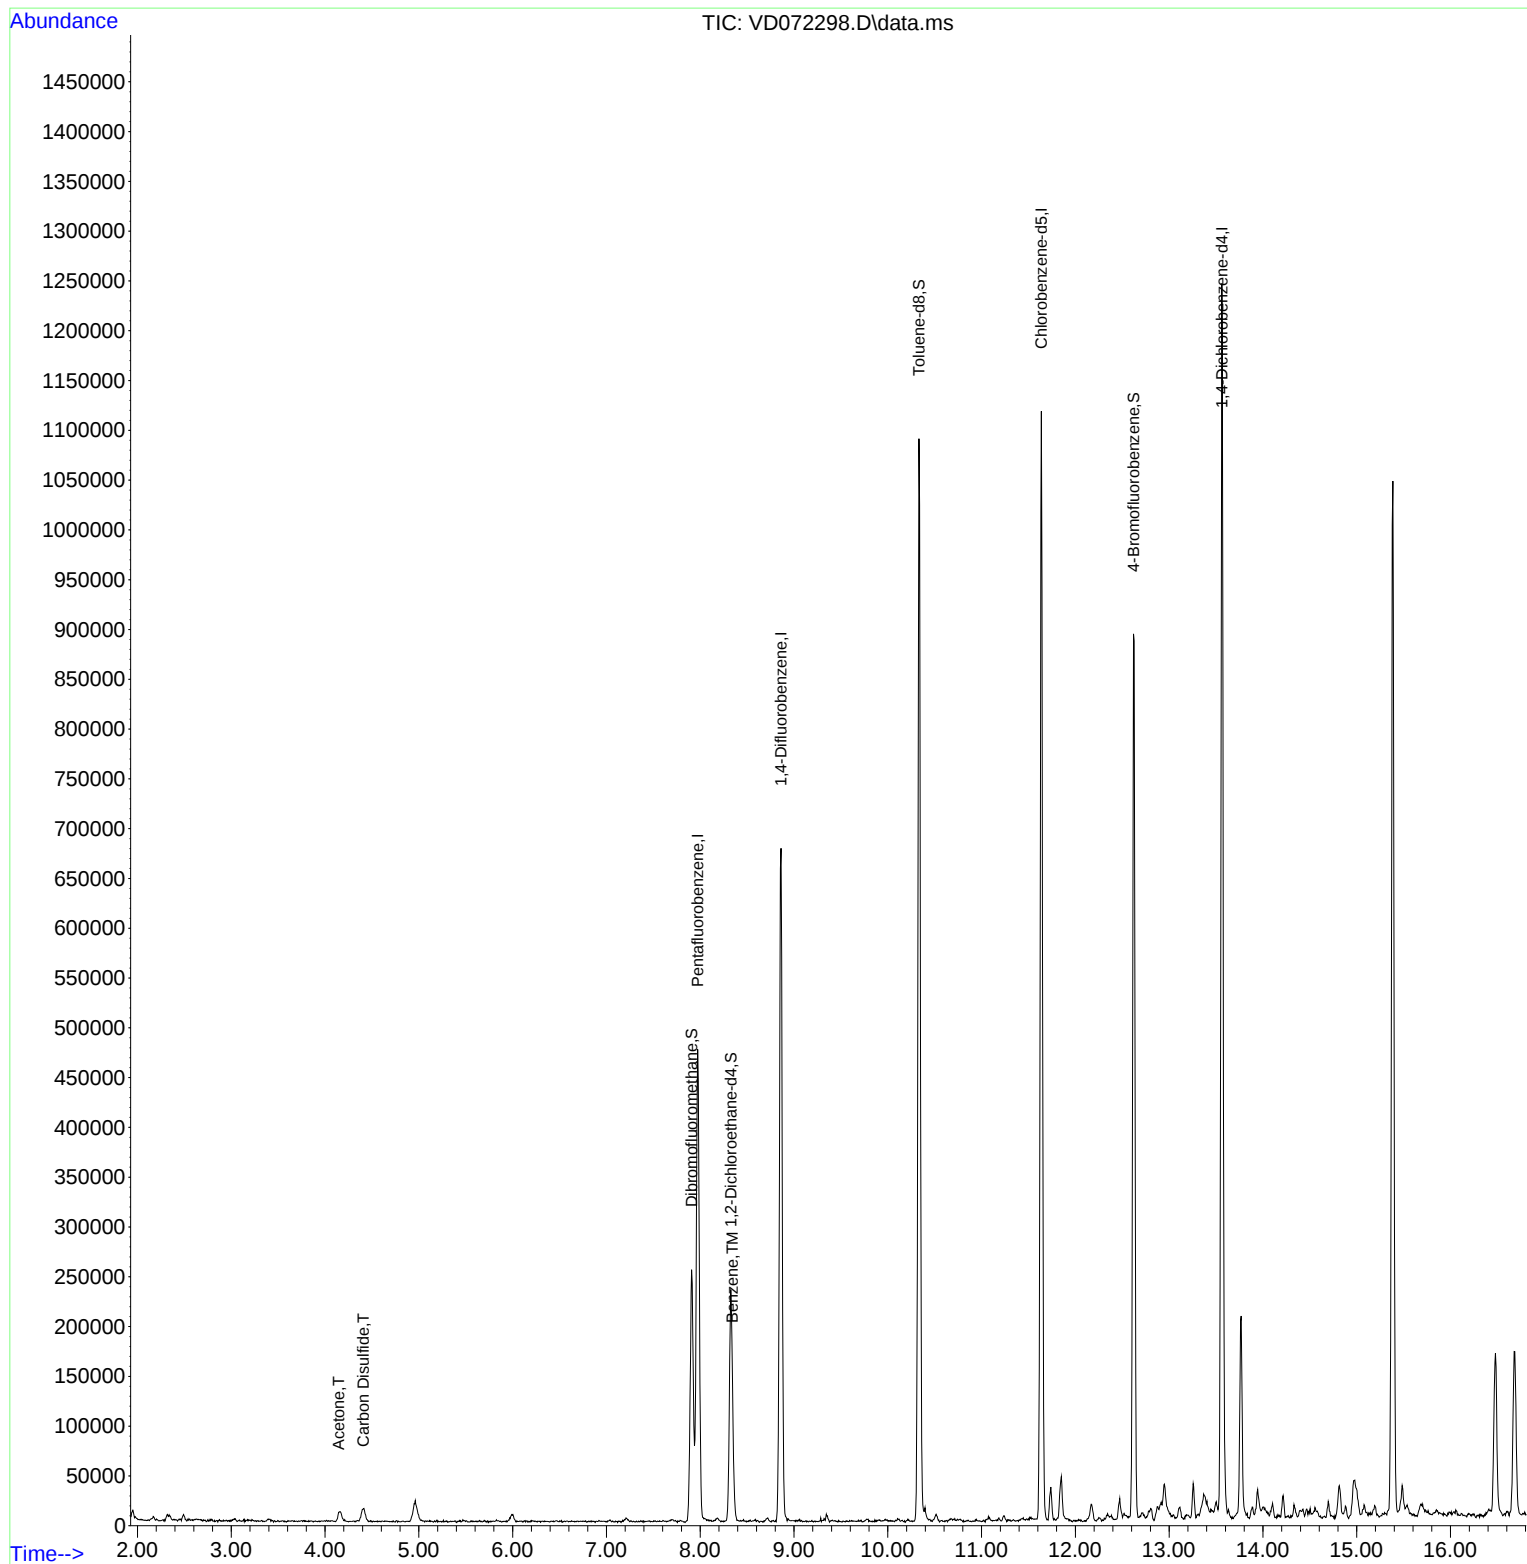


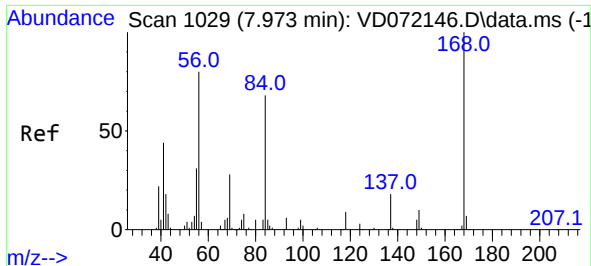

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. 0.000 min
Lab File: VD072298.D
Acq: 18 Mar 2022 19:08




Instrument :
MSVOA_D
ClientSampleId :
C-17-16-17


Tgt Ion:168 Resp: 340529
Ion Ratio Lower Upper
168 100
99 59.2 49.8 74.6

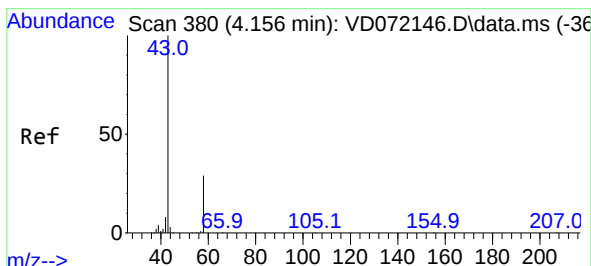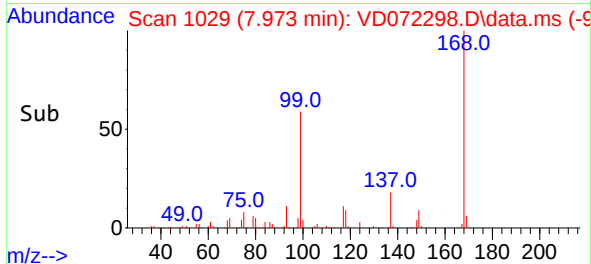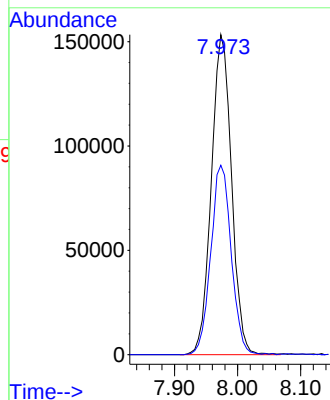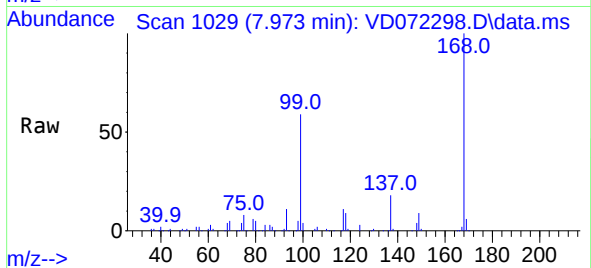

#16
Acetone
Concen: 22.122 ug/l
RT: 4.144 min Scan# 378
Delta R.T. -0.012 min
Lab File: VD072298.D
Acq: 18 Mar 2022 19:08

Tgt Ion: 43 Resp: 18228
Ion Ratio Lower Upper
43 100
58 27.6 22.1 33.1


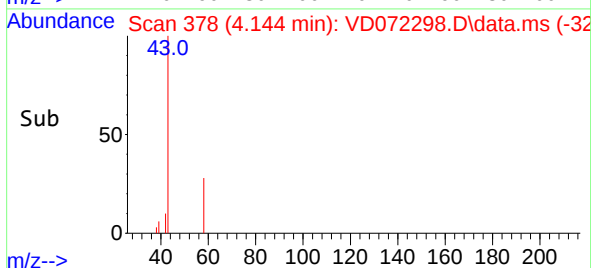
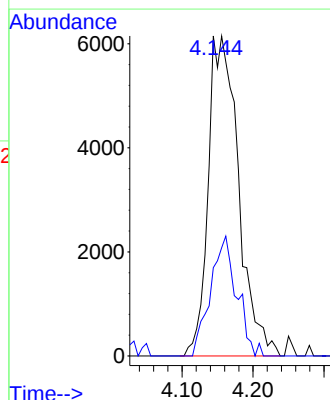
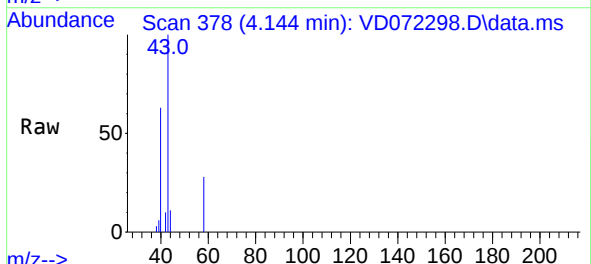


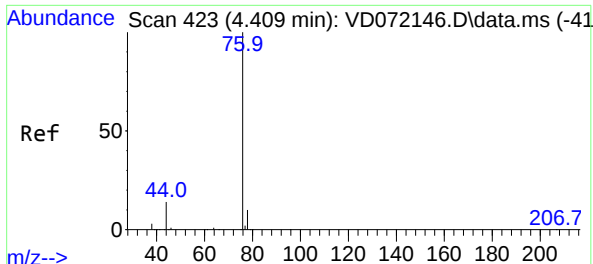

#17
Carbon Disulfide
Concen: 5.478 ug/l
RT: 4.409 min Scan# 41
Delta R.T. -0.000 min
Lab File: VD072298.D
Acq: 18 Mar 2022 19:08




Instrument :
MSVOA_D
ClientSampleId :
C-17-16-17


Tgt Ion: 76 Resp: 29934
Ion Ratio Lower Upper
76 100
78 8.5 7.5 11.3

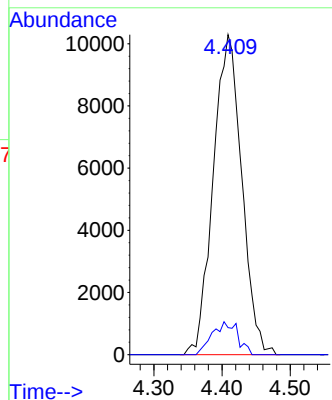

#33
1,2-Dichloroethane-d4
Concen: 44.084 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD072298.D
Acq: 18 Mar 2022 19:08

Tgt Ion: 65 Resp: 167299
Ion Ratio Lower Upper
65 100
67 51.5 0.0 101.4

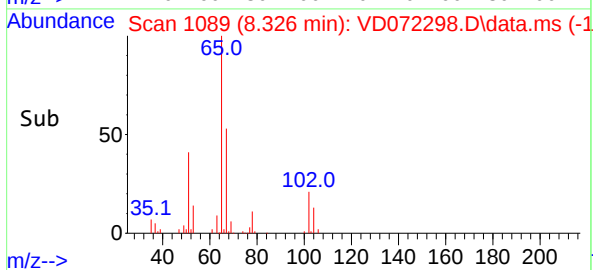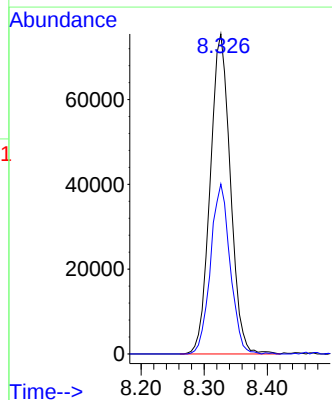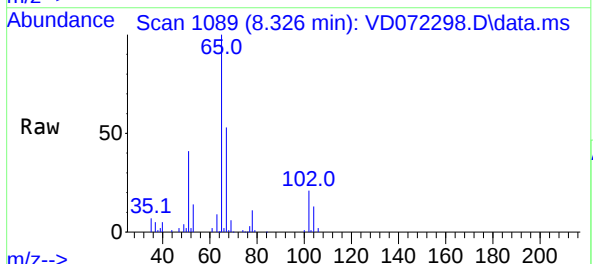



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VD072298.D

Acq: 18 Mar 2022 19:08

Instrument :

MSVOA_D

ClientSampleId :

C-17-16-17





Tgt Ion:114 Resp: 568490

Ion Ratio Lower Upper

114 100

63 20.4 0.0 46.6

88 15.9 0.0 33.2

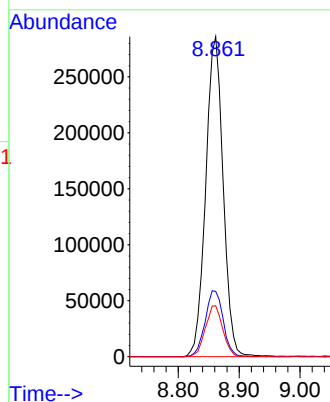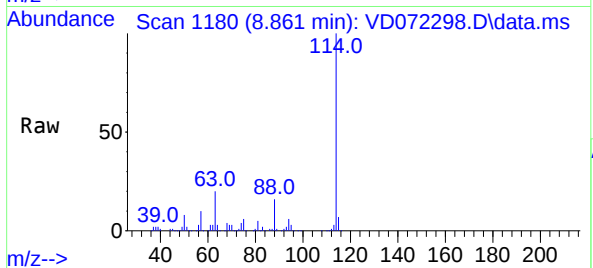

#35

Dibromofluoromethane

Concen: 44.542 ug/l

RT: 7.909 min Scan# 1018

Delta R.T. 0.000 min

Lab File: VD072298.D

Acq: 18 Mar 2022 19:08




Tgt Ion:113 Resp: 178192


Ion Ratio Lower Upper

113 100

111 101.7 83.8 125.6

192 18.7 14.6 21.8


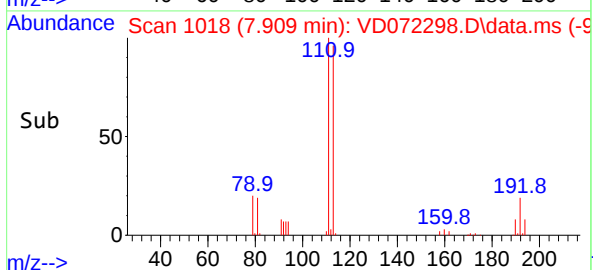
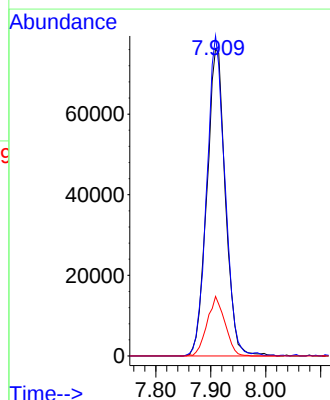





#40
Benzene
Concen: 2.724 ug/l
RT: 8.344 min Scan# 1092
Delta R.T. 0.000 min
Lab File: VD072298.D
Acq: 18 Mar 2022 19:08




Instrument :
MSVOA_D
ClientSampleId :
C-17-16-17


Tgt Ion: 78 Resp: 43608
Ion Ratio Lower Upper
78 100
77 22.0 19.1 28.7

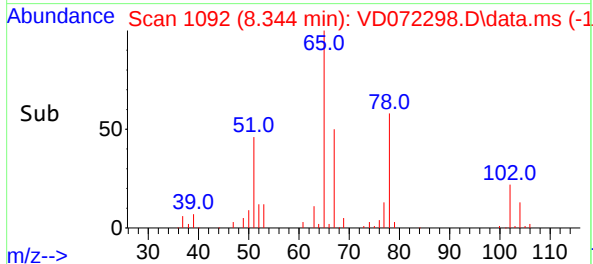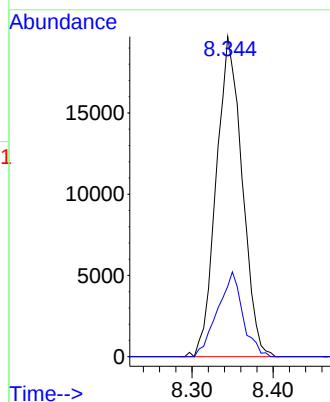

#50
Toluene-d8
Concen: 49.056 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. 0.000 min
Lab File: VD072298.D
Acq: 18 Mar 2022 19:08

Tgt Ion: 98 Resp: 717589
Ion Ratio Lower Upper
98 100
100 66.2 52.4 78.6


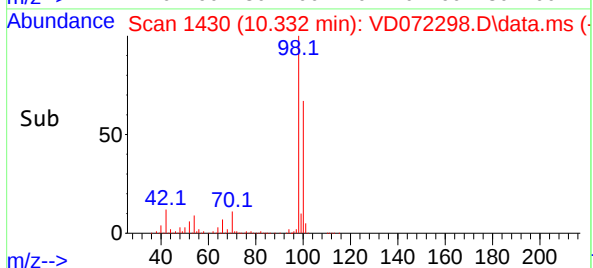
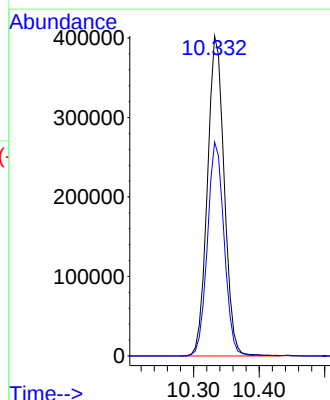
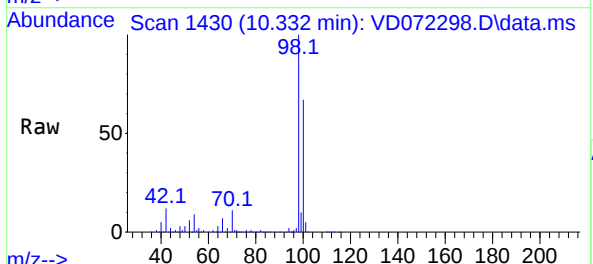


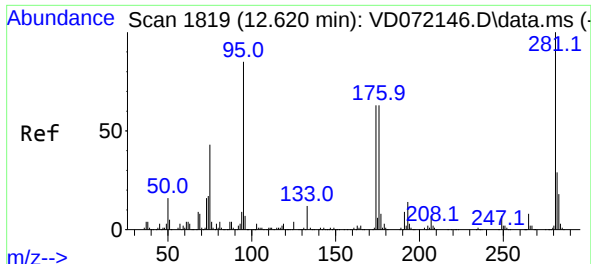

#62
4-Bromofluorobenzene
Concen: 53.020 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.000 min
Lab File: VD072298.D
Acq: 18 Mar 2022 19:08




Instrument :
MSVOA_D
ClientSampleId :
C-17-16-17


Tgt Ion: 95 Resp: 301352
Ion Ratio Lower Upper
95 100
174 79.9 0.0 152.8
176 74.8 0.0 145.4

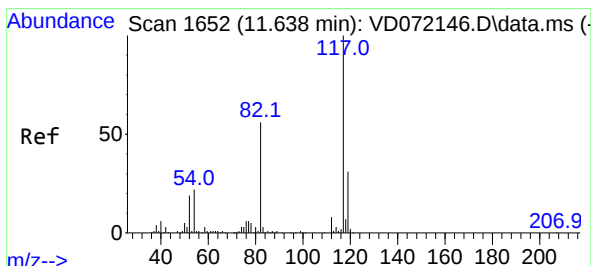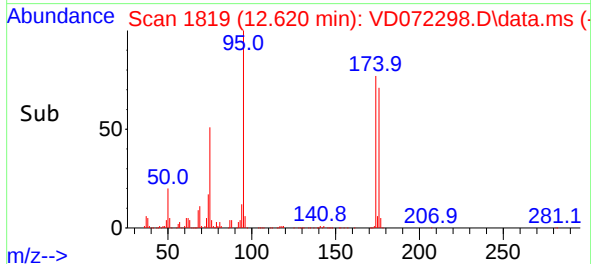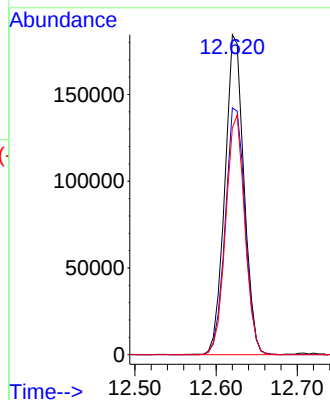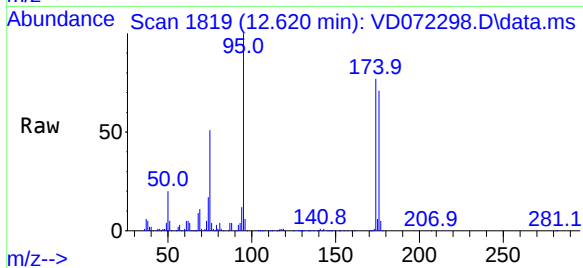

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1652
Delta R.T. 0.000 min
Lab File: VD072298.D
Acq: 18 Mar 2022 19:08

Tgt Ion: 117 Resp: 624051
Ion Ratio Lower Upper
117 100
82 55.6 45.3 67.9
119 30.0 26.6 40.0

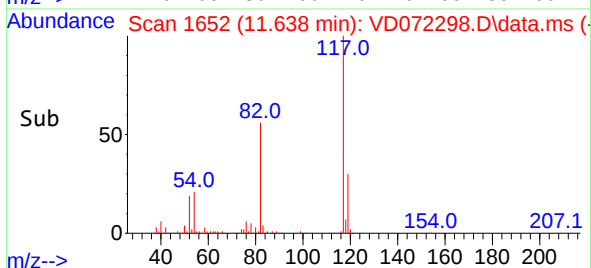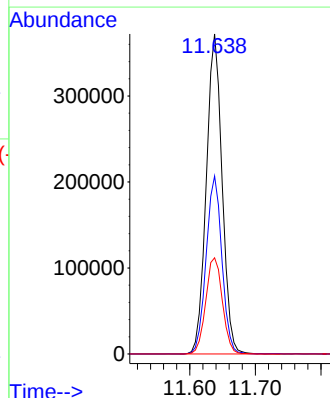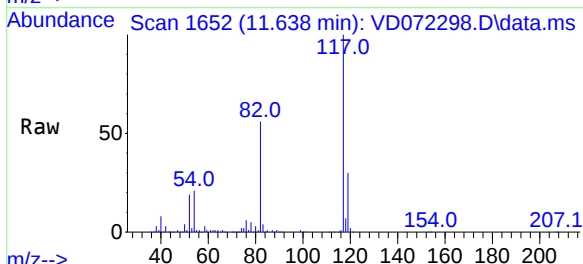

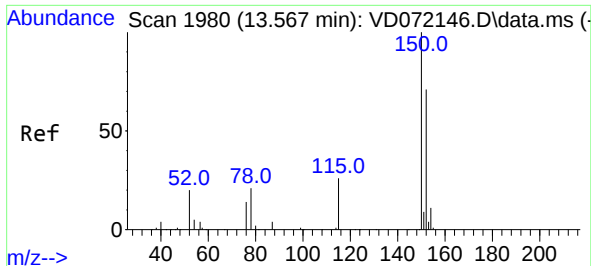

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.561 min Scan# 19

Delta R.T. -0.006 min

Lab File: VD072298.D


Acq: 18 Mar 2022 19:08

Instrument :

MSVOA_D

ClientSampleId :

C-17-16-17

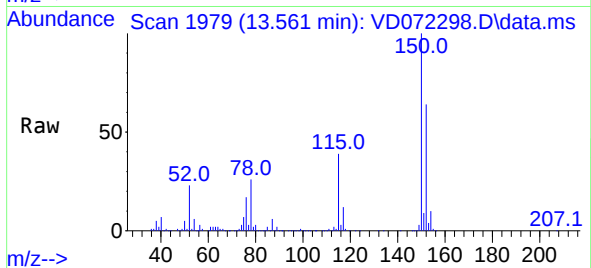

Tgt Ion:152 Resp: 326735

Ion Ratio Lower Upper

152 100

115 58.8 31.3 93.8

150 153.4 0.0 348.6

