

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031822\
 Data File : VD072303.D
 Acq On : 18 Mar 2022 21:31
 Operator : VA/SY
 Sample : N1962-09
 Misc : 5.10G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C-22-23-25

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M
 Title : SW846 8260

Signal : TIC: VD072303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.156	371	380	394	rBV3	14325	46030	1.97%	0.271%
2	4.409	414	423	433	rBV2	10866	28328	1.21%	0.167%
3	4.956	507	516	517	rBV	25090	46079	1.97%	0.271%
4	7.909	1008	1018	1023	rBV	256611	593479	25.43%	3.497%
5	7.973	1023	1029	1039	rVB	496271	1105540	47.36%	6.514%
6	8.332	1080	1090	1103	rBV3	327902	947261	40.58%	5.581%
7	8.861	1171	1180	1194	rBV	694607	1421153	60.89%	8.373%
8	9.350	1250	1263	1270	rBV5	25824	60909	2.61%	0.359%
9	10.120	1383	1394	1403	rVB6	9343	26769	1.15%	0.158%
10	10.332	1422	1430	1438	rBV	1139951	2058891	88.21%	12.131%
11	10.514	1454	1461	1471	rVB8	15442	40765	1.75%	0.240%
12	10.767	1499	1504	1509	rBV6	12488	26883	1.15%	0.158%
13	11.238	1579	1584	1589	rVB4	26824	46688	2.00%	0.275%
14	11.420	1607	1615	1616	rBV4	14717	24600	1.05%	0.145%
15	11.520	1627	1632	1636	rBV3	16168	27678	1.19%	0.163%
16	11.638	1644	1652	1662	rBV	1170903	1992405	85.36%	11.739%
17	11.738	1662	1669	1678	rVV	454440	760396	32.58%	4.480%
18	11.844	1678	1687	1696	rBV	160185	345737	14.81%	2.037%
19	12.167	1731	1742	1751	rBV6	38554	130410	5.59%	0.768%
20	12.261	1754	1758	1762	rVB2	17326	26463	1.13%	0.156%
21	12.349	1764	1773	1774	rBV7	19282	35014	1.50%	0.206%
22	12.473	1787	1794	1799	rBV	67006	116954	5.01%	0.689%
23	12.538	1799	1805	1809	rVV8	14140	32531	1.39%	0.192%
24	12.626	1813	1820	1829	rVB	926033	1597493	68.44%	9.412%
25	12.720	1833	1836	1843	rVB6	21990	39425	1.69%	0.232%
26	12.797	1843	1849	1855	rVB4	26360	67317	2.88%	0.397%
27	12.873	1857	1862	1865	rBV4	29463	53787	2.30%	0.317%
28	12.908	1865	1868	1870	rVV	22226	33119	1.42%	0.195%
29	12.944	1870	1874	1881	rVB6	51056	98682	4.23%	0.581%
30	13.108	1895	1902	1910	rVB2	33237	65303	2.80%	0.385%
31	13.173	1910	1913	1920	rVB9	15802	28233	1.21%	0.166%
32	13.255	1920	1927	1934	rBV	128909	214664	9.20%	1.265%
33	13.455	1955	1961	1965	rBV4	15395	28376	1.22%	0.167%
34	13.561	1972	1979	1990	rBV2	1282199	2334127	100.00%	13.752%
35	13.767	2007	2014	2023	rVB	752445	1249343	53.53%	7.361%
36	13.885	2029	2034	2038	rBV5	29563	50651	2.17%	0.298%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031822\
 Data File : VD072303.D
 Acq On : 18 Mar 2022 21:31
 Operator : VA/SY
 Sample : N1962-09
 Misc : 5.10G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C-22-23-25

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M
 Title : SW846 8260

37	13.944	2039	2044	2050	rVB2	64794	102266	4.38%	0.603%
38	14.102	2065	2071	2076	rVB5	25493	47270	2.03%	0.279%
39	14.208	2084	2089	2095	rVB3	33551	60036	2.57%	0.354%
40	14.338	2107	2111	2116	rBV6	18022	32494	1.39%	0.191%
41	14.467	2130	2133	2137	rVB2	26131	34856	1.49%	0.205%
42	14.538	2141	2145	2159	rVB2	27502	65462	2.80%	0.386%
43	14.696	2168	2172	2176	rBV3	19906	33191	1.42%	0.196%
44	14.808	2184	2191	2198	rBV4	53701	140795	6.03%	0.830%
45	14.967	2212	2218	2223	rVB5	19774	36369	1.56%	0.214%
46	15.079	2233	2237	2242	rBV8	13604	23677	1.01%	0.140%
47	15.190	2251	2256	2263	rVB7	23738	49329	2.11%	0.291%
48	15.385	2278	2289	2297	rBV2	184046	365907	15.68%	2.156%
49	15.679	2332	2339	2342	rBV9	10434	25948	1.11%	0.153%
50	16.479	2468	2475	2480	rBV3	26695	50354	2.16%	0.297%
51	16.679	2503	2509	2519	rBV3	44704	103021	4.41%	0.607%


Sum of corrected areas: 16972458

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031822\
Data File : VD072303.D
Acq On : 18 Mar 2022 21:31
Operator : VA/SY
Sample : N1962-09
Misc : 5.10G/5.00ml/MSVOA_D/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C-22-23-25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

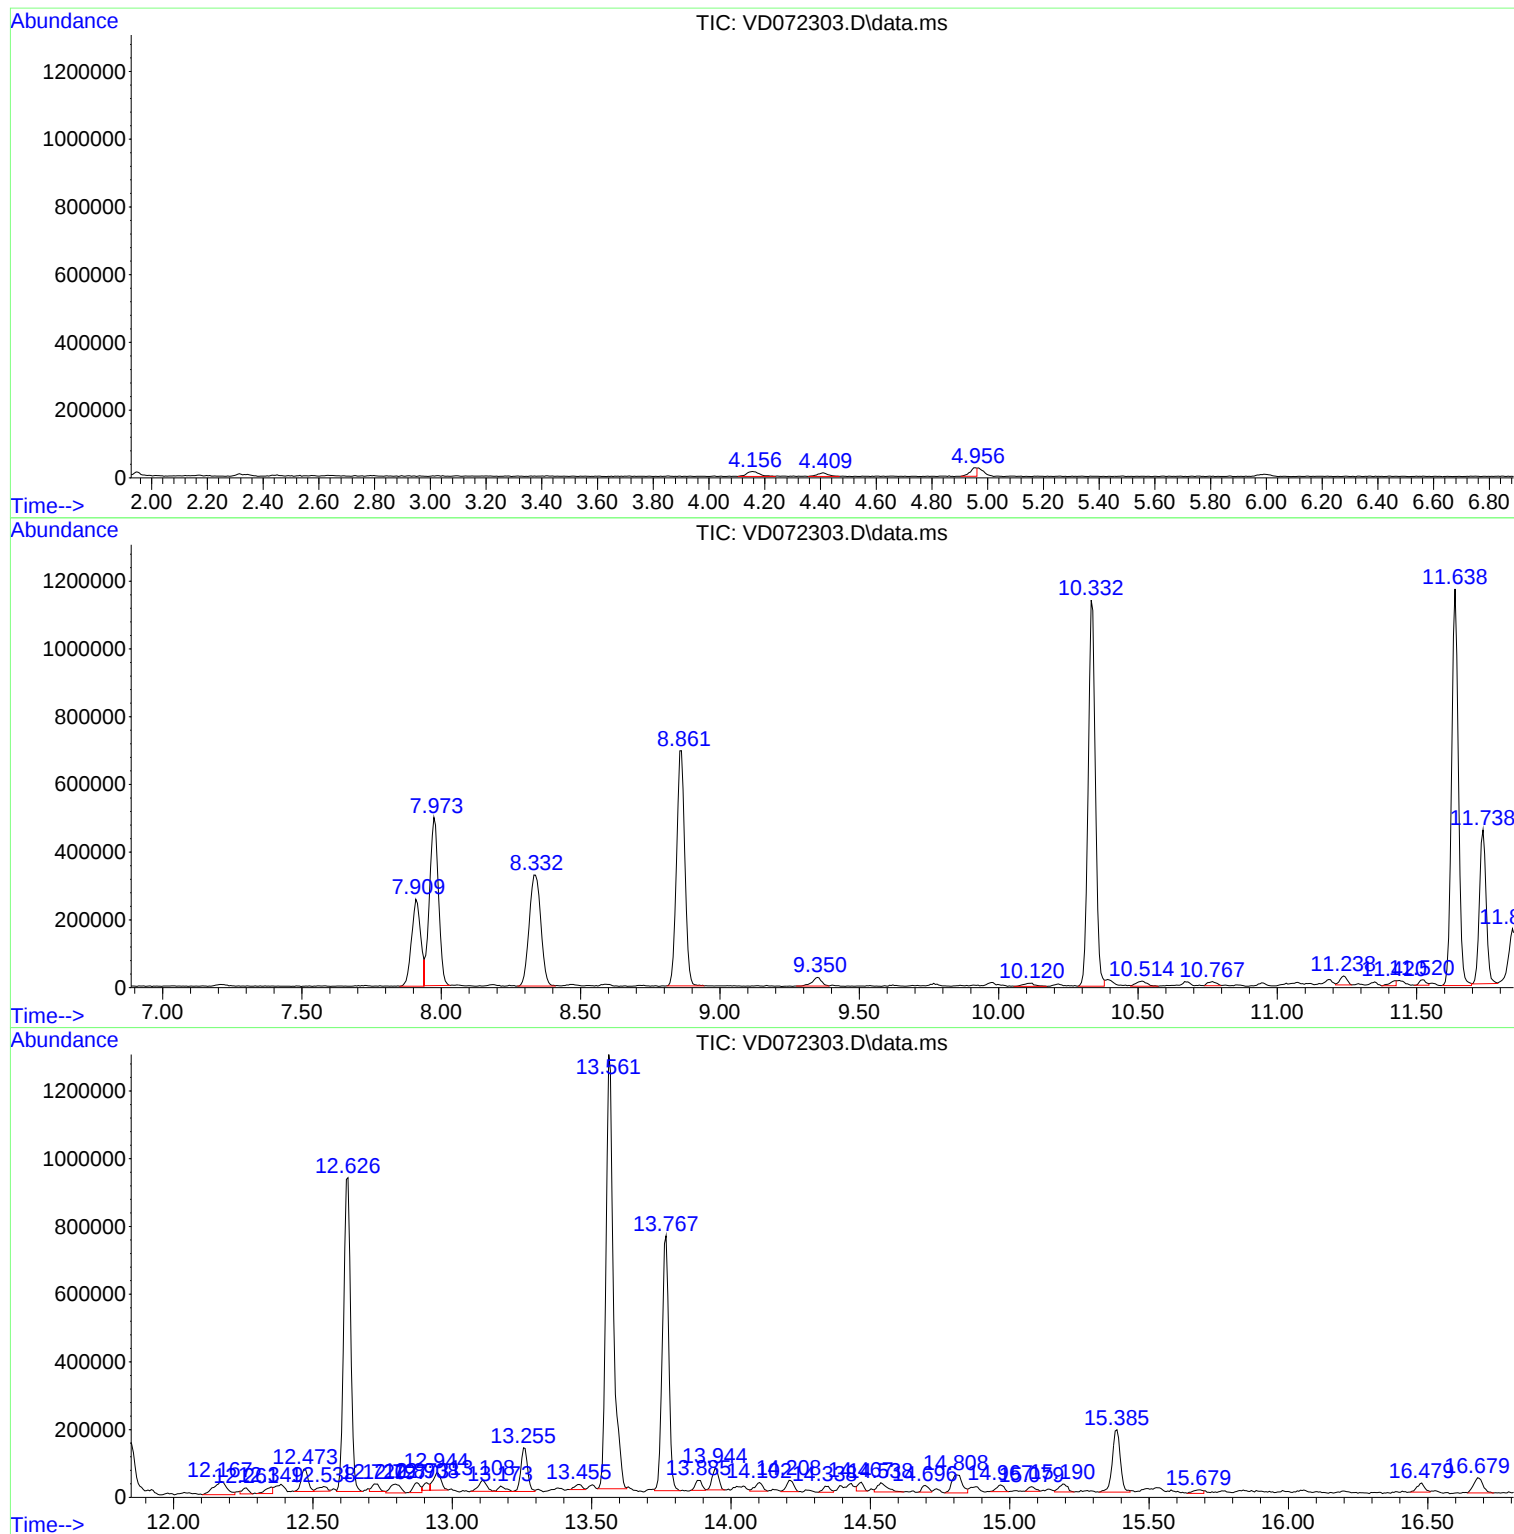

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031822\
Data File : VD072303.D
Acq On : 18 Mar 2022 21:31
Operator : VA/SY
Sample : N1962-09
Misc : 5.10G/5.00ml/MSVOA_D/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C-22-23-25










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Indane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.767	26.76 ug/l	1249340	1,4-Dichlorobenzene-d4	13.561

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Indane	118	C9H10	000496-11-7	95
2			Benzene, 1-ethenyl-4-methyl-	118	C9H10	000622-97-9	72
3			Benzene, cyclopropyl-	118	C9H10	000873-49-4	72
4			Delta-cyclene	118	C9H10	007785-10-6	72
5			Benzene, 1-ethenyl-2-methyl-	118	C9H10	000611-15-4	60

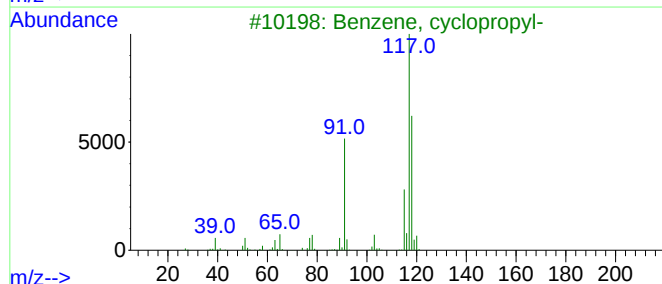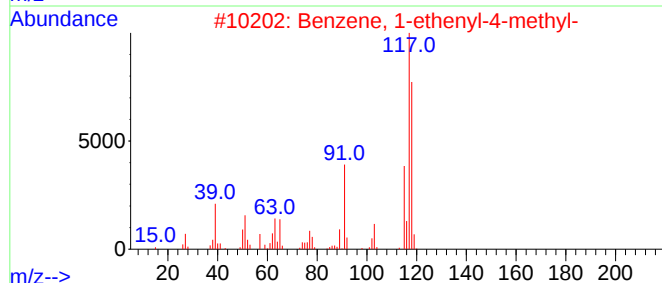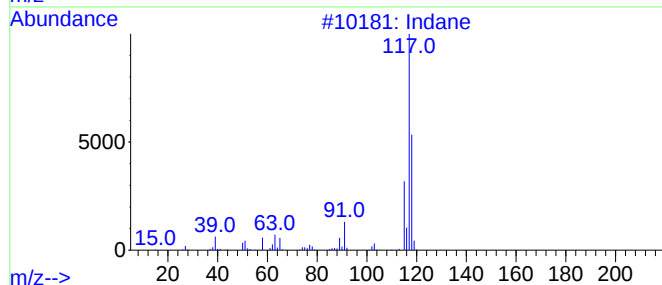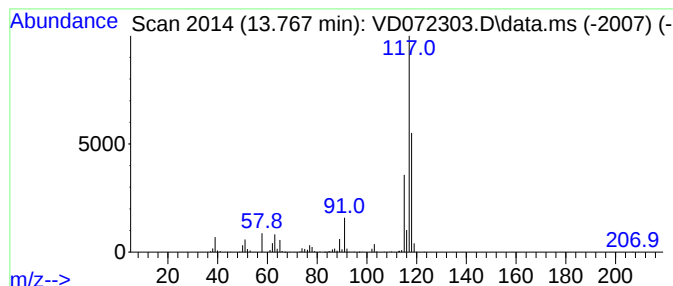

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031822\
Data File : VD072303.D
Acq On : 18 Mar 2022 21:31
Operator : VA/SY
Sample : N1962-09
Misc : 5.10G/5.00ml/MSVOA_D/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C-22-23-25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	13.767	26.8	ug/l	1249340	4	13.561	2334130	50.0