
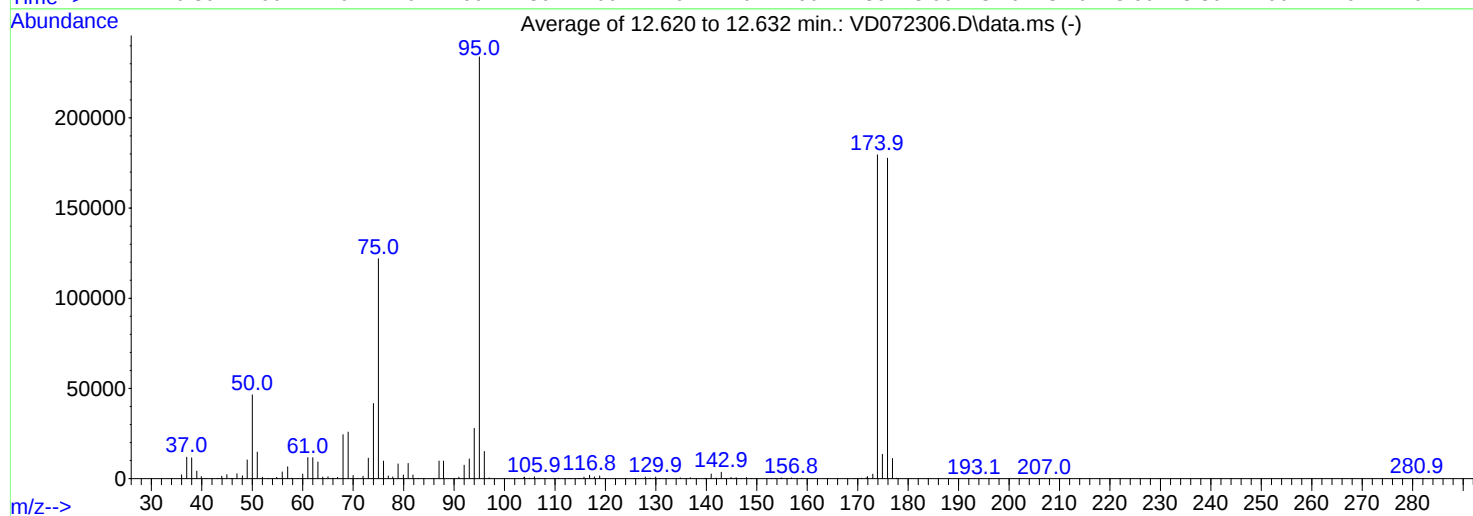


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031822\
 Data File : VD072306.D
 Acq On : 18 Mar 2022 23:24
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031122S.M
 Title : SW846 8260
 Last Update : Mon Mar 14 05:18:06 2022

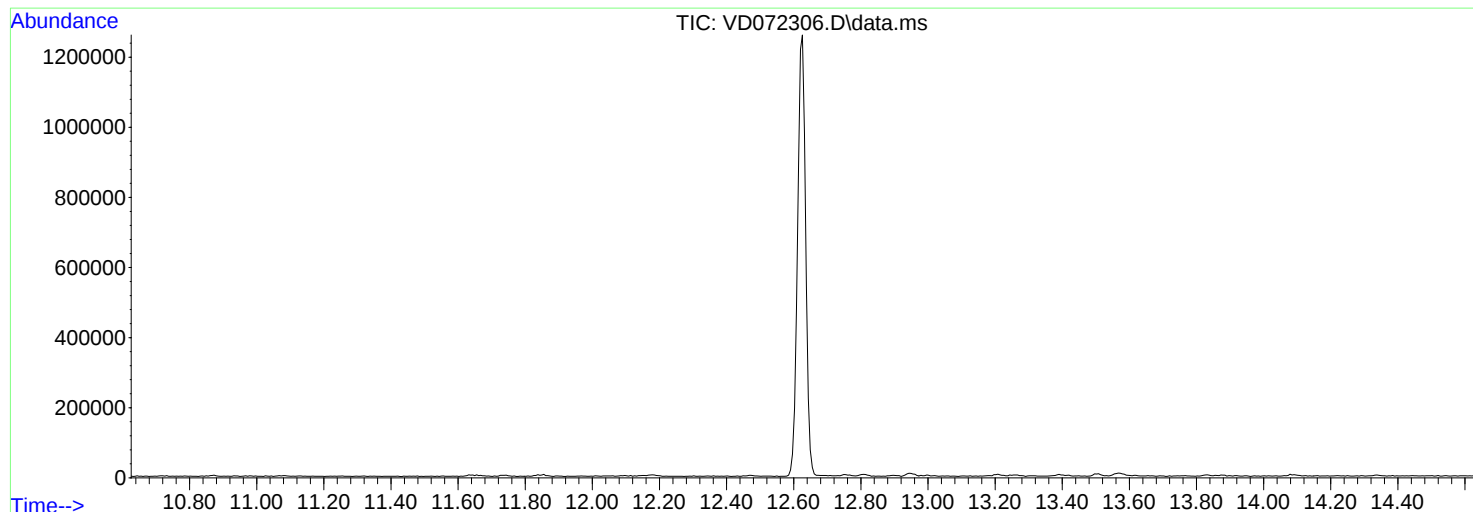

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	46507	PASS
75	95	30	60	52.2	121971	PASS
95	95	100	100	100.0	233856	PASS
96	95	5	9	6.4	15046	PASS
173	174	0.00	2	1.4	2453	PASS
174	95	50	100	76.8	179563	PASS
175	174	5	9	7.5	13484	PASS
176	174	95	101	98.9	177664	PASS
177	176	5	9	6.3	11157	PASS