


## Methyl Iodide

Response Ratio

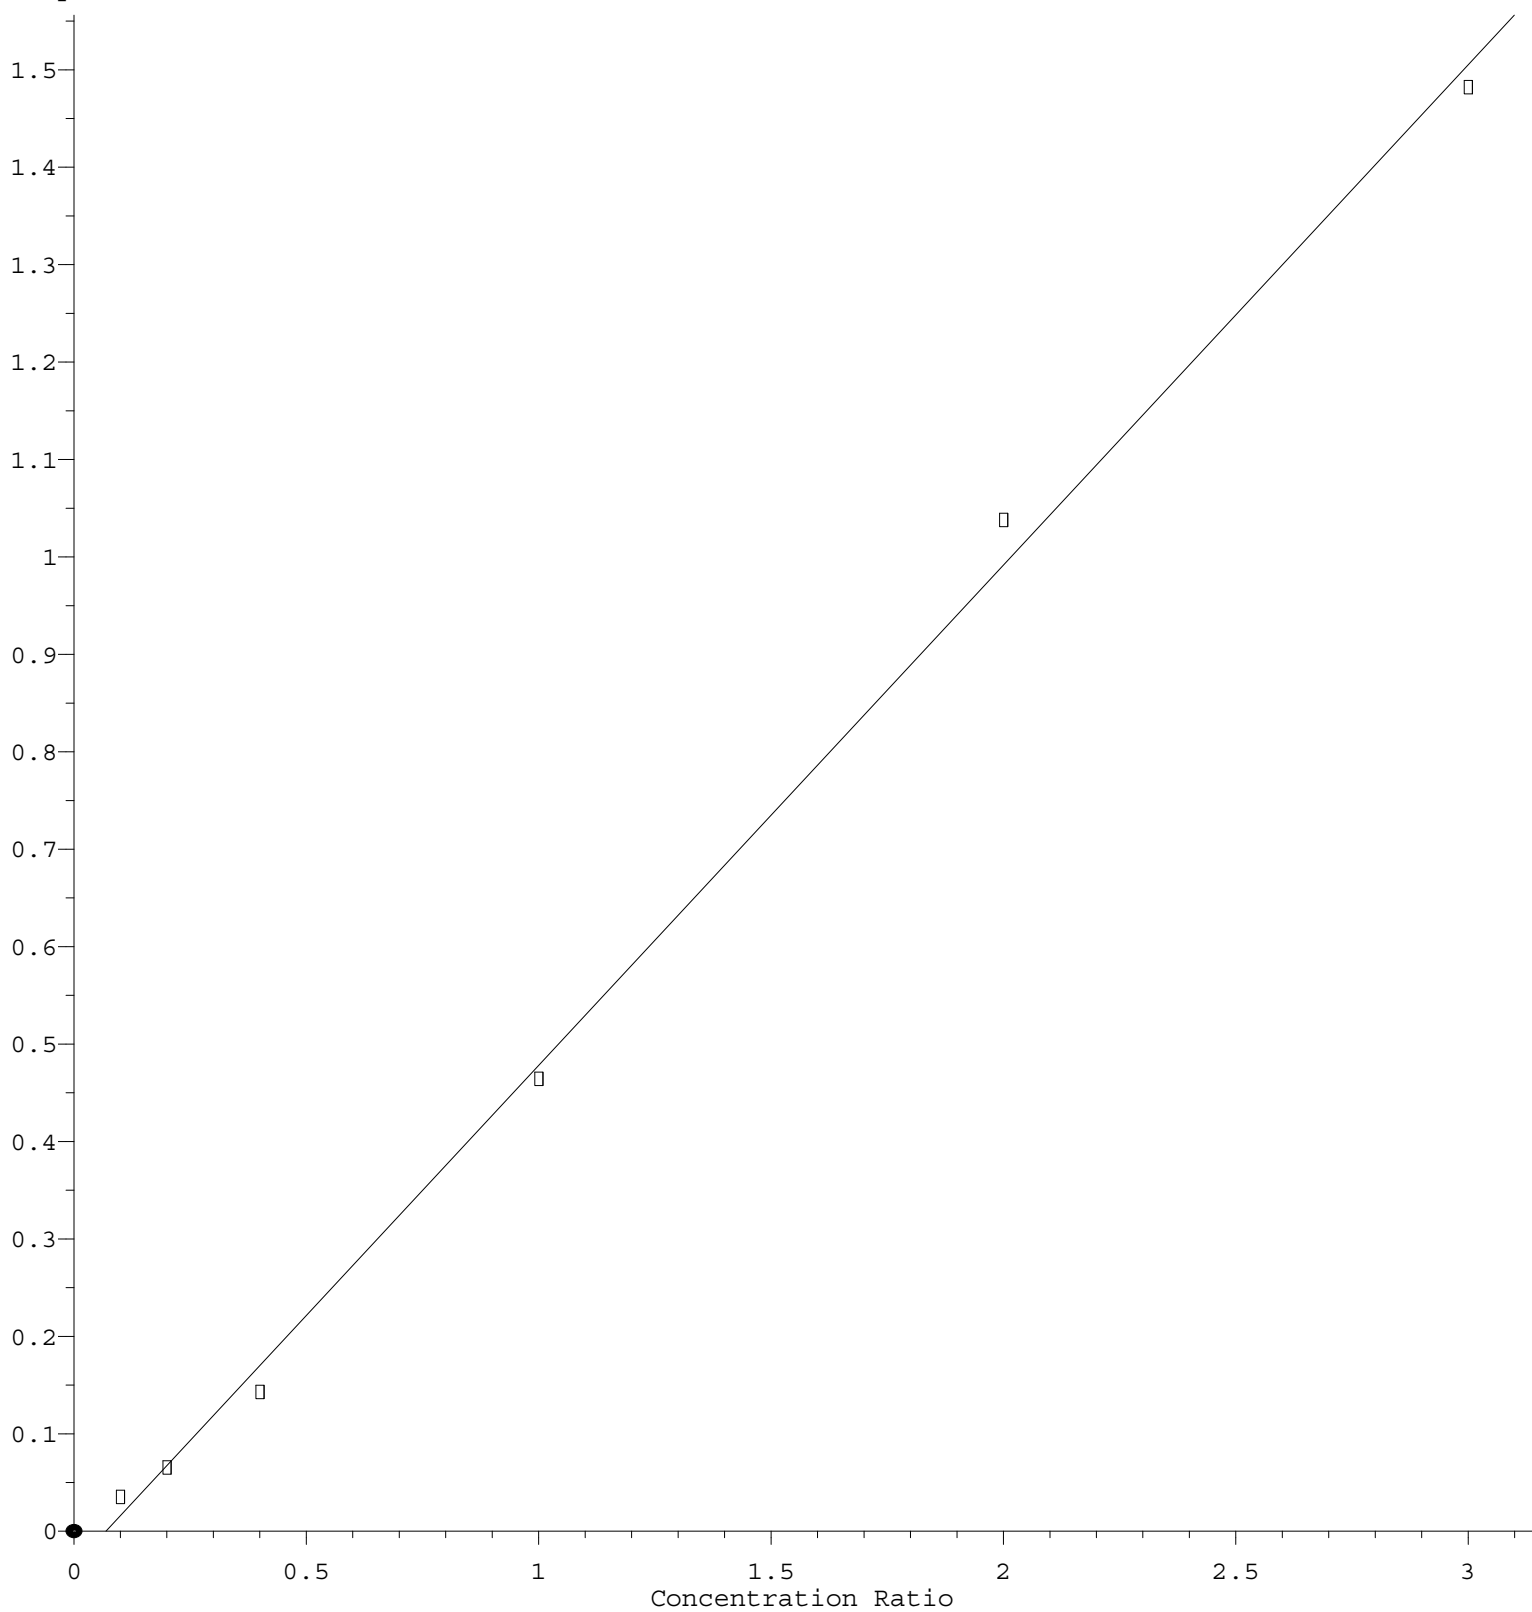


$$\text{Response} = 5.136\text{e-}001 * \text{Amt} - 3.561\text{e-}002$$

Coef of Det ( $r^2$ ) = 0.997762 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D031921S.M

Calibration Table Last Updated: Sat Mar 20 02:00:55 2021


# Acrolein

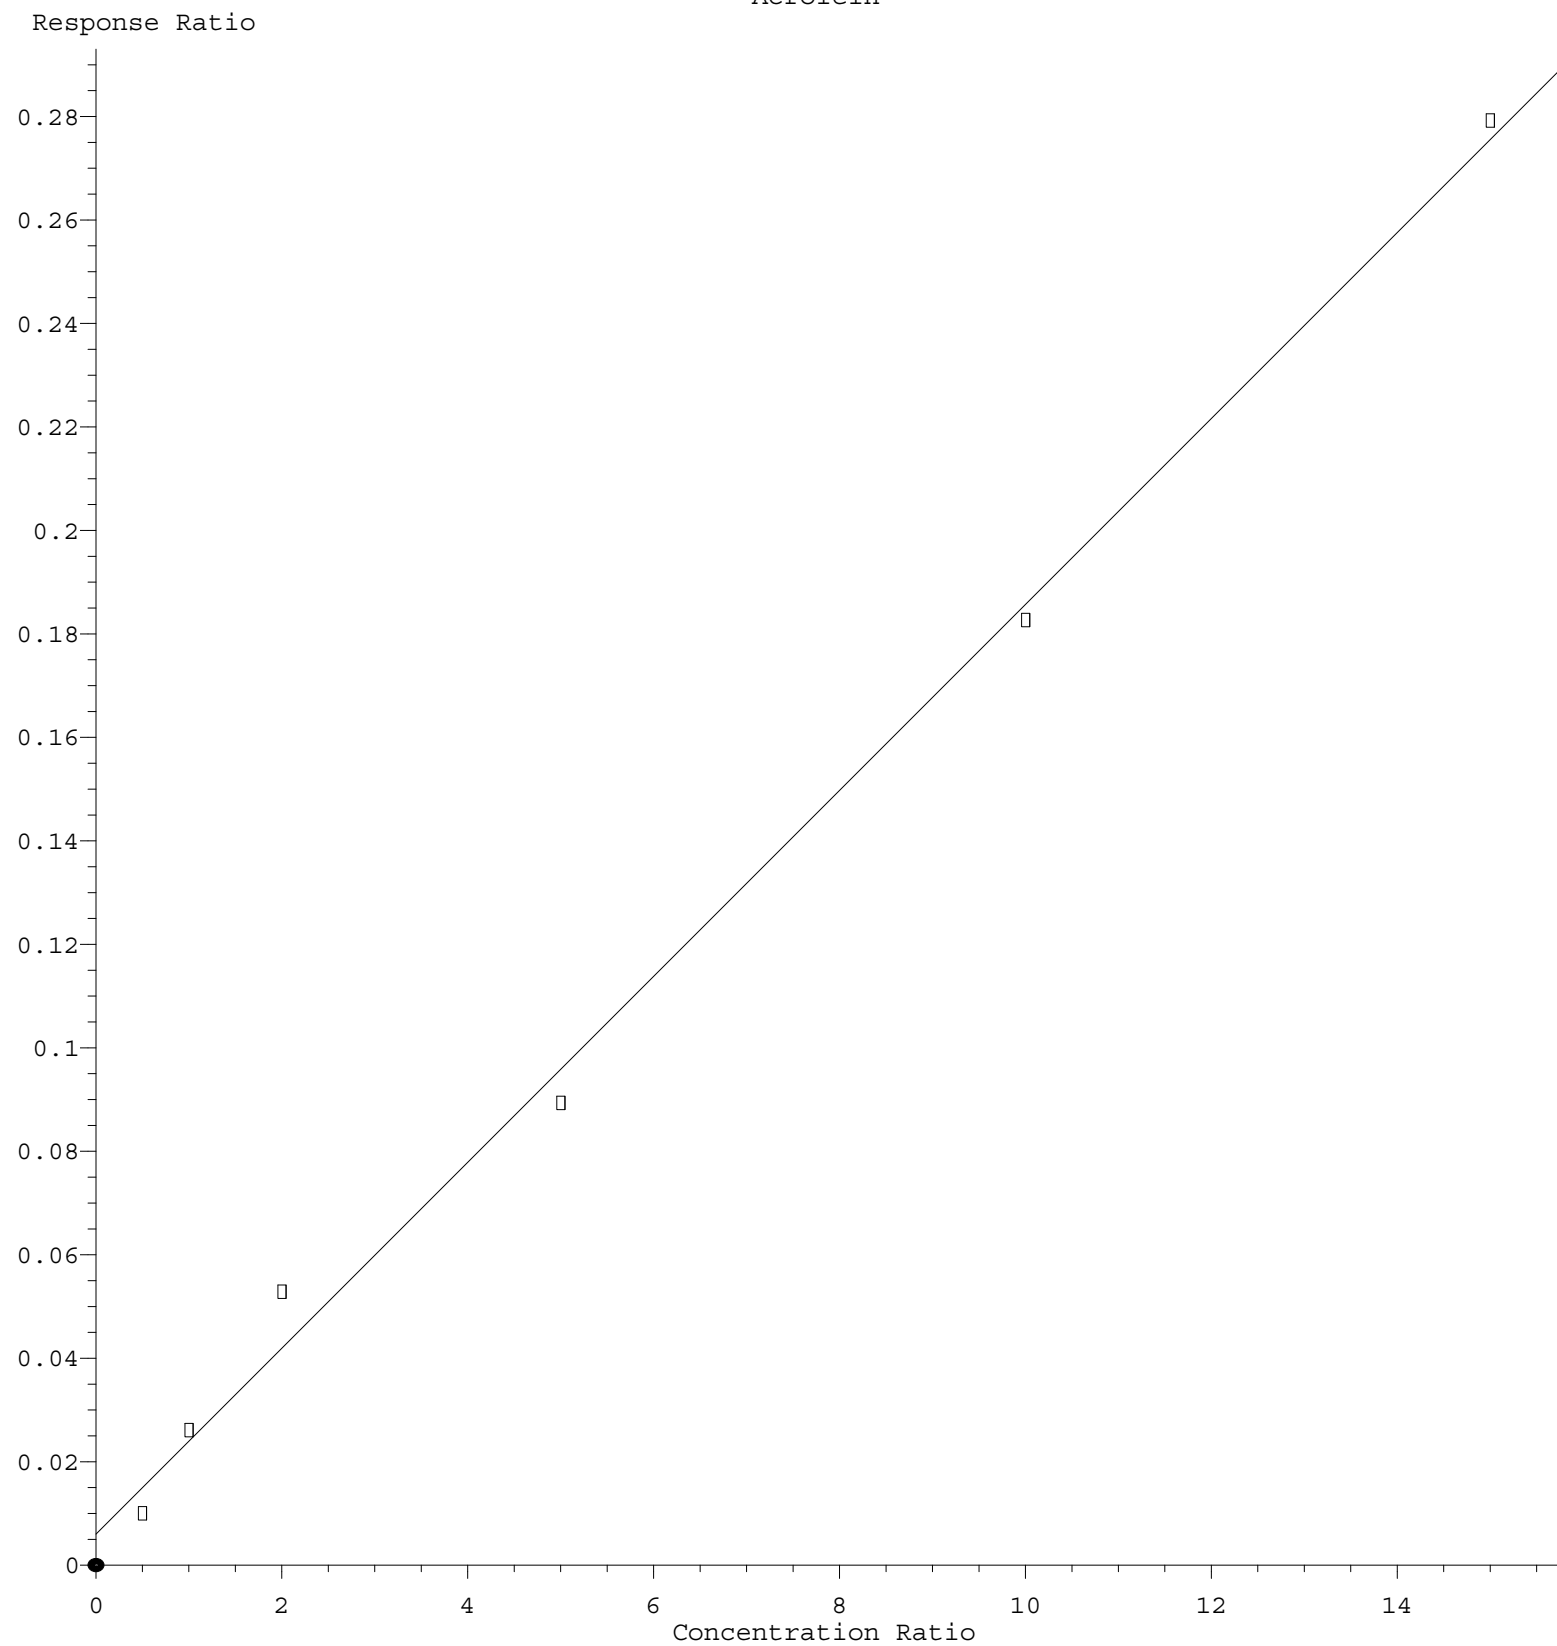

$\text{Response} = 1.798\text{e-}002 * \text{Amt} + 6.323\text{e-}003$   
 Coef of Det ( $r^2$ ) = 0.996108    Curve Fit: Linear  
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D031921S.M  
 Calibration Table Last Updated: Sat Mar 20 02:00:55 2021

## Methylene Chloride

Response Ratio

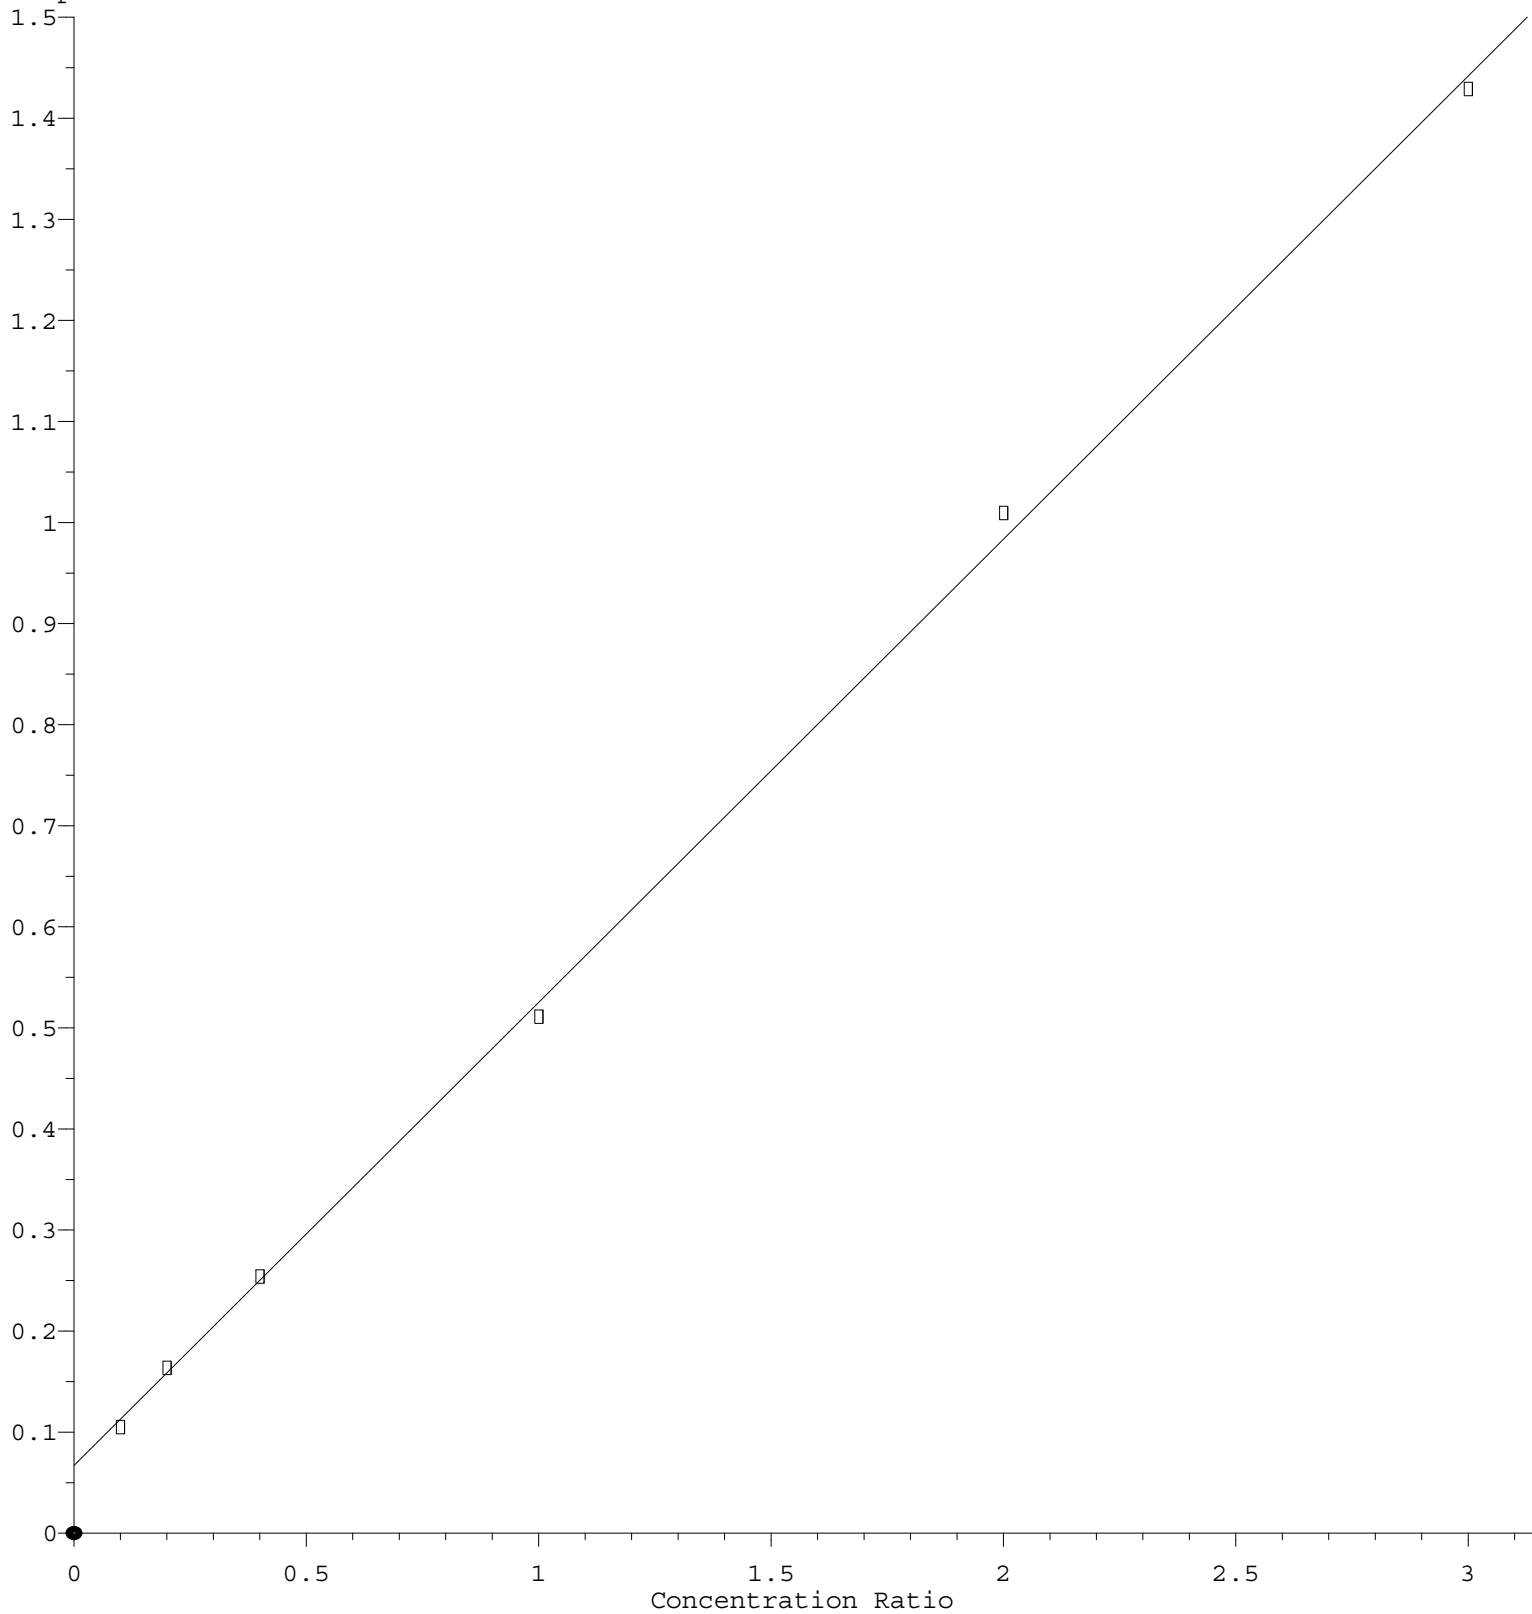

$$\text{Response} = 4.584\text{e-}001 * \text{Amt} + 6.669\text{e-}002$$

Coef of Det ( $r^2$ ) = 0.999195 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D031921S.M

Calibration Table Last Updated: Sat Mar 20 02:00:55 2021