
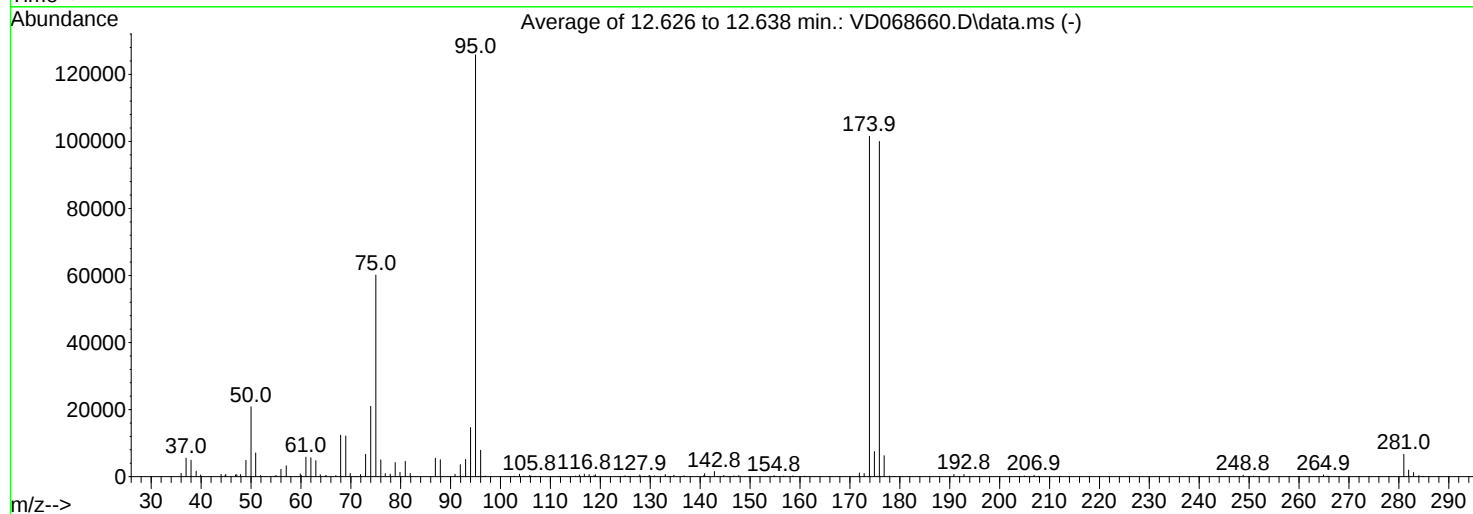


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD031921\
Data File : VD068660.D
Acq On : 19 Mar 2021 12:05
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031921S.M
Title : SW846 8260
Last Update : Sat Mar 20 02:00:55 2021

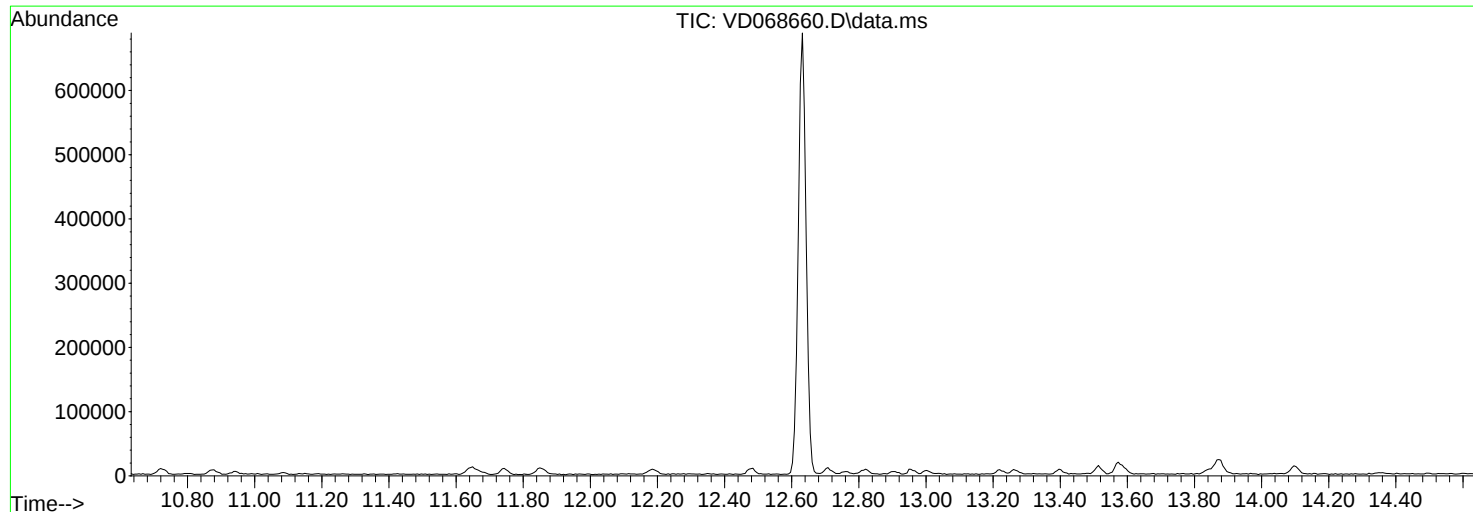

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	20845	PASS
75	95	30	60	47.8	60149	PASS
95	95	100	100	100.0	125816	PASS
96	95	5	9	6.3	7869	PASS
173	174	0.00	2	1.0	980	PASS
174	95	50	100	80.7	101515	PASS
175	174	5	9	7.4	7490	PASS
176	174	95	101	98.5	99987	PASS
177	176	5	9	6.3	6256	PASS