
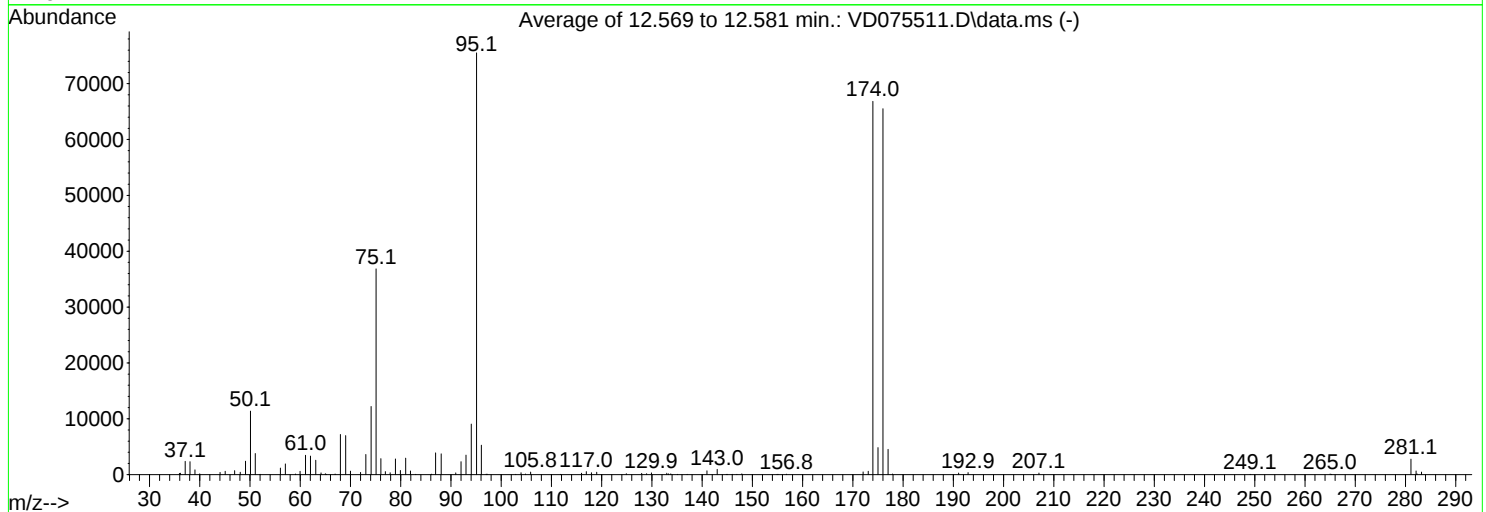


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032023\
Data File : VD075511.D
Acq On : 20 Mar 2023 09:12
Operator : KP/SY
Sample : BFB106
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB106

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Title : SFAM01.0
Last Update : Tue Mar 21 06:31:16 2023

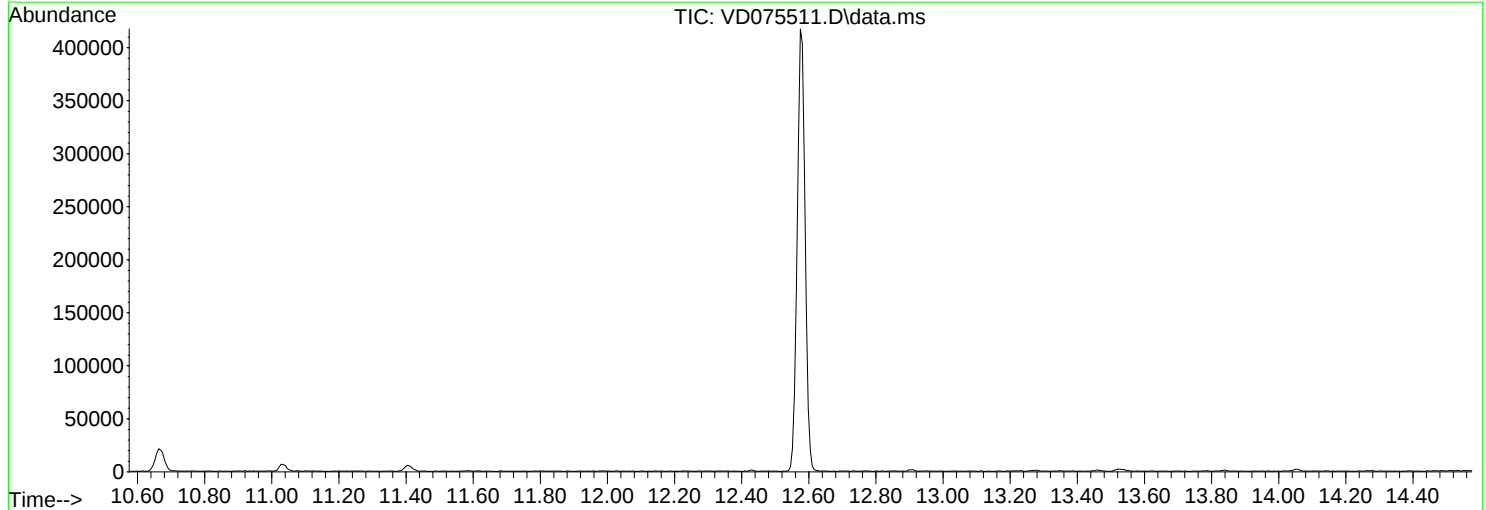

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	11383	PASS
75	95	30	80	48.8	36835	PASS
95	95	100	100	100.0	75517	PASS
96	95	5	9	7.0	5267	PASS
173	174	0.00	2	0.9	608	PASS
174	95	50	120	88.5	66837	PASS
175	174	5	9	7.3	4858	PASS
176	174	95	105	98.0	65501	PASS
177	176	5	10	6.9	4535	PASS

m/z	Abundance
40.00	430.0
44.00	158.0

Instrument :
MSVOA_D
ClientSampleId :
BFB106

m/z	Abundance
36.00	333.0
37.10	2115.0
38.10	2186.0
39.10	900.0
40.10	661.0
44.10	548.0
45.10	460.0
46.90	603.0
48.00	378.0
49.10	2124.0
50.10	10370.0
51.10	2978.0
56.00	1079.0
57.10	1513.0
60.00	515.0
61.10	3185.0
62.10	2478.0
63.10	2525.0
64.10	261.0
65.00	262.0
66.90	170.0
68.00	6279.0
69.10	6133.0
70.10	593.0
71.90	370.0
73.10	2823.0
74.10	9973.0
75.10	32232.0
76.10	2725.0
76.90	496.0
77.90	265.0
79.00	2339.0
79.90	766.0
81.00	2483.0
81.90	581.0
87.00	3129.0
88.10	2982.0
90.90	343.0
92.00	1956.0
93.00	2789.0
94.10	7459.0
95.10	62696.0
96.00	4784.0
97.00	264.0
104.00	328.0
105.90	471.0
111.80	157.0
115.90	261.0
116.90	314.0
117.90	243.0
119.00	325.0
127.90	305.0
129.90	252.0
133.00	360.0
141.00	655.0
143.00	798.0
144.80	210.0
172.00	530.0
173.00	470.0
174.00	52880.0
175.00	4112.0
176.00	52440.0
177.00	3570.0
191.00	250.0
193.00	311.0
207.00	177.0
281.10	1665.0
282.10	431.0
283.20	188.0

Instrument :
MSVOA_D
ClientSampleId :
BFB106

m/z	Abundance
35.90	322.0
36.20	371.0
37.10	2479.0
38.10	2549.0
39.00	849.0
40.00	487.0
44.10	419.0
45.10	585.0
46.90	794.0
48.00	531.0
49.10	3010.0
50.10	12268.0
51.10	4399.0
52.00	223.0
56.10	1334.0
57.00	2103.0
59.00	184.0
59.90	735.0
61.10	3906.0
62.00	3822.0
63.10	2578.0
64.10	401.0
65.00	239.0
67.00	155.0
68.00	7881.0
69.00	7688.0
70.00	662.0
72.00	415.0
73.00	3933.0
74.10	13446.0
75.10	40568.0
76.10	3453.0
77.00	691.0
77.90	439.0
79.00	3314.0
80.00	816.0
81.00	3257.0
82.00	763.0
83.00	175.0
86.10	247.0
86.90	4237.0
88.00	4095.0
91.00	296.0
92.00	2776.0
93.00	3986.0
94.10	9893.0
95.10	83520.0
96.10	5913.0
97.20	248.0
103.90	309.0
104.80	207.0
105.90	431.0
116.00	355.0
117.00	717.0
117.90	471.0
119.00	367.0
124.90	265.0
127.90	178.0
128.90	235.0
129.90	375.0
132.90	402.0
133.70	160.0
135.10	188.0
140.90	633.0
143.00	1129.0
145.00	179.0
146.90	173.0
147.90	230.0
154.90	206.0
172.10	477.0
173.00	798.0
174.00	73984.0
175.00	5259.0
176.00	72168.0
177.00	4858.0
177.90	189.0
191.10	307.0
192.90	342.0
207.00	357.0
265.30	166.0
281.10	2681.0
282.00	394.0
282.30	421.0
283.20	563.0

Instrument :
MSVOA_D
ClientSampleId :
BFB106

m/z	Abundance
36.10	434.0
37.10	2531.0
38.00	2241.0
39.10	822.0
40.00	600.0
44.10	699.0
45.00	731.0
47.00	735.0
48.10	409.0
49.10	2089.0
50.10	11511.0
51.00	3990.0
56.00	1106.0
57.10	2153.0
59.10	161.0
59.90	568.0
61.00	3319.0
62.10	3656.0
63.10	2604.0
64.20	313.0
65.20	204.0
68.00	7462.0
69.10	7135.0
69.90	643.0
72.10	402.0
73.10	4113.0
74.10	13185.0
75.10	37704.0
76.00	2438.0
76.90	487.0
77.90	332.0
78.90	2804.0
80.00	648.0
81.00	3118.0
81.90	639.0
87.00	4355.0
88.00	4071.0
90.90	332.0
92.00	2207.0
93.00	3747.0
94.00	9840.0
95.10	80336.0
96.10	5104.0
102.90	210.0
103.90	421.0
104.90	151.0
105.80	477.0
116.10	197.0
117.00	566.0
118.00	346.0
119.00	613.0
124.90	228.0
128.00	231.0
129.00	280.0
129.90	293.0
133.30	465.0
133.80	246.0
137.00	155.0
140.90	790.0
143.00	904.0
146.00	214.0
147.90	243.0
155.10	205.0
156.80	228.0
172.10	484.0
173.10	557.0
174.00	73648.0
175.00	5203.0
176.00	71896.0
177.00	5177.0
177.90	170.0
191.00	353.0
193.00	438.0
207.10	350.0
249.10	179.0
265.00	331.0
281.10	3961.0
282.10	1119.0
283.20	657.0

Instrument :
MSVOA_D
ClientSampleId :
BFB106