

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032024\
 Data File : VD078712.D
 Acq On : 20 Mar 2024 10:34
 Operator : RP/MD
 Sample : VD0320SBL01
 Misc : 5.00G/5ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0320SBL01

Quant Time: Mar 21 04:44:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031424S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 15 05:38:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	104242	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	189934	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	172650	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	72173	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	55203	56.507	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	113.020%
35) Dibromofluoromethane	7.810	113	61174	50.024	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.040%
50) Toluene-d8	10.269	98	224853	49.996	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	100.000%
62) 4-Bromofluorobenzene	12.575	95	58178	44.217	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	88.440%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032024\
Data File : VD078712.D
Acq On : 20 Mar 2024 10:34
Operator : RP/MD
Sample : VD0320SBL01
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0320SBL01

Quant Time: Mar 21 04:44:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031424S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 15 05:38:03 2024
Response via : Initial Calibration




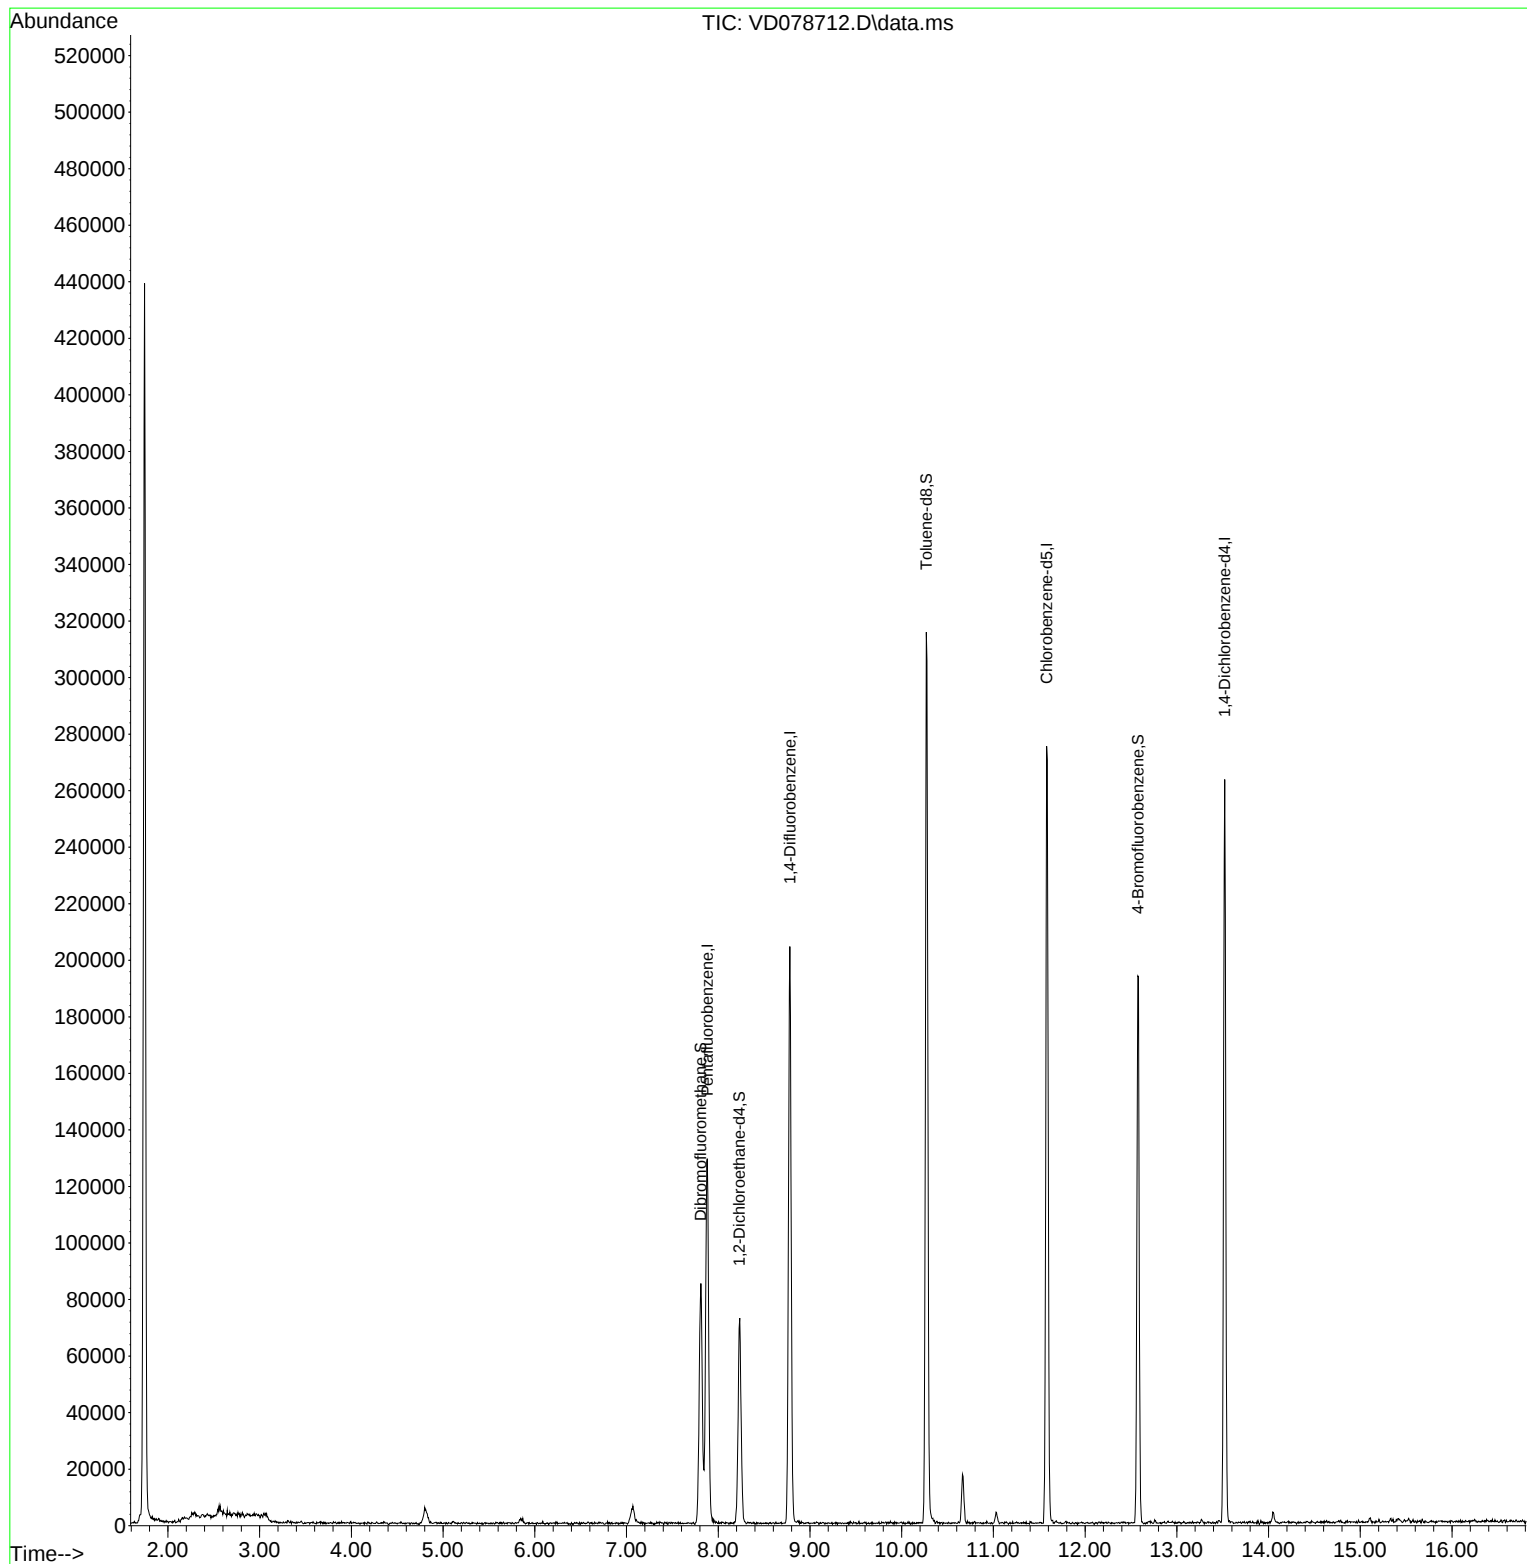


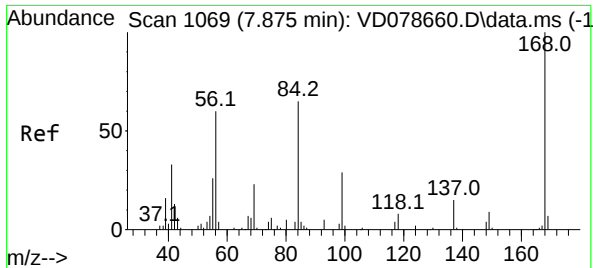

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1129
Delta R.T. 0.006 min
Lab File: VD078712.D
Acq: 20 Mar 2024 10:34




Instrument :
MSVOA_D
ClientSampleId :
VD0320SBL01


Tgt Ion:168 Resp: 104242
Ion Ratio Lower Upper
168 100
99 45.9 38.8 58.2

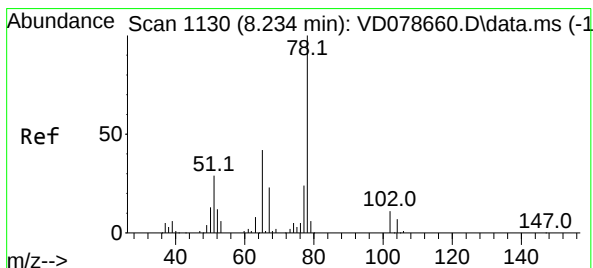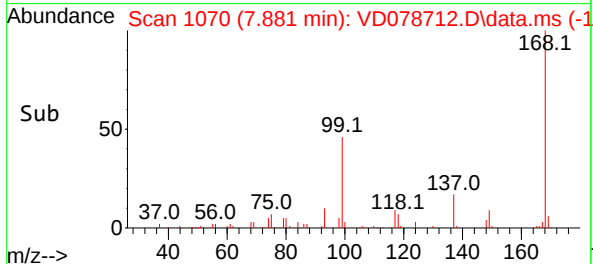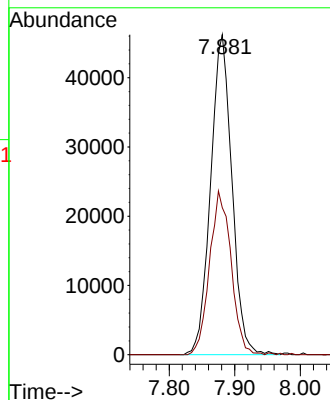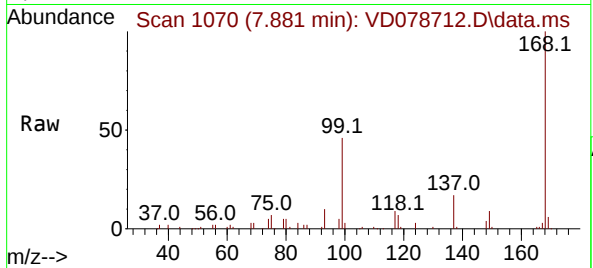

#33
1,2-Dichloroethane-d4
Concen: 56.507 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.006 min
Lab File: VD078712.D
Acq: 20 Mar 2024 10:34

Tgt Ion: 65 Resp: 55203
Ion Ratio Lower Upper
65 100
67 54.1 0.0 110.2

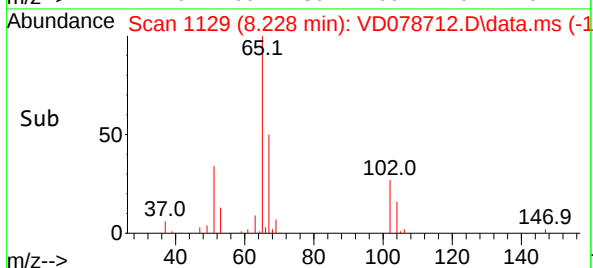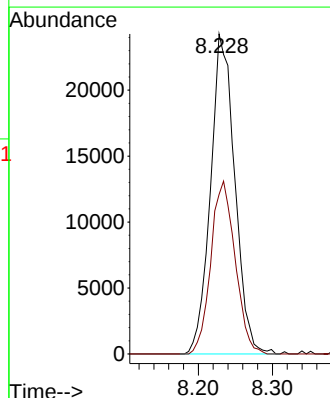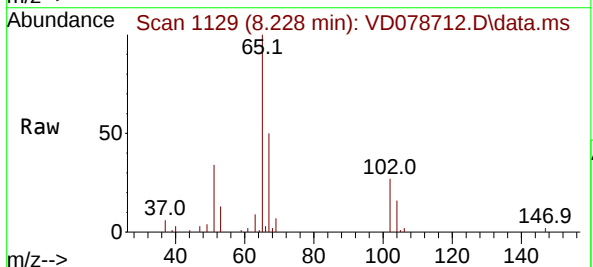

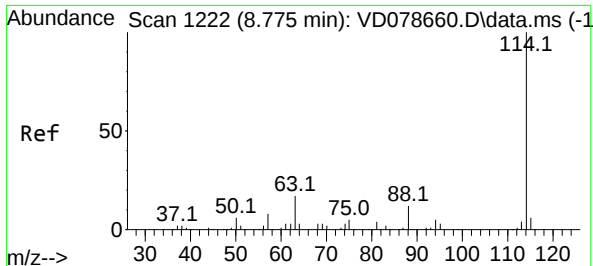

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. 0.006 min

Lab File: VD078712.D

Acq: 20 Mar 2024 10:34

Instrument :

MSVOA_D

ClientSampleId :

VD0320SBL01





Tgt Ion:114 Resp: 189934

Ion Ratio Lower Upper

114 100

63 17.8 0.0 33.4

88 13.2 0.0 24.6

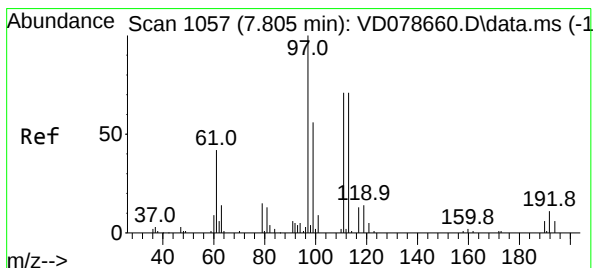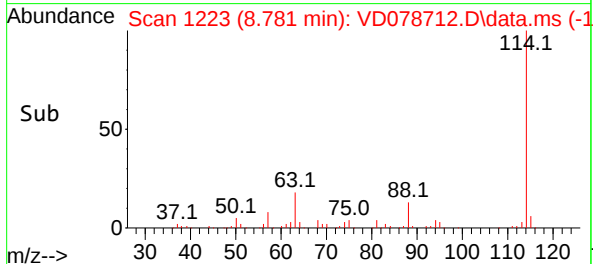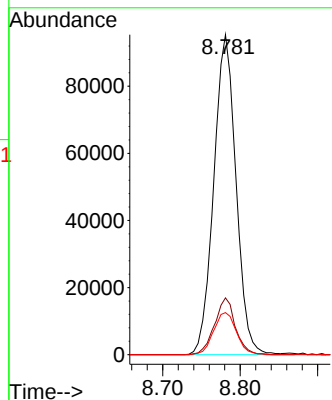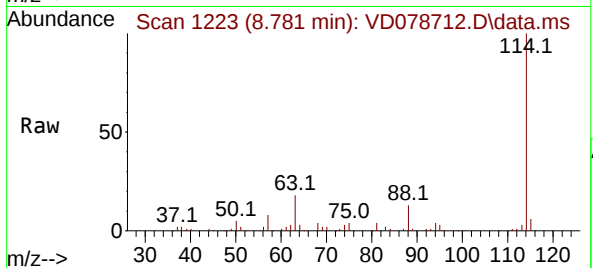

#35

Dibromofluoromethane

Concen: 50.024 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD078712.D

Acq: 20 Mar 2024 10:34




Tgt Ion:113 Resp: 61174


Ion Ratio Lower Upper

113 100

111 105.5 81.9 122.9

192 18.2 15.4 23.0

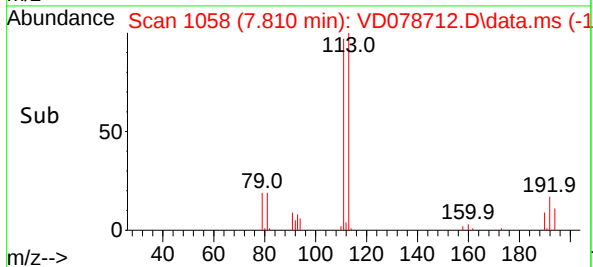
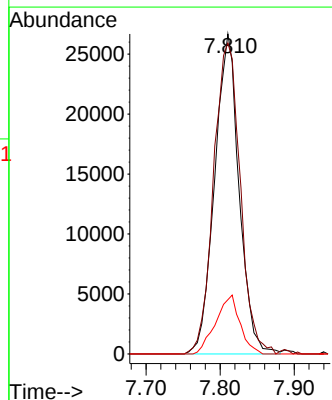
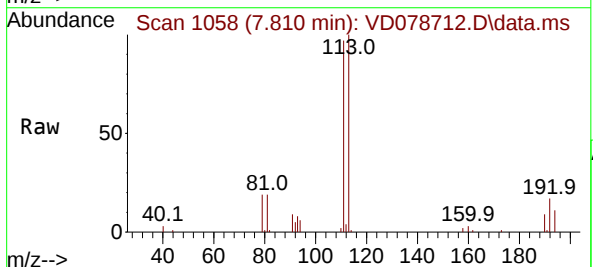


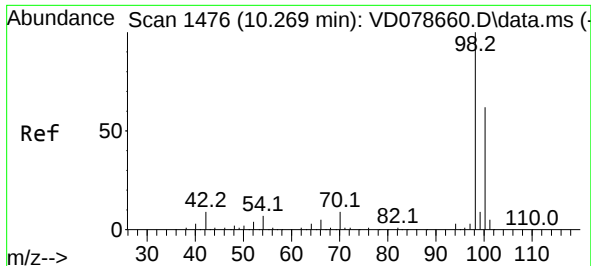

#50
Toluene-d8
Concen: 49.996 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD078712.D
Acq: 20 Mar 2024 10:34




Instrument :
MSVOA_D
ClientSampleId :
VD0320SBL01


Tgt Ion: 98 Resp: 224853
Ion Ratio Lower Upper
98 100
100 65.2 50.5 75.7

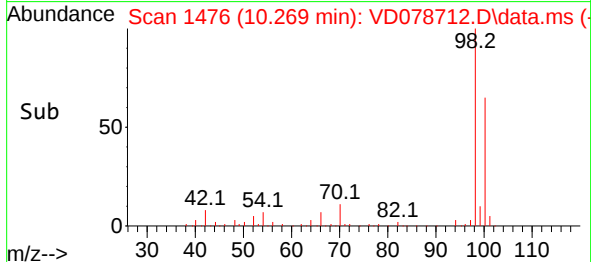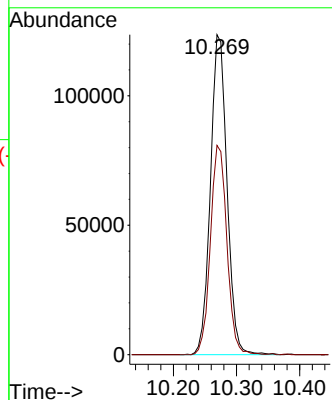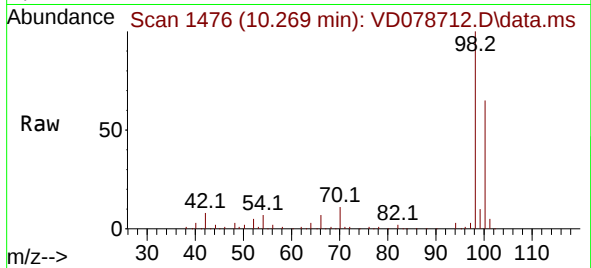

#62
4-Bromofluorobenzene
Concen: 44.217 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. 0.006 min
Lab File: VD078712.D
Acq: 20 Mar 2024 10:34

Tgt Ion: 95 Resp: 58178
Ion Ratio Lower Upper
95 100
174 93.9 0.0 195.2
176 93.0 0.0 188.2

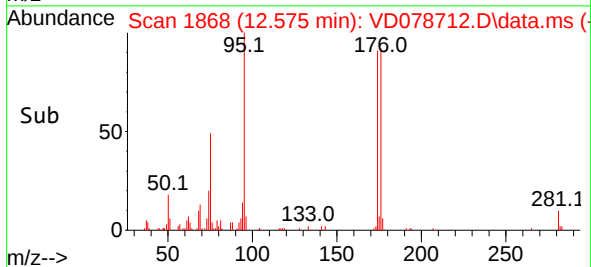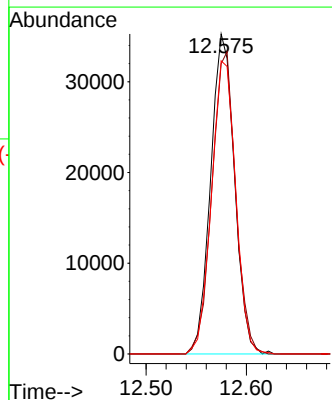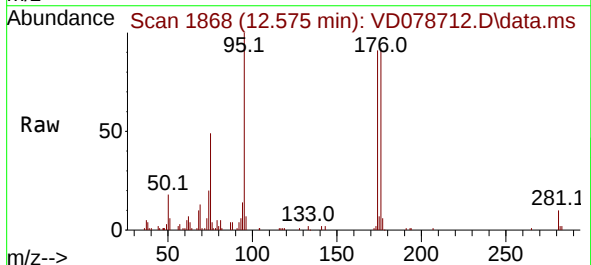

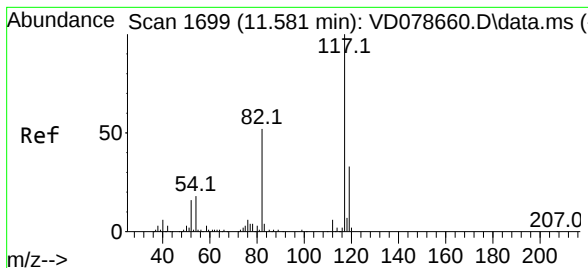

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.581 min Scan# 1

Delta R.T. 0.000 min

Lab File: VD078712.D

Acq: 20 Mar 2024 10:34

Instrument :

MSVOA_D

ClientSampleId :

VD0320SBL01





Tgt Ion:117 Resp: 172650

Ion Ratio Lower Upper

117 100

82 50.6 41.4 62.2

119 30.5 26.5 39.7

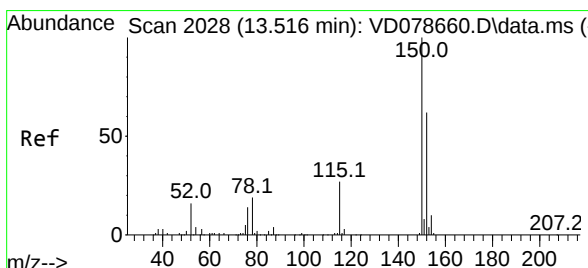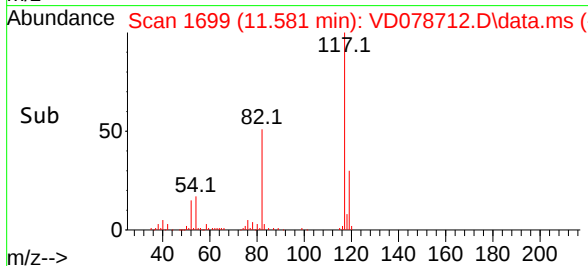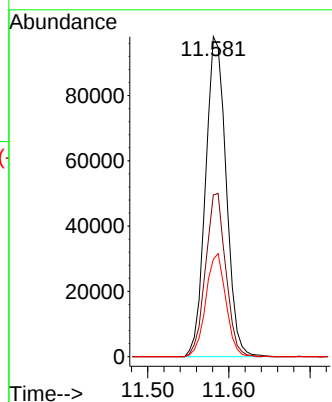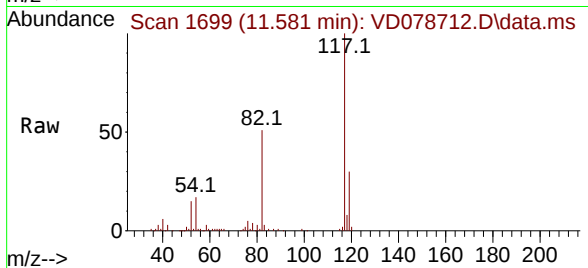

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.522 min Scan# 2029

Delta R.T. 0.006 min

Lab File: VD078712.D

Acq: 20 Mar 2024 10:34

Tgt Ion:152 Resp: 72173

Ion Ratio Lower Upper

152 100

115 54.4 27.1 81.2

150 160.1 0.0 350.2

