
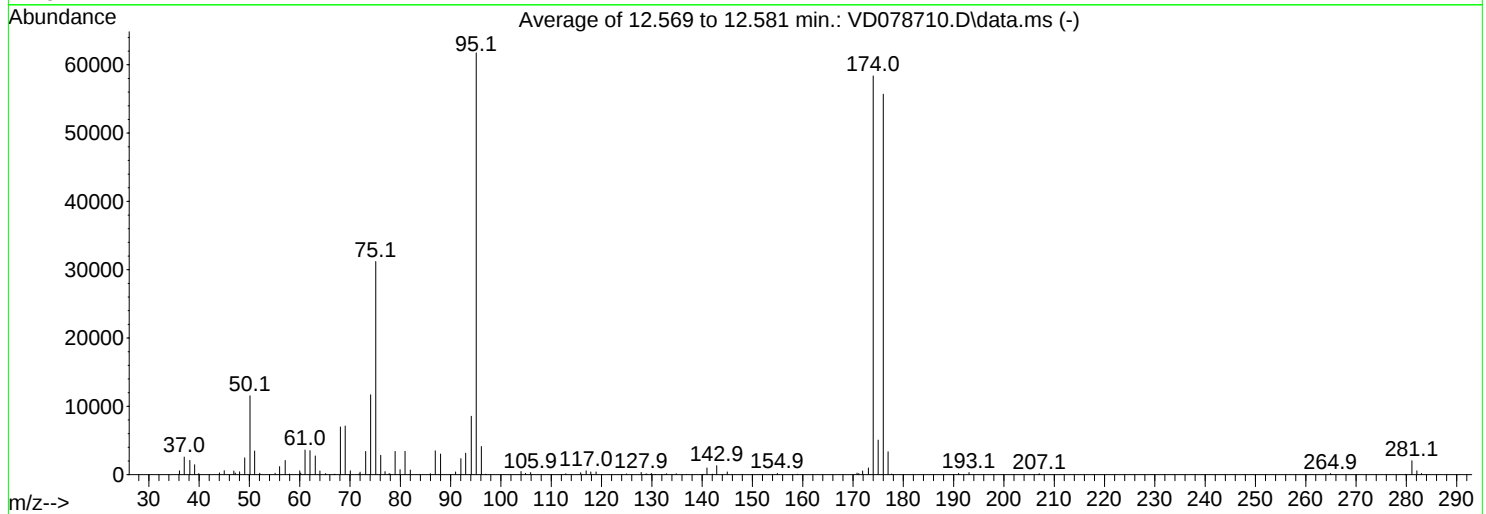


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032024\
Data File : VD078710.D
Acq On : 20 Mar 2024 09:23
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031424S.M
Title : SW846 8260
Last Update : Fri Mar 15 05:38:03 2024

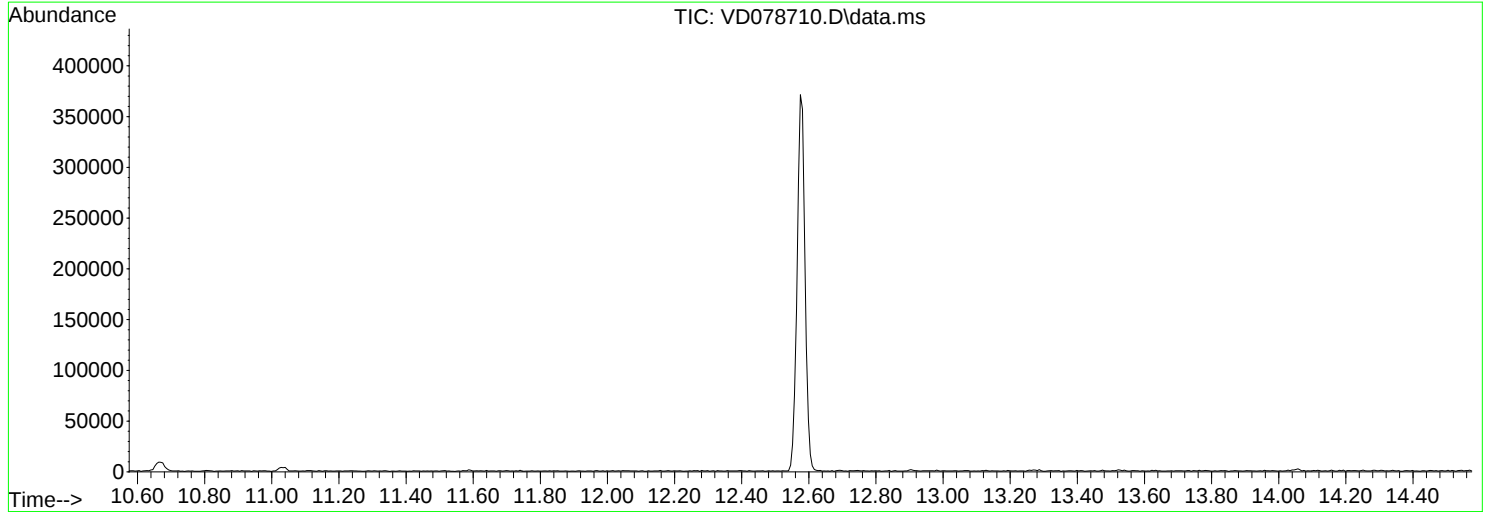

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	11551	PASS
75	95	30	60	50.5	31192	PASS
95	95	100	100	100.0	61747	PASS
96	95	5	9	6.7	4124	PASS
173	174	0.00	2	1.7	986	PASS
174	95	50	100	94.5	58381	PASS
175	174	5	9	8.7	5053	PASS
176	174	95	101	95.4	55691	PASS
177	176	5	9	6.0	3348	PASS