


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD032119\
Data File : VD061236.D
Acq On : 21 Mar 2019 10:00
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
Title : SW846 8260
Last Update : Fri Mar 08 02:35:39 2019

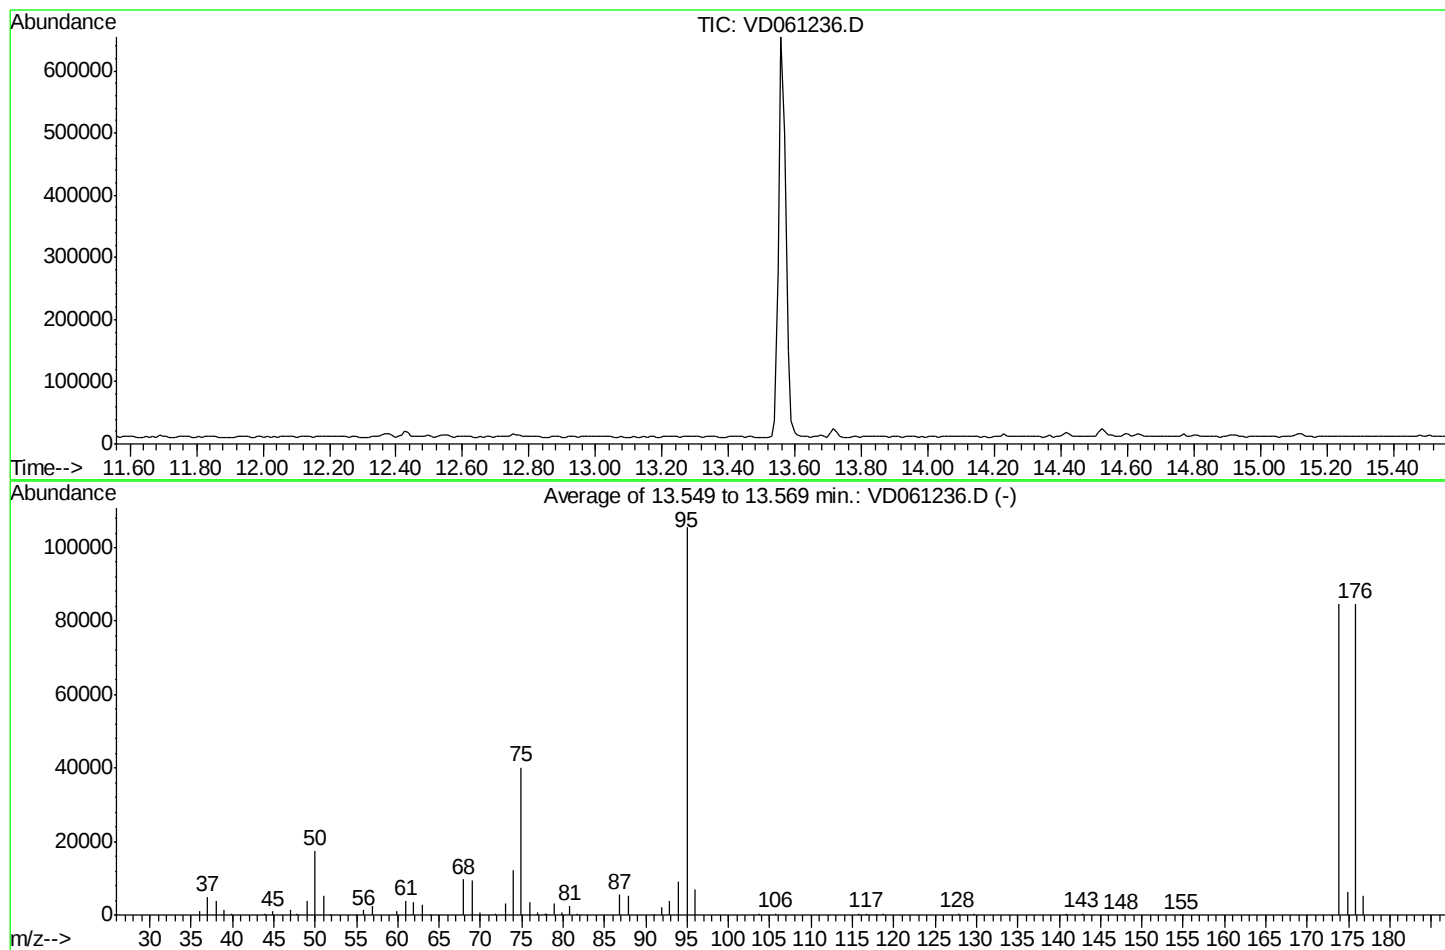

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	17468	PASS
75	95	30	60	38.0	40149	PASS
95	95	100	100	100.0	105520	PASS
96	95	5	9	6.6	6949	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.2	84653	PASS
175	174	5	9	7.6	6431	PASS
176	174	95	101	100.2	84840	PASS
177	176	5	9	6.1	5184	PASS