
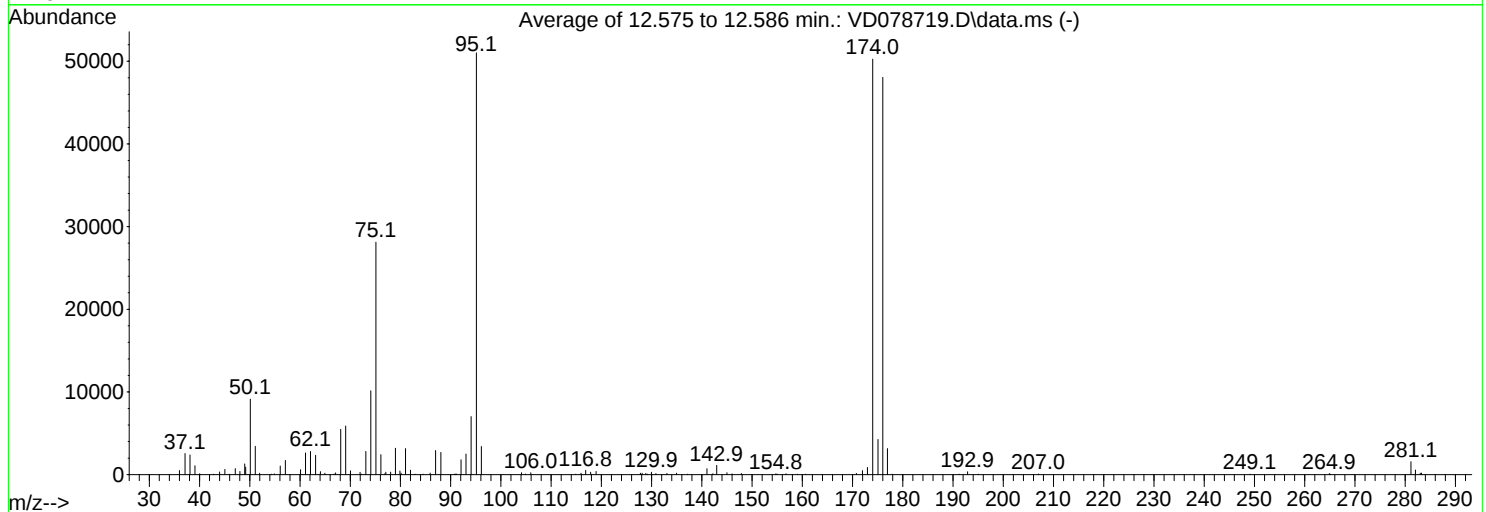


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032124\
Data File : VD078719.D
Acq On : 21 Mar 2024 08:46
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031424S.M
Title : SW846 8260
Last Update : Fri Mar 15 05:38:03 2024

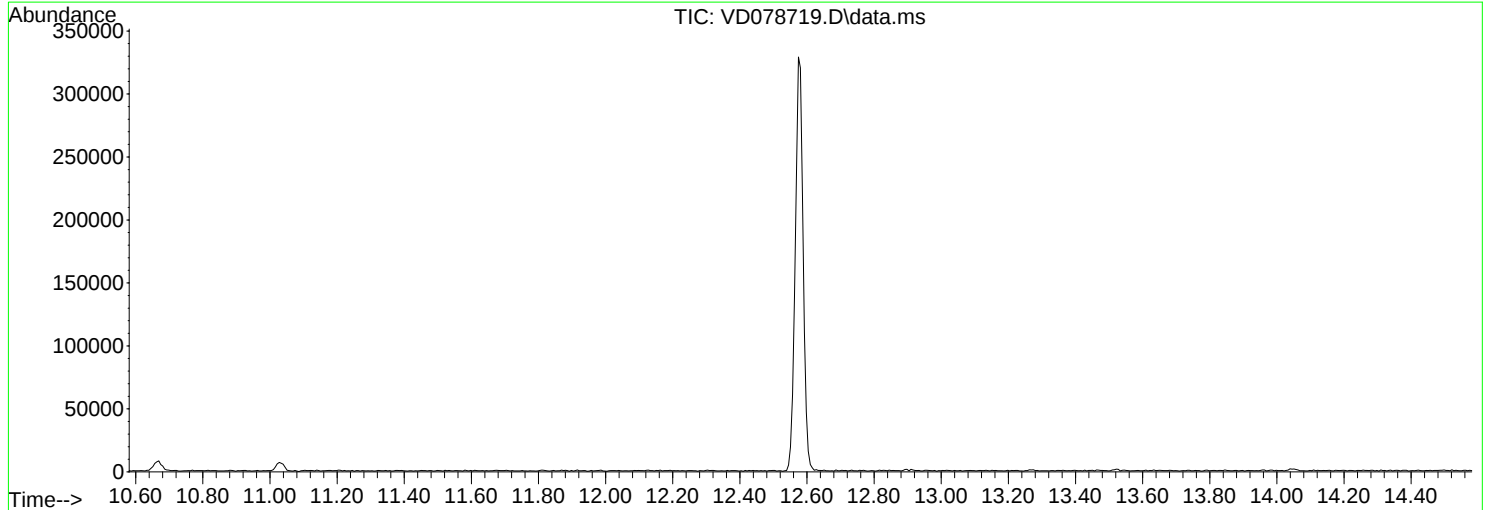

AutoFind: Scans 1868, 1869, 1870; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	9145	PASS
75	95	30	60	55.1	28115	PASS
95	95	100	100	100.0	51019	PASS
96	95	5	9	6.7	3408	PASS
173	174	0.00	2	1.7	867	PASS
174	95	50	100	98.5	50261	PASS
175	174	5	9	8.5	4265	PASS
176	174	95	101	95.6	48053	PASS
177	176	5	9	6.6	3150	PASS