


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD032219\
 Data File : VD061251.D
 Acq On : 22 Mar 2019 9:31
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
 Title : SW846 8260
 Last Update : Fri Mar 08 02:35:39 2019

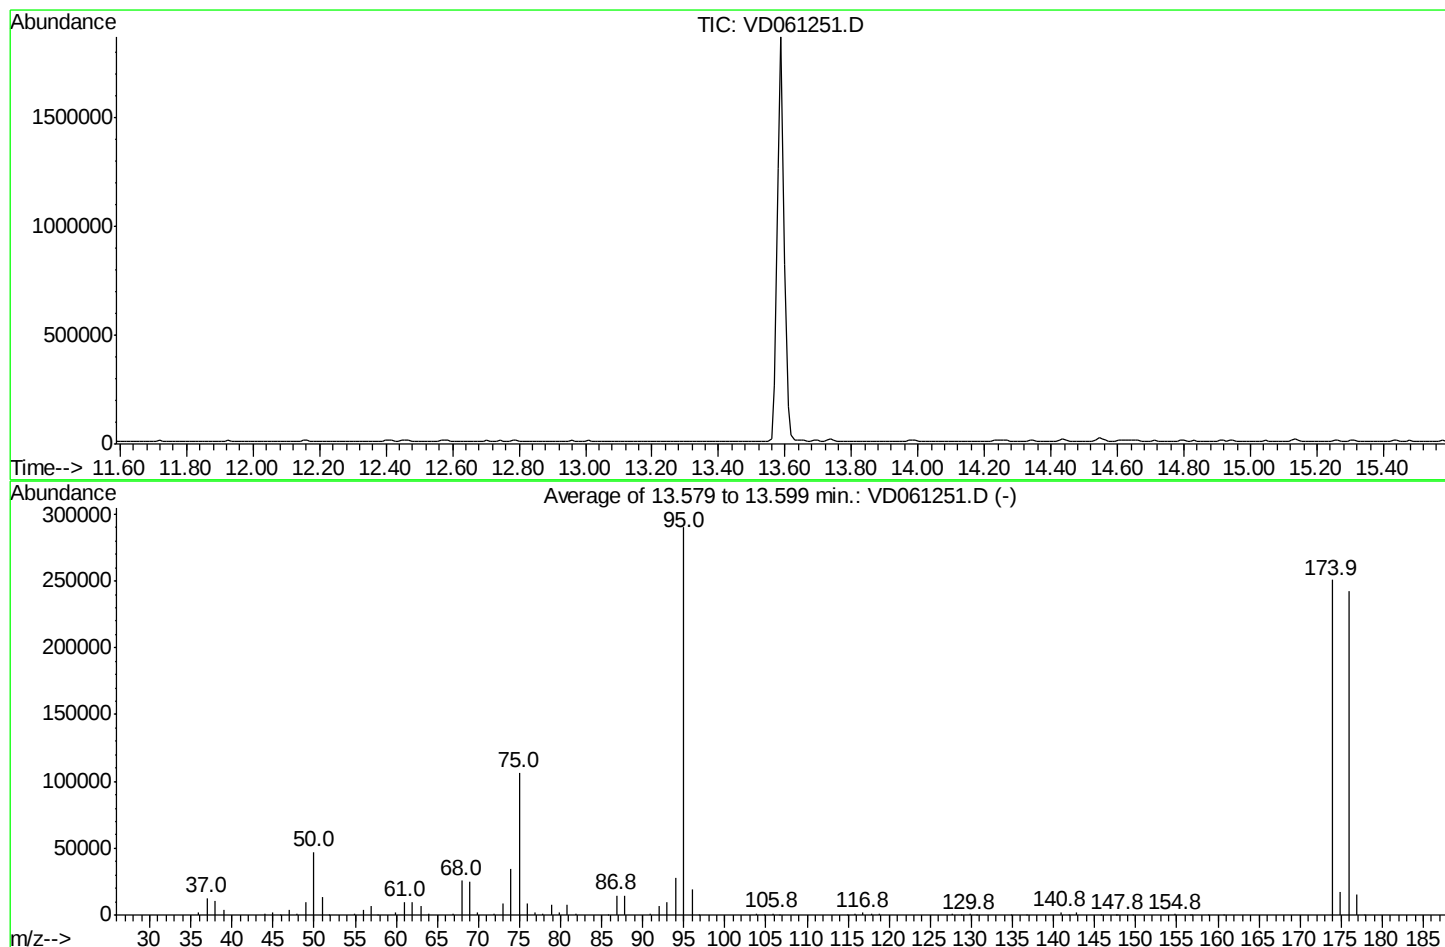

AutoFind: Scans 1235, 1236, 1237; Background Corrected with Scan 1230

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	47144	PASS
75	95	30	60	36.8	106829	PASS
95	95	100	100	100.0	290176	PASS
96	95	5	9	6.5	18948	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.4	250645	PASS
175	174	5	9	6.8	17142	PASS
176	174	95	101	96.7	242282	PASS
177	176	5	9	6.4	15461	PASS